
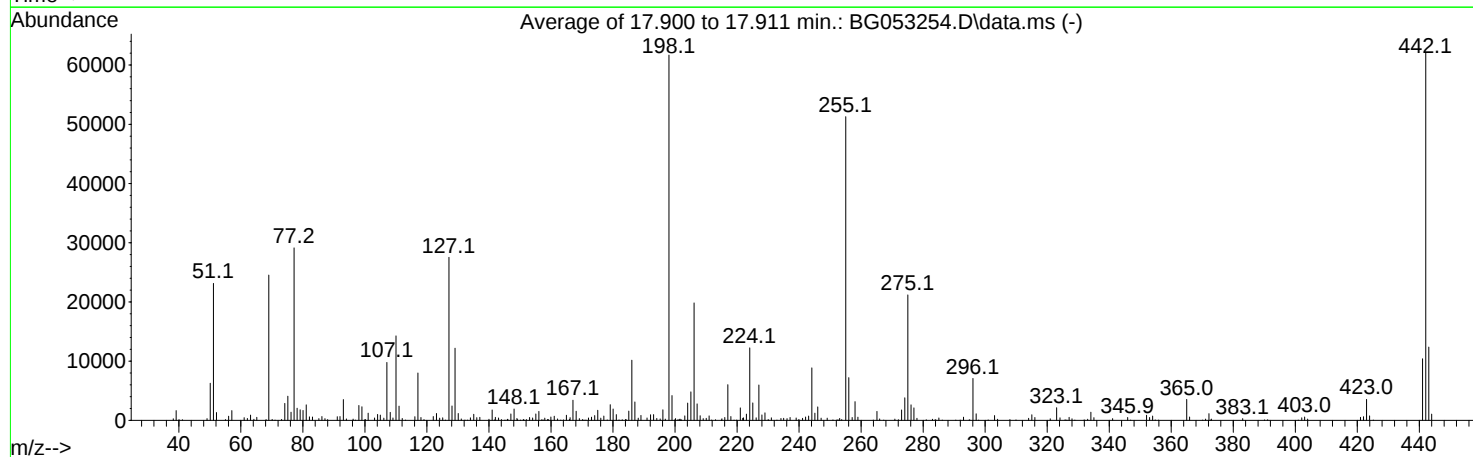


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
 Data File : BG053254.D
 Acq On : 22 Apr 2022 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 01:13:30 2022

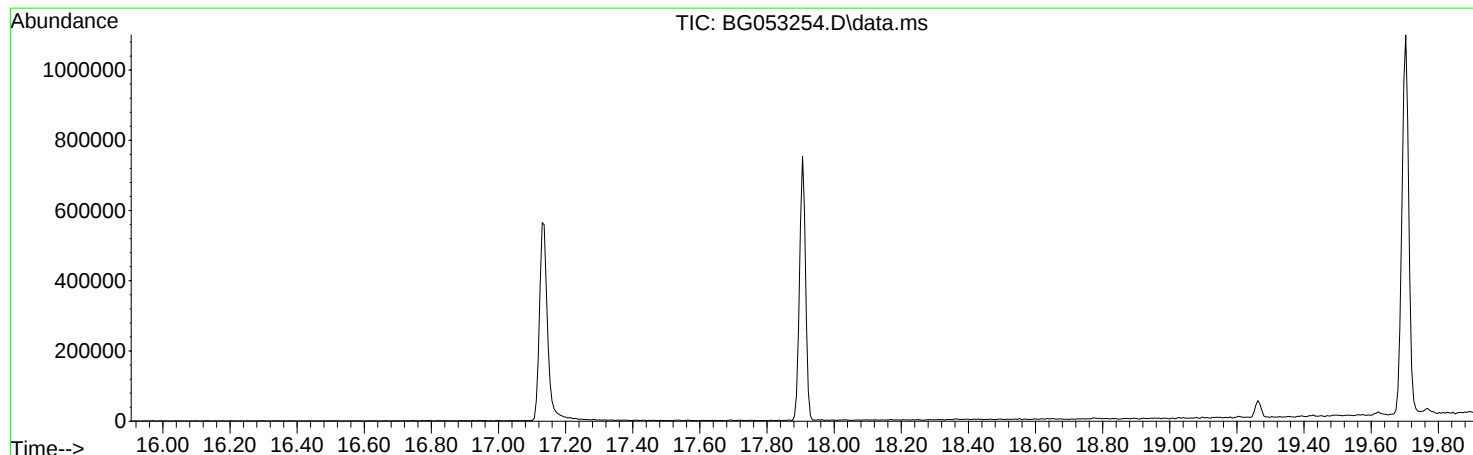

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	23141	PASS
68	69	0.00	2	0.6	149	PASS
69	198	0.00	100	39.8	24525	PASS
70	69	0.00	2	0.7	164	PASS
127	198	10	80	44.6	27528	PASS
197	198	0.00	2	0.4	224	PASS
198	198	100	100	100.0	61675	PASS
199	198	5	9	6.8	4181	PASS
275	198	10	60	34.3	21173	PASS
365	198	1	100	5.7	3528	PASS
441	198	0.01	100	16.8	10391	PASS
442	442	50	100	100.0	62120	PASS
443	442	15	24	19.9	12387	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/22/2022	BNA_G	<u>BG053254.D</u>
Compound Name	Response	Retention Time
DDT	225128	20.937
DDD	12274	20.49
DDE	65	20.061
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12339	237467	5.20

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
 Data File : BG053254.D
 Acq On : 22 Apr 2022 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Apr 24 04:30:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Apr 24 01:13:30 2022
 Response via : Initial Calibration

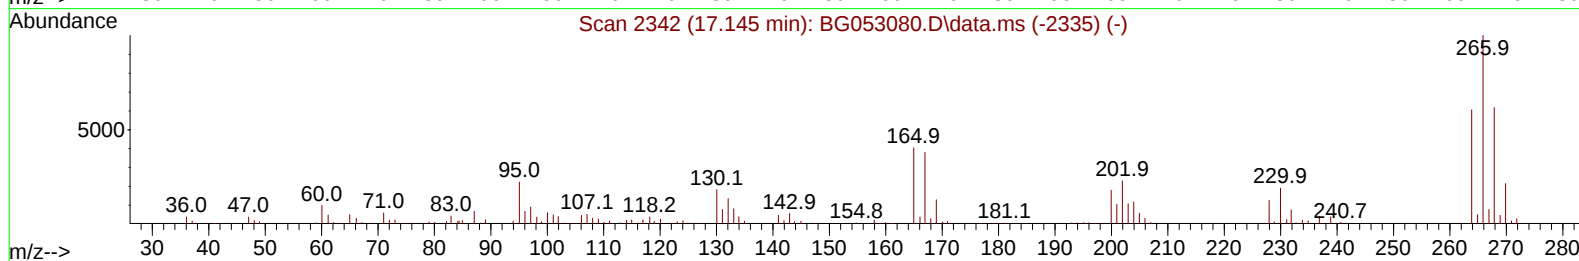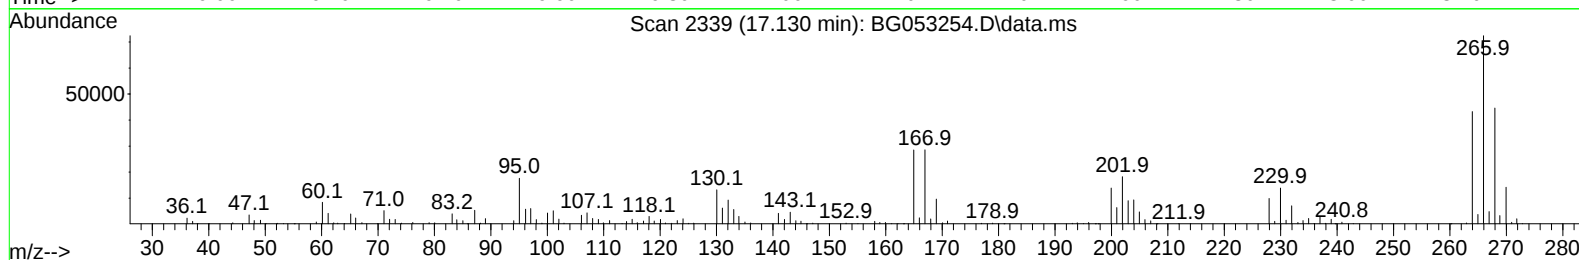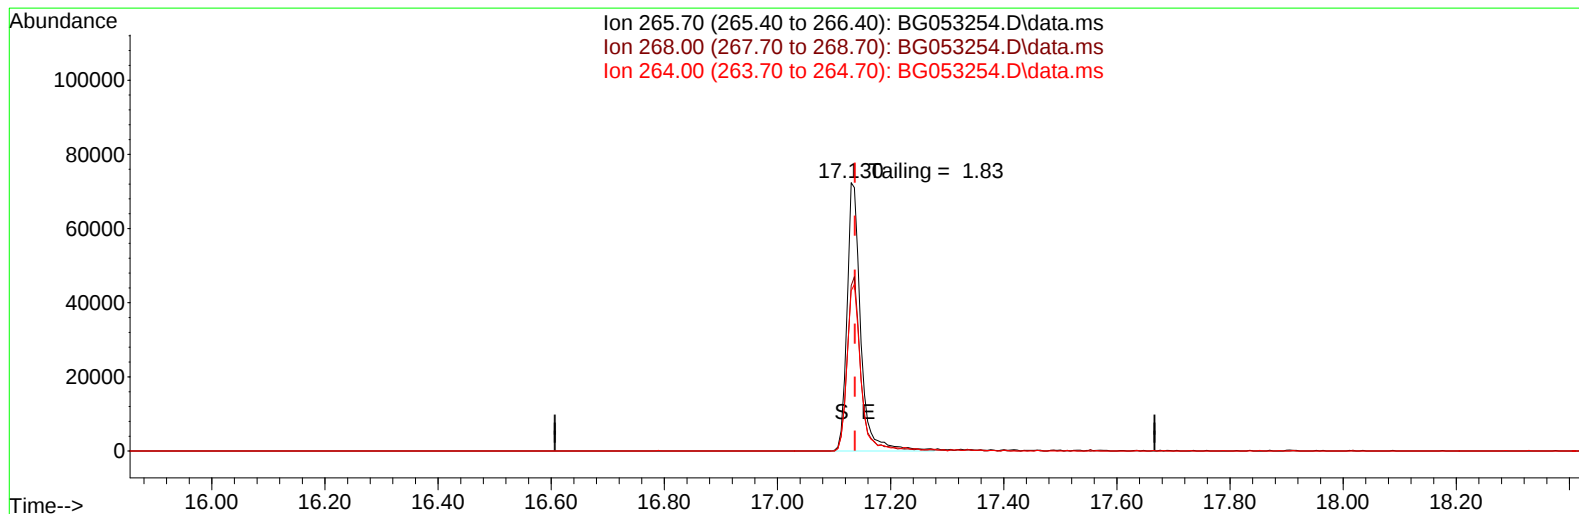

TIC: BG053254.D\data.ms

(70) Pentachlorophenol (C)

17.130min (-0.006) 40187.77 ng




response 121606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.63
264.00	56.60	59.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053254.D
Acq On : 22 Apr 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 24 04:30:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

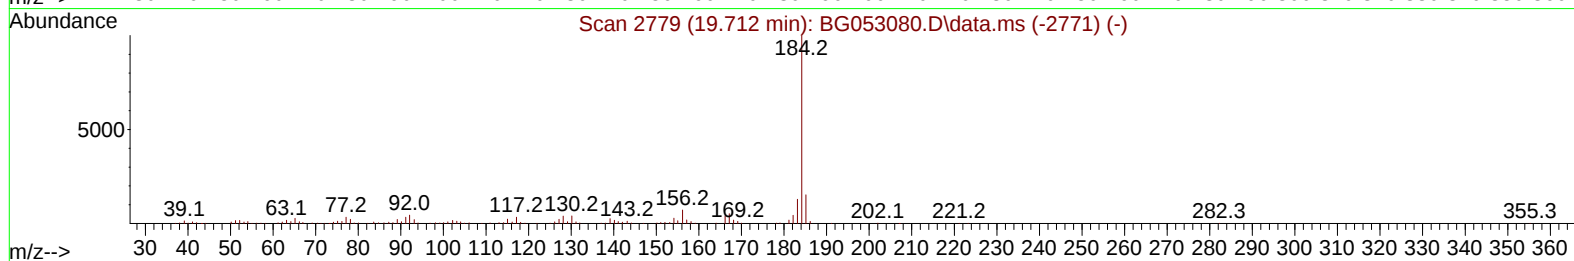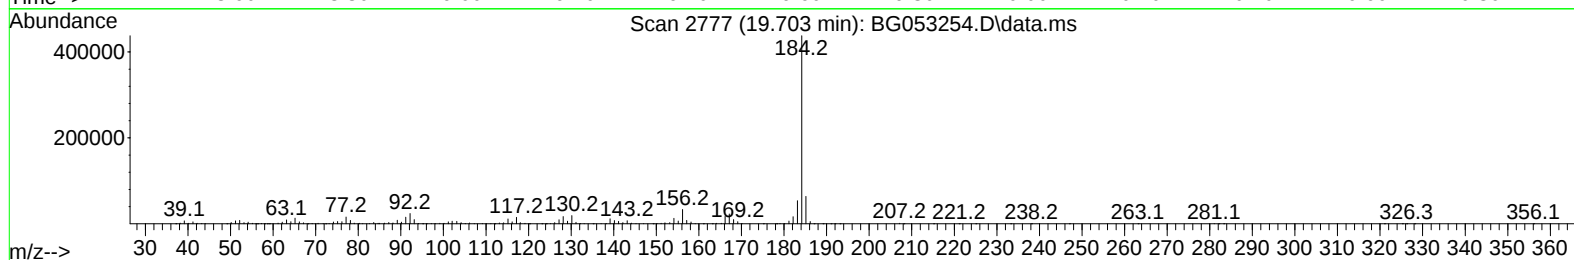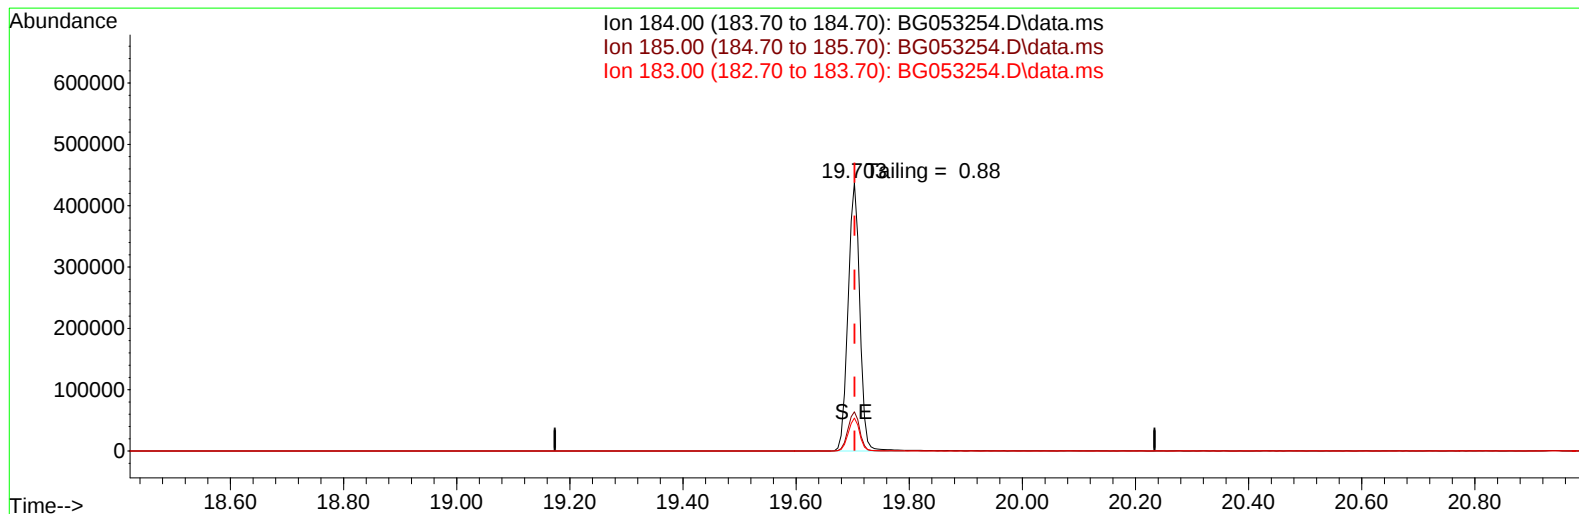

TIC: BG053254.D\data.ms

(77) Benzidine

19.703min (-0.001) 329371.94 ng

response 629633

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.62
183.00	11.80	12.32
0.00	0.00	0.00