
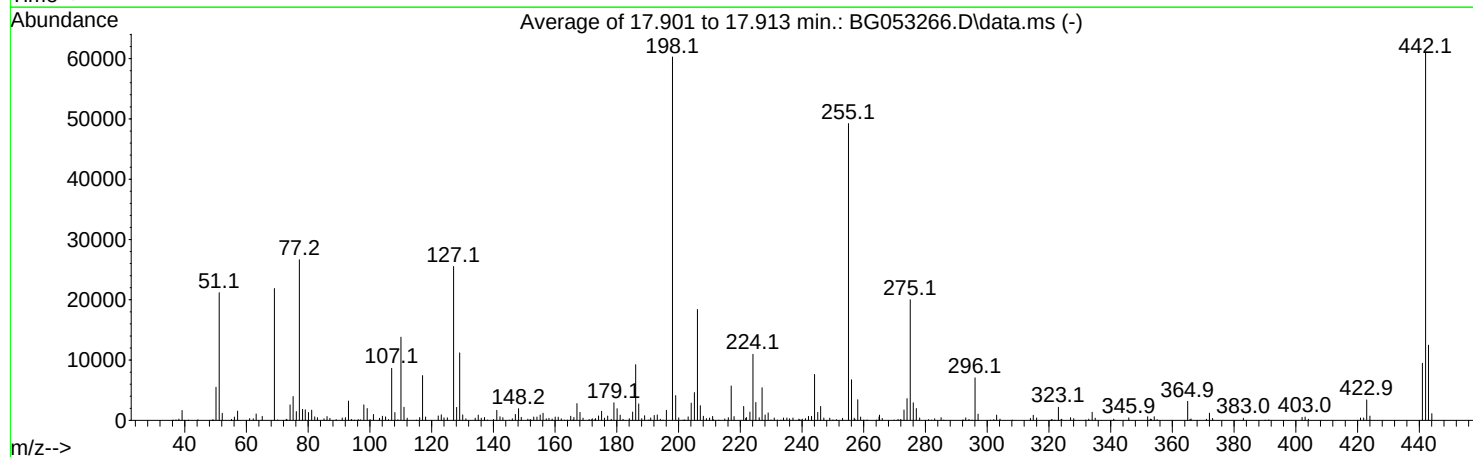


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
 Data File : BG053266.D
 Acq On : 22 Apr 2022 18:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 01:13:30 2022

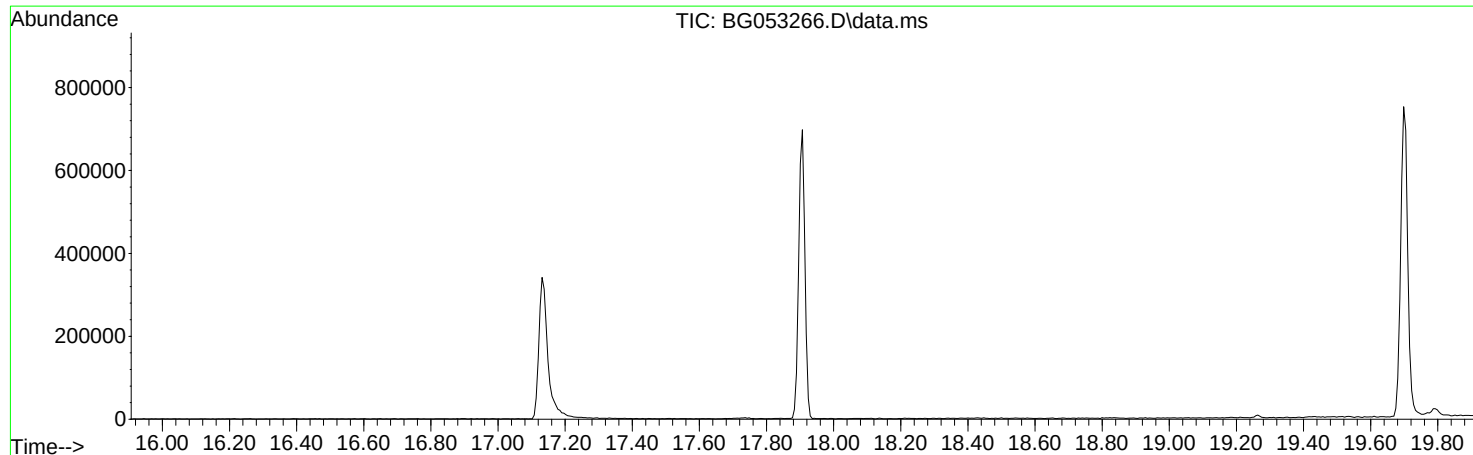

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	21178	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.3	21865	PASS
70	69	0.00	2	0.4	77	PASS
127	198	10	80	42.4	25533	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60275	PASS
199	198	5	9	6.8	4120	PASS
275	198	10	60	33.2	20000	PASS
365	198	1	100	5.2	3147	PASS
441	198	0.01	100	15.7	9472	PASS
442	442	50	100	100.0	61019	PASS
443	442	15	24	20.4	12472	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/22/2022	BNA_G	<u>BG053266.D</u>
Compound Name	Response	Retention Time
DDT	237100	20.938
DDD	15008	20.497
DDE	223	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15231	252331	6.04

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042222\
Data File : BG053266.D
Acq On : 22 Apr 2022 18:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 24 04:37:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

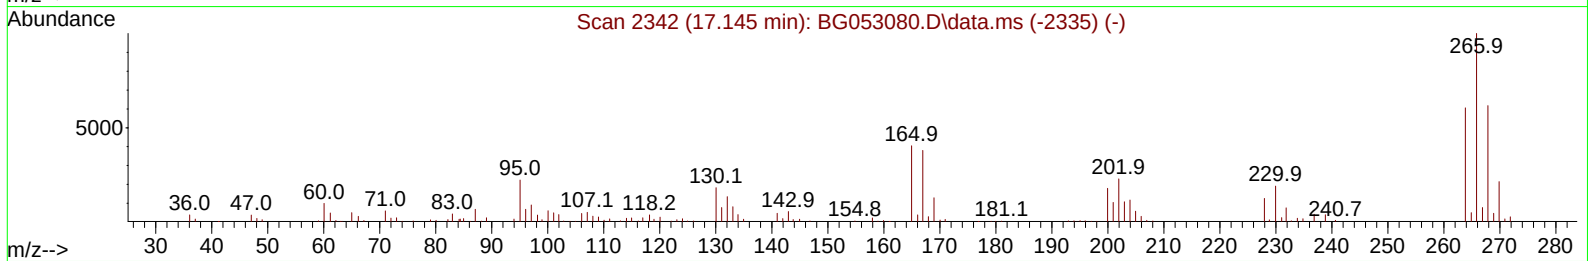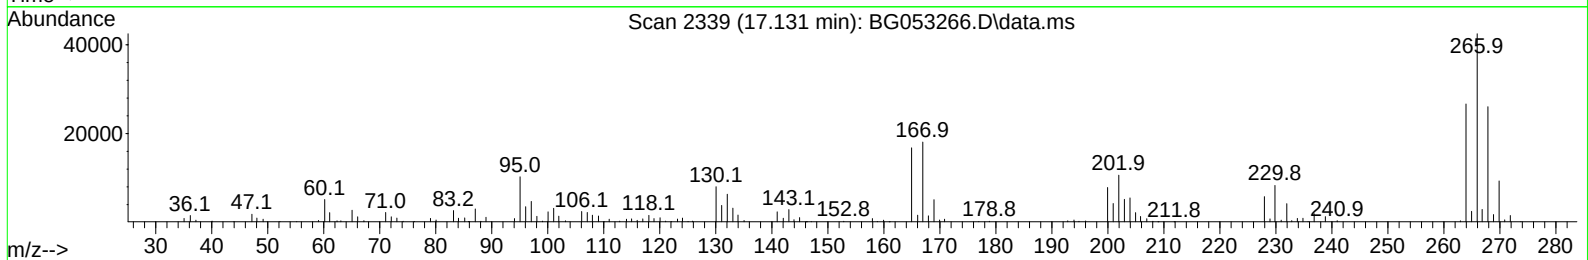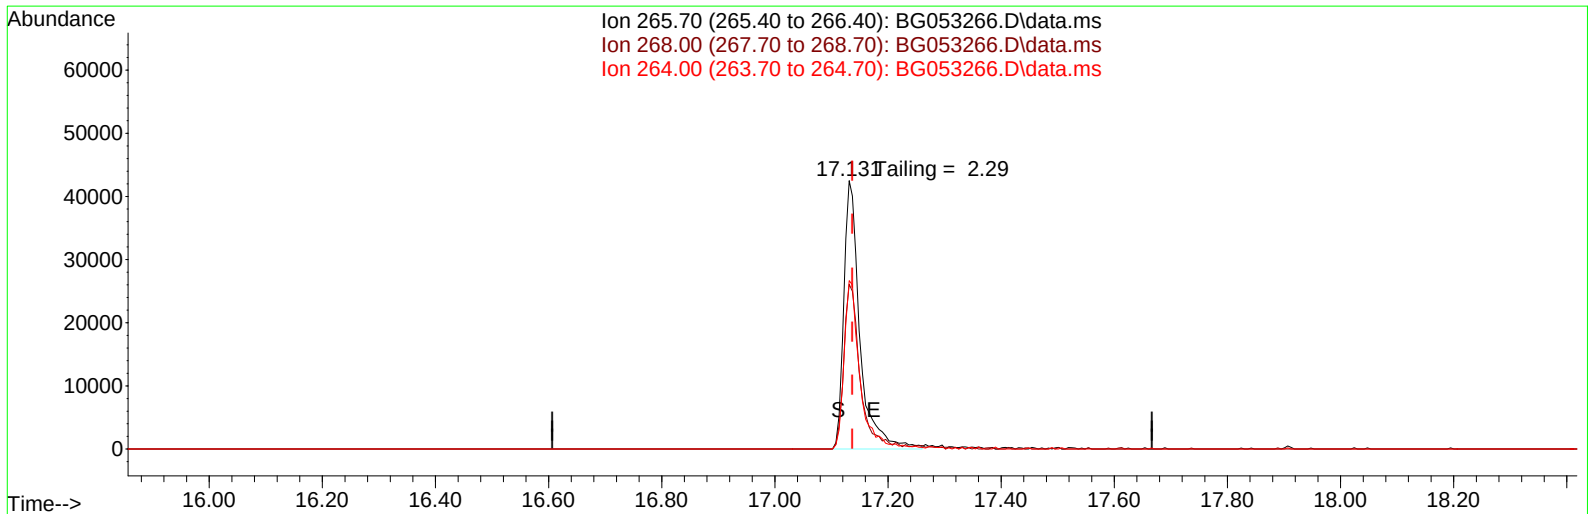

TIC: BG053266.D\data.ms

(70) Pentachlorophenol (C)

17.131min (-0.005) 23834.97 ng

response 84415

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	61.34
264.00	56.60	62.75
0.00	0.00	0.00

