
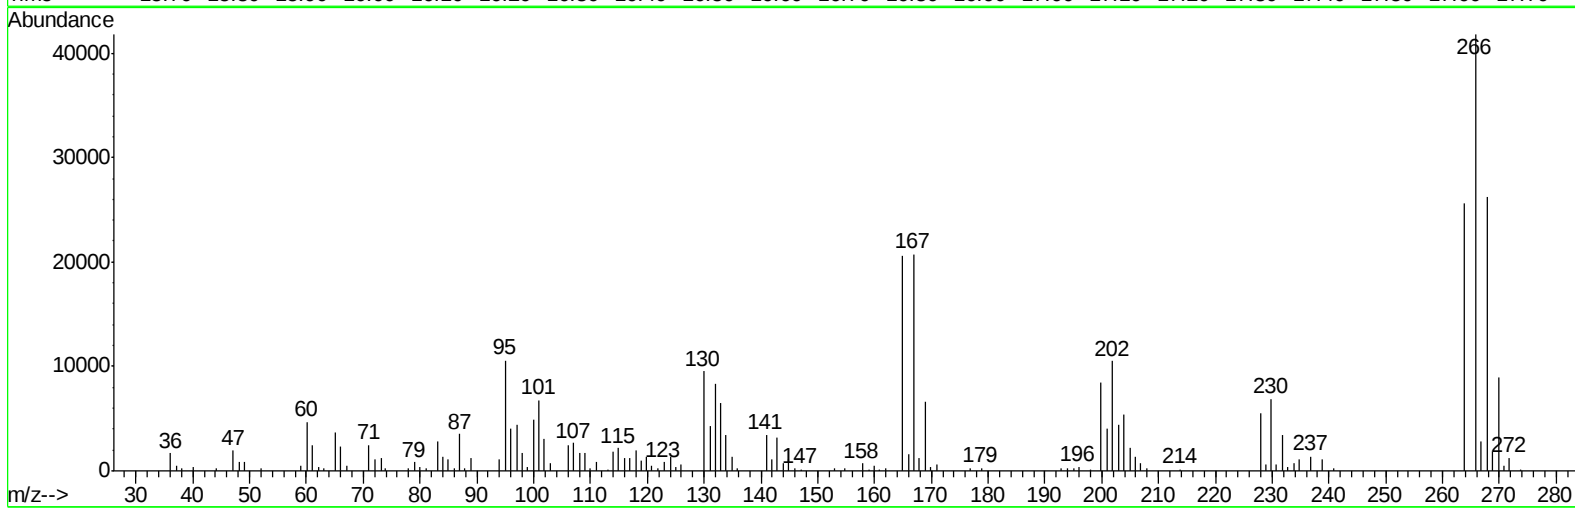


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042315\
Data File : BG016651.D
Acq On : 23 Apr 2015 13:15
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 03:44:56 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

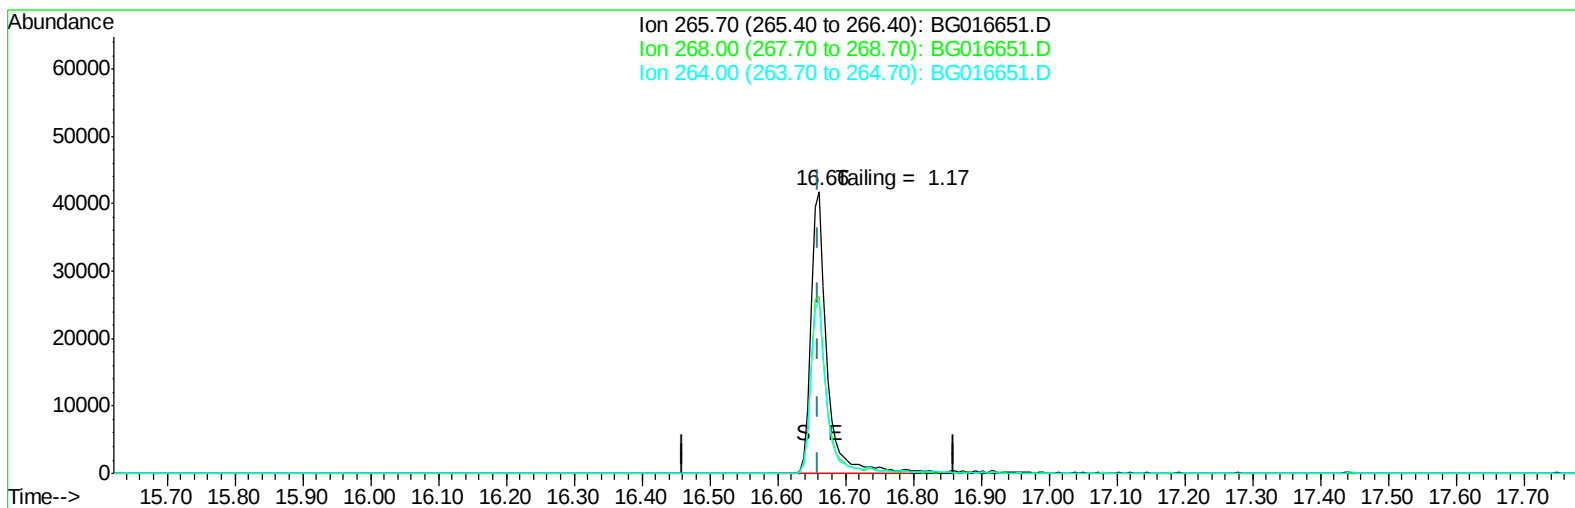

TIC: BG016651.D

(69) Pentachlorophenol (C)



16.662min (+0.002) 38882.79ng

response 67337

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	62.72
264.00	64.70	61.32
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042315\
Data File : BG016651.D
Acq On : 23 Apr 2015 13:15
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 03:44:56 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

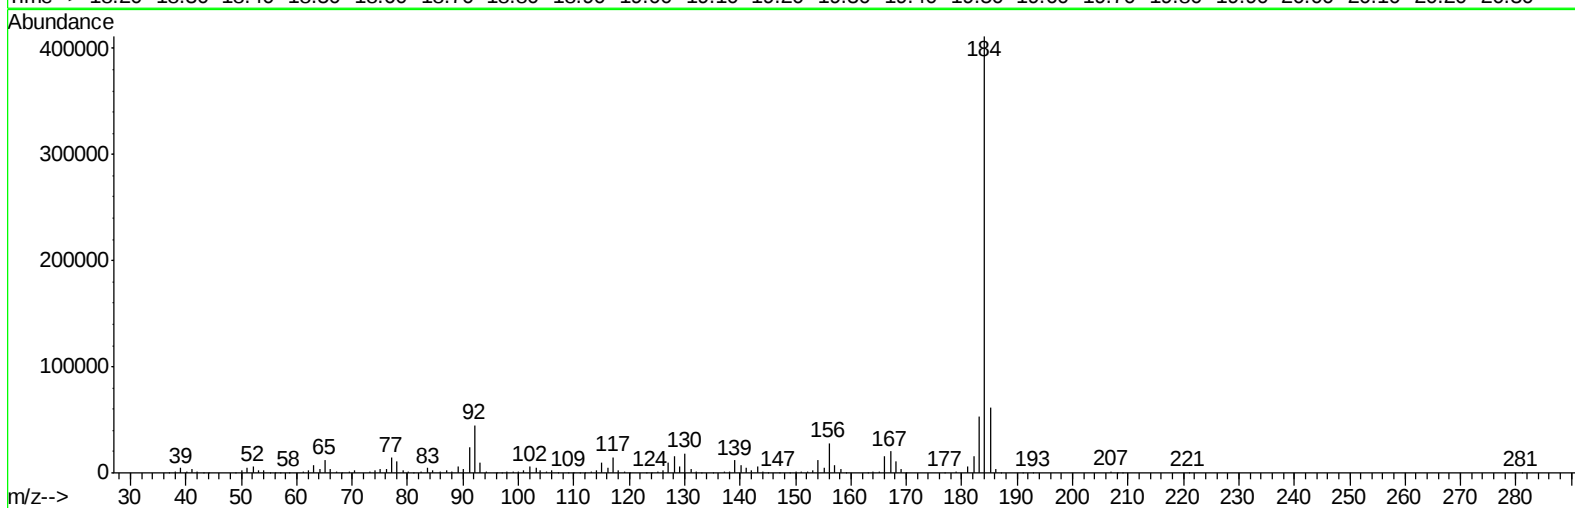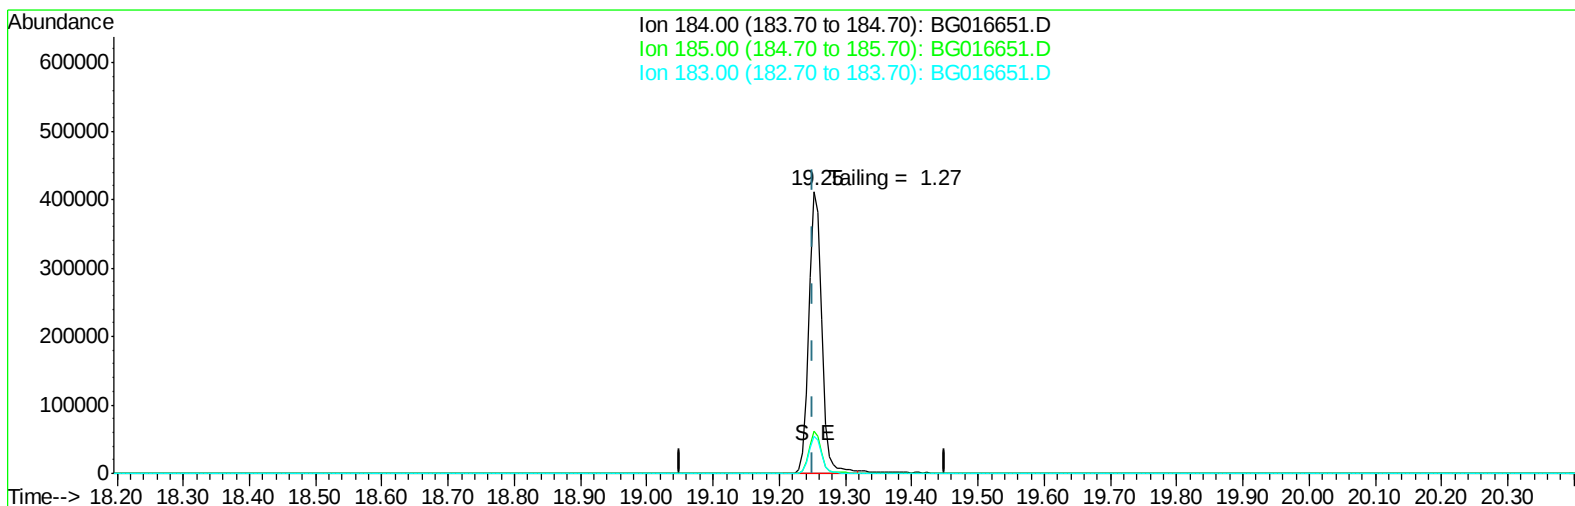

TIC: BG016651.D

(76) Benzidine

19.253min (+0.002) 24371.12ng

response 573567

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.96
183.00	12.60	13.06
0.00	0.00	0.00