
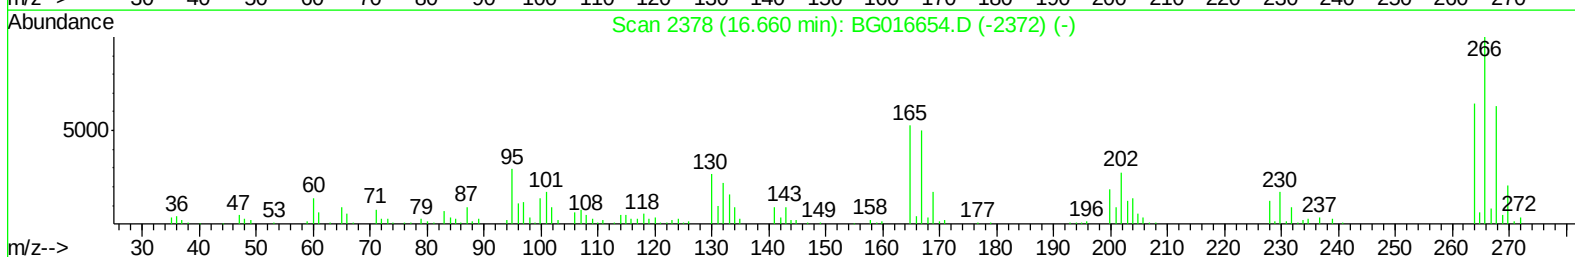
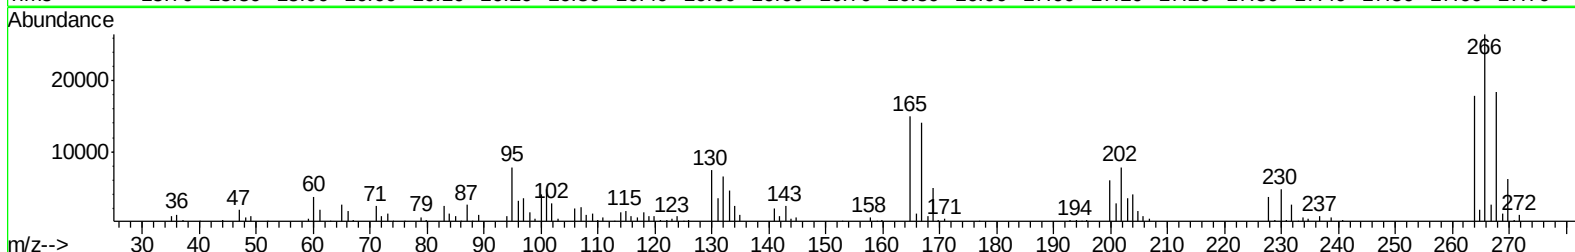


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042315\
Data File : BG016668.D
Acq On : 24 Apr 2015 1:30
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 03:45:48 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

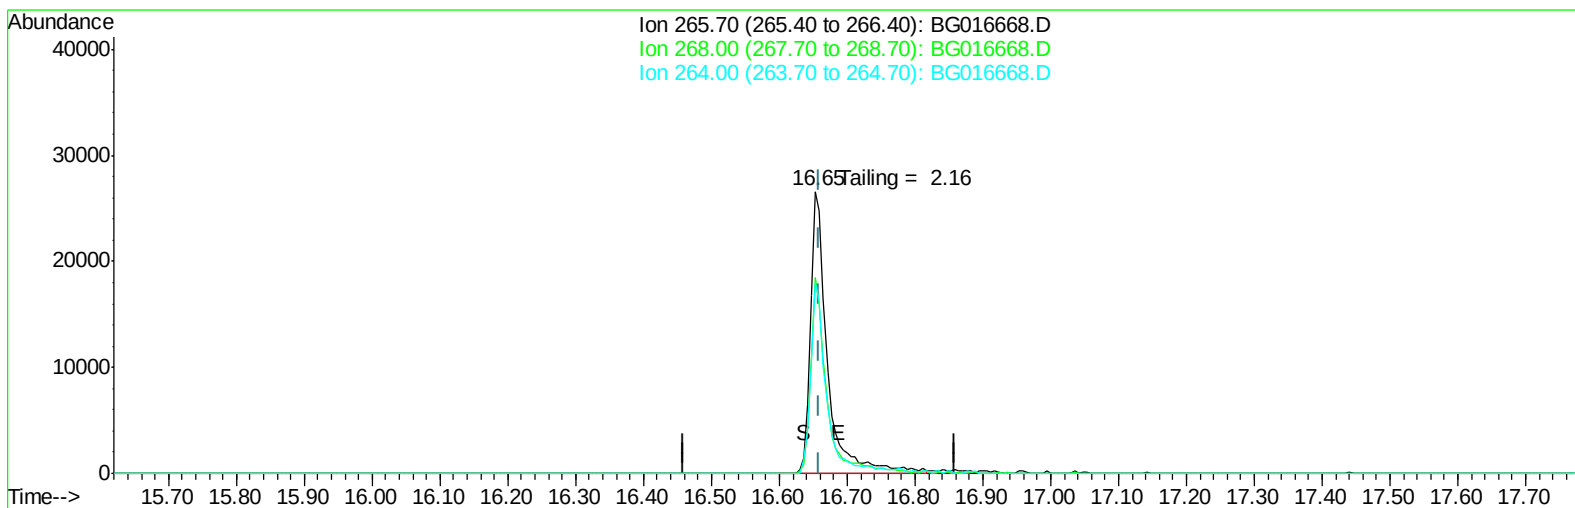

TIC: BG016668.D

(69) Pentachlorophenol (C)




16.653min (-0.007) 26860.53ng m

response 46629

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	69.65
264.00	64.70	67.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042315\
Data File : BG016668.D
Acq On : 24 Apr 2015 1:30
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 03:45:48 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

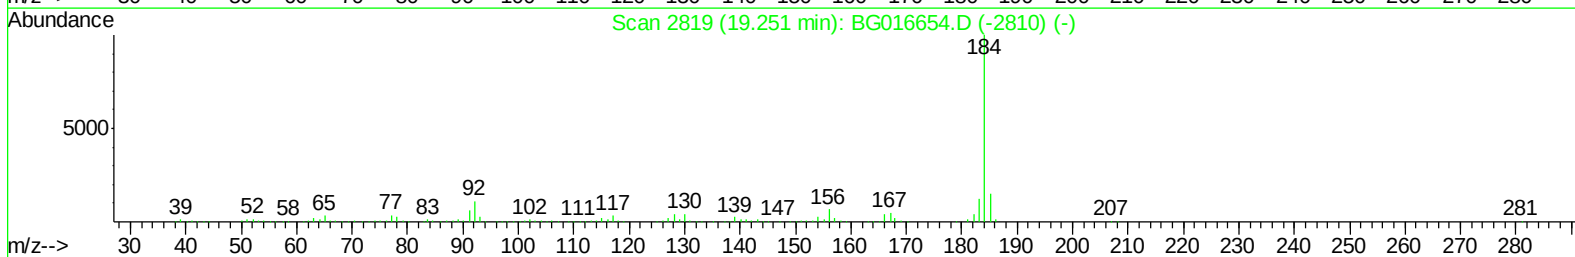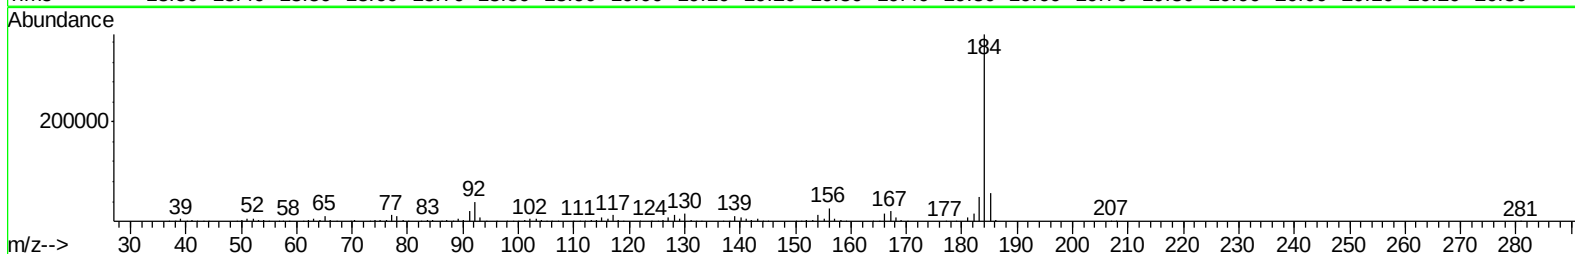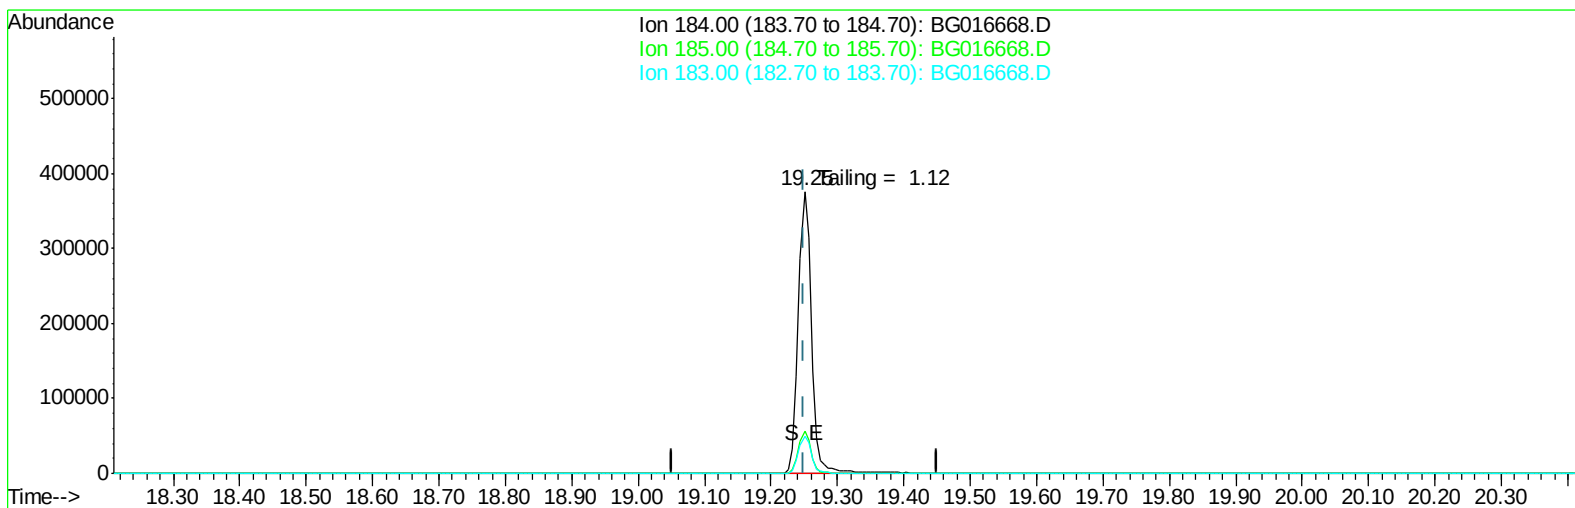

TIC: BG016668.D

(76) Benzidine

19.250min (-0.001) 25560.10ng

response 497954

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.82
183.00	12.60	13.10
0.00	0.00	0.00