

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042315\
 Data File : BG016662.D
 Acq On : 23 Apr 2015 20:53
 Operator : TP/IZ
 Sample : PB82956BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB82956BL

Quant Time: Apr 24 02:24:59 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 23 19:19:11 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	53461	20.00	ng	0.00
21) Naphthalene-d8	10.38	136	215041	20.00	ng	0.00
38) Acenaphthene-d10	14.25	164	120594	20.00	ng	0.00
63) Phenanthrene-d10	16.99	188	281375	20.00	ng	0.00
75) Chrysene-d12	21.18	240	284770	20.00	ng	0.00
86) Perylene-d12	23.39	264	258478	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	350001	106.24	ng	0.00
7) Phenol-d6	6.79	99	456618	98.80	ng	0.00
23) Nitrobenzene-d5	8.76	82	222043	65.25	ng	0.00
41) 2,4,6-Tribromophenol	15.74	330	94474	105.60	ng	0.00
44) 2-Fluorobiphenyl	12.87	172	515218	68.64	ng	0.00
78) Terphenyl-d14	19.63	244	775652	62.74	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042315\
Data File : BG016662.D
Acq On : 23 Apr 2015 20:53
Operator : TP/IZ
Sample : PB82956BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB82956BL

Quant Time: Apr 24 02:24:59 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

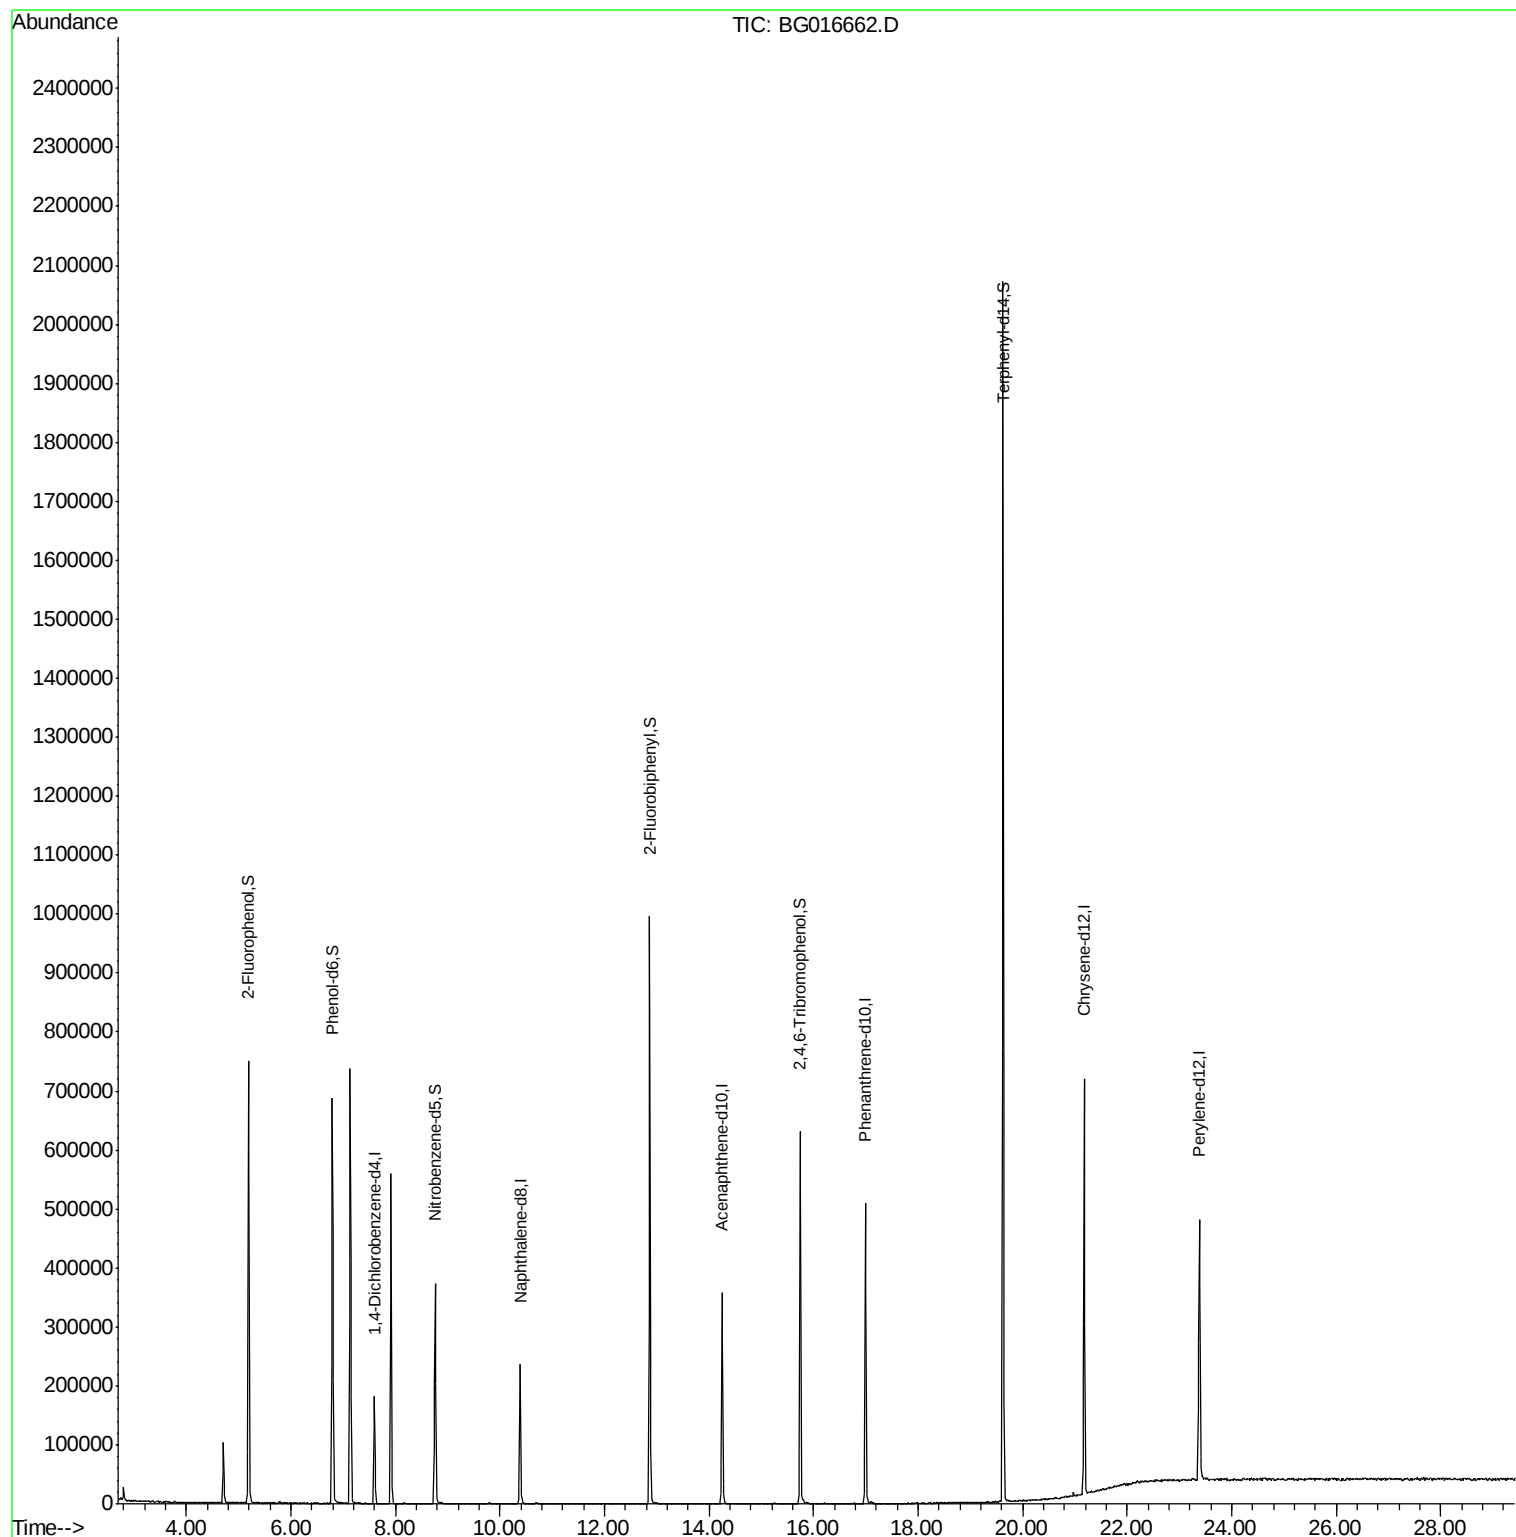

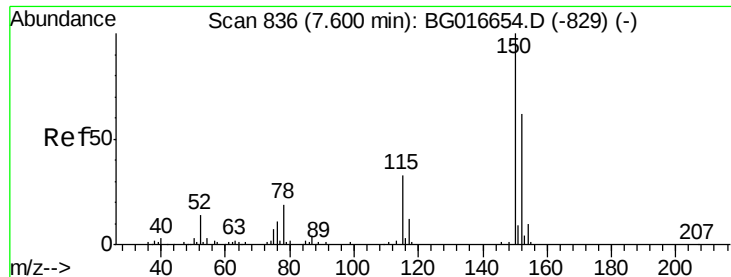


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.60 min Scan# 836
Delta R.T. -0.00 min
Lab File: BG016662.D
Acq: 23 Apr 2015 20:53

Instrument :
BNA_G
ClientSampleId :
PB82956BL

Tot Ion	Ratio	Lower	Upper
152	100		
150	150.1	129.6	194.4
115	51.1	43.0	64.6

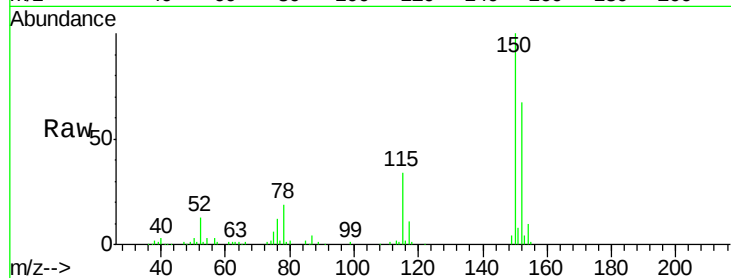


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

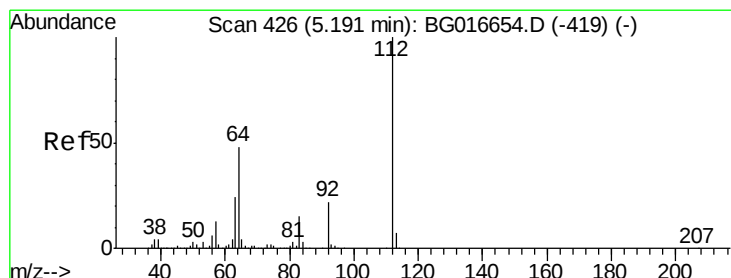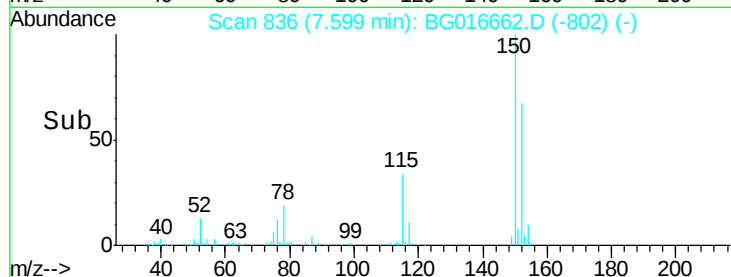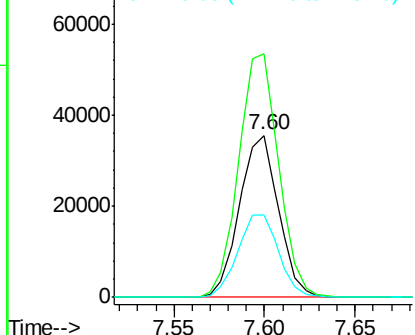



#5

2-Fluorophenol
Concen: 106.24 ng
RT: 5.19 min Scan# 426
Delta R.T. -0.00 min
Lab File: BG016662.D
Acq: 23 Apr 2015 20:53

Tgt Ion	Ratio	Lower	Upper
112	100		
64	47.8	38.3	57.5
63	23.6	18.9	28.3

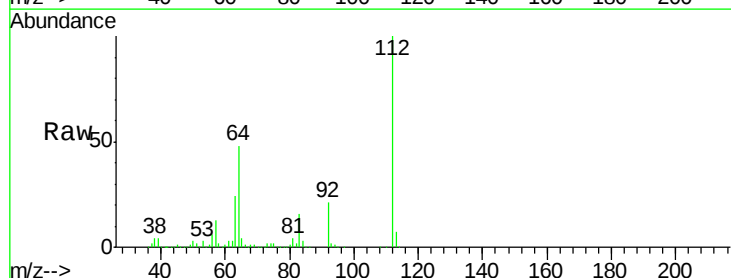

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

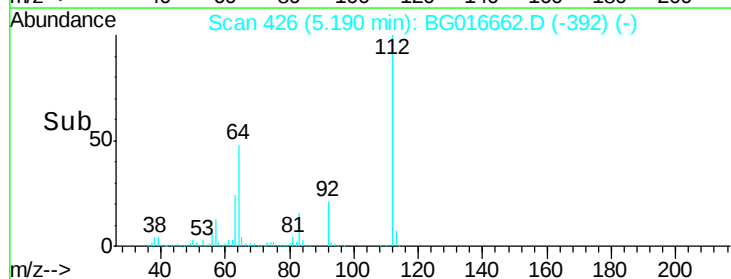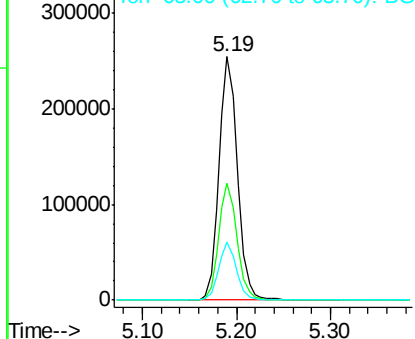



#7

Phenol-d6

Concen: 98.80 ng

RT: 6.79 min Scan# 699

Delta R.T. -0.01 min

Lab File: BG016662.D

Acq: 23 Apr 2015 20:53

Instrument :

BNA_G

ClientSampleId :

PB82956BL


Tot Ion: 99 Resp: 456618

Ion Ratio Lower Upper




99 100

42 11.9 8.8 13.2

71 25.2 19.9 29.9

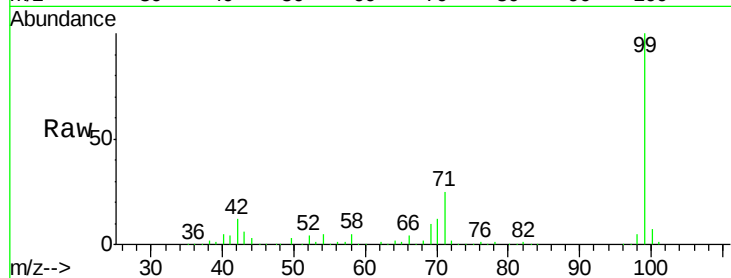

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

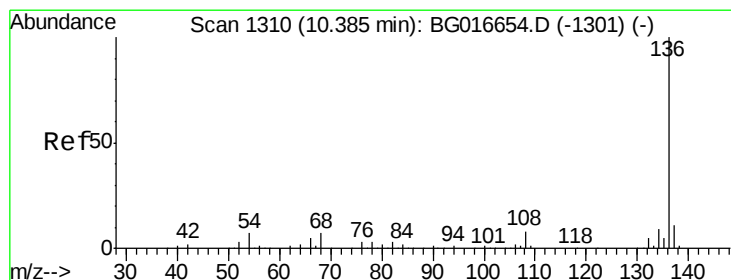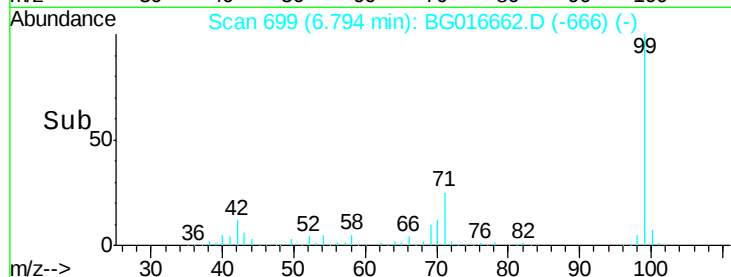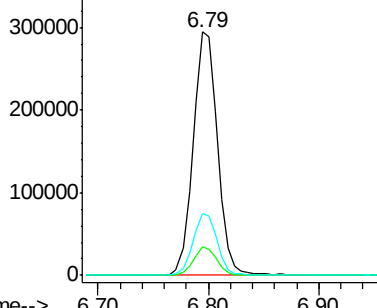

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.38 min Scan# 1310

Delta R.T. -0.00 min

Lab File: BG016662.D

Acq: 23 Apr 2015 20:53

Tgt Ion: 136 Resp: 215041


Ion Ratio Lower Upper

136 100



137 11.0 8.5 12.7

54 6.2 5.4 8.2

68 6.0 5.2 7.8

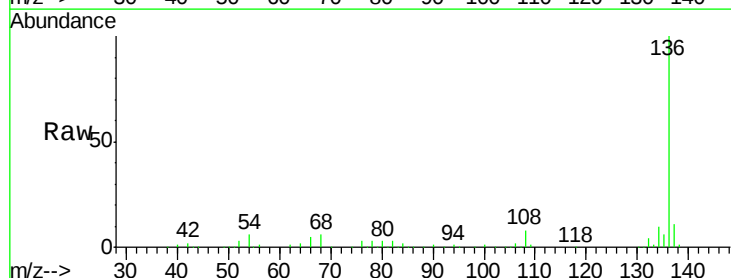

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

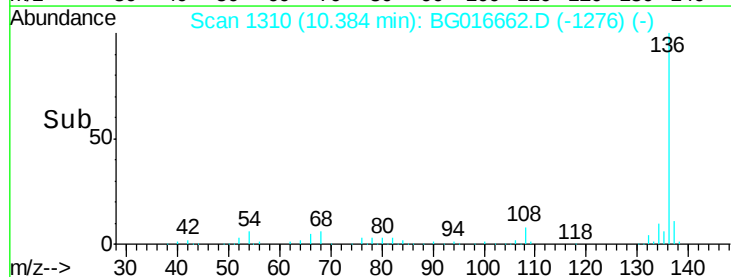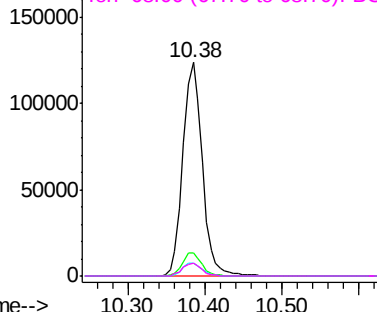







#23
 Nitrobenzene-d5
 Concen: 65.25 ng
 RT: 8.76 min Scan# 1033
 Delta R.T. -0.01 min
 Lab File: BG016662.D
 Acq: 23 Apr 2015 20:53

Instrument :
 BNA_G
 ClientSampleID :
 PB82956BL

Tot Ion	82	Resp	222043
Ion Ratio	100	Lower	Upper
128	53.0	44.7	67.1
54	38.6	30.9	46.3

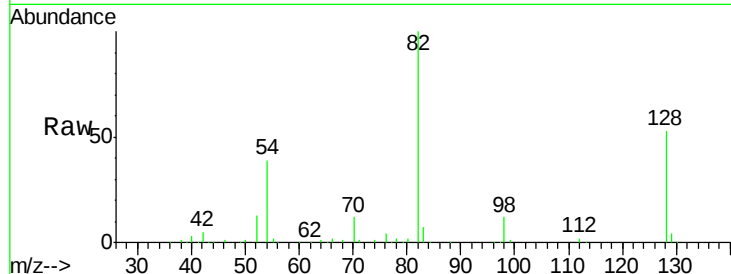


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

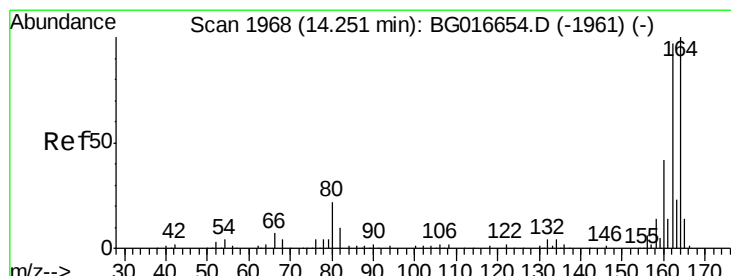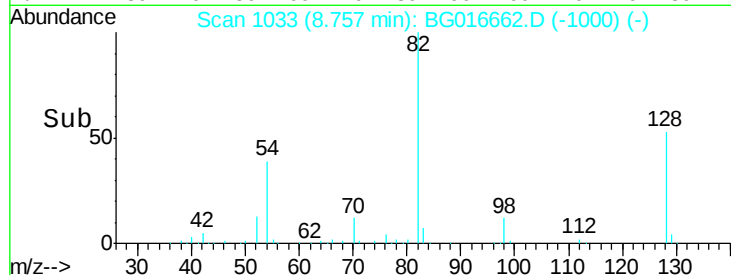
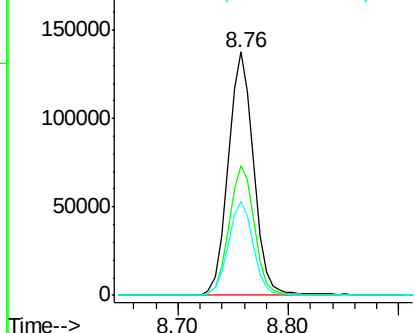


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.25 min Scan# 1968
 Delta R.T. -0.00 min
 Lab File: BG016662.D
 Acq: 23 Apr 2015 20:53

Tgt Ion	164	Resp	120594
Ion Ratio	100	Lower	Upper
162	94.3	77.3	115.9
160	44.3	33.7	50.5

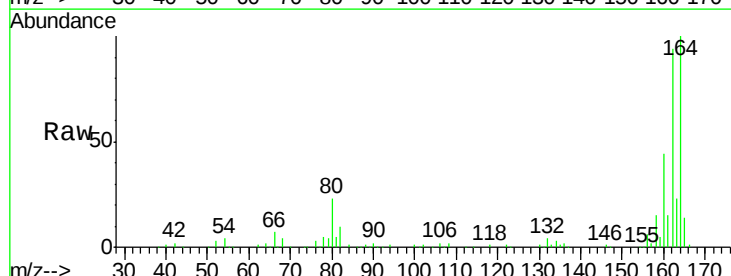

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

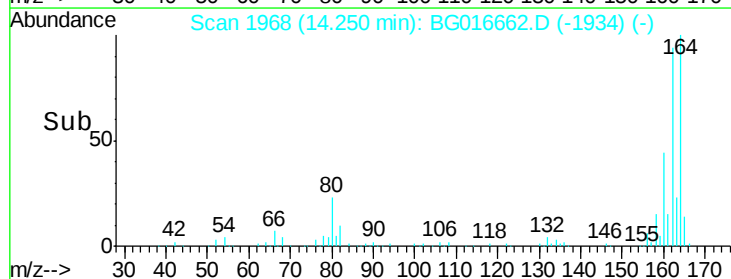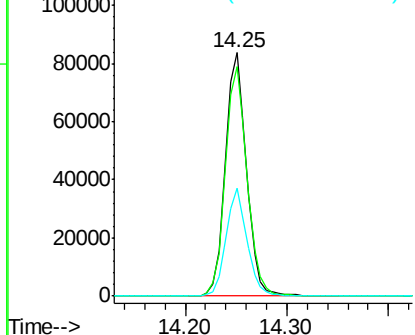







#41
 2,4,6-Tribromophenol
 Concen: 105.60 ng
 RT: 15.74 min Scan# 2222
 Delta R.T. -0.01 min
 Lab File: BG016662.D
 Acq: 23 Apr 2015 20:53

Instrument :
 BNA_G
 ClientSampleId :
 PB82956BL

Tot Ion:330 Resp: 94474
 Ion Ratio Lower Upper
 330 100
 332 94.9 76.2 114.4
 141 52.8 43.0 64.6

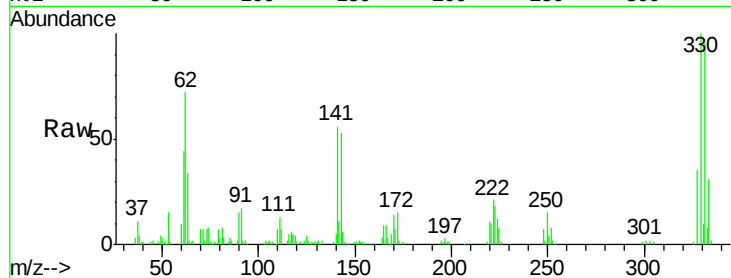


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

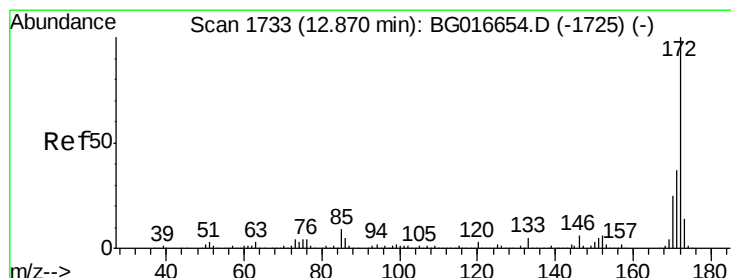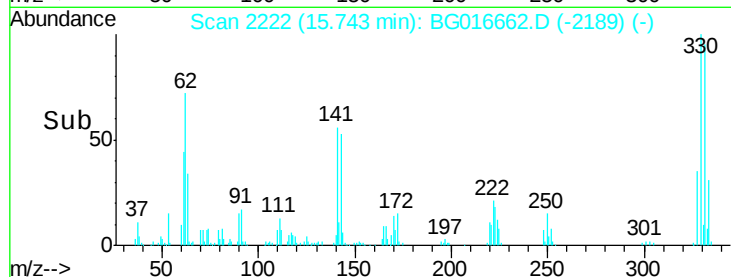
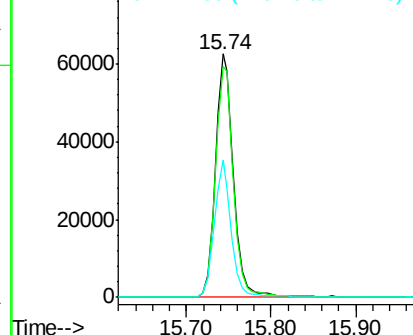



#44
 2-Fluorobiphenyl
 Concen: 68.64 ng
 RT: 12.87 min Scan# 1733
 Delta R.T. -0.00 min
 Lab File: BG016662.D
 Acq: 23 Apr 2015 20:53

Tgt Ion:172 Resp: 515218
 Ion Ratio Lower Upper
 172 100
 171 35.5 29.9 44.9
 170 23.7 19.8 29.8

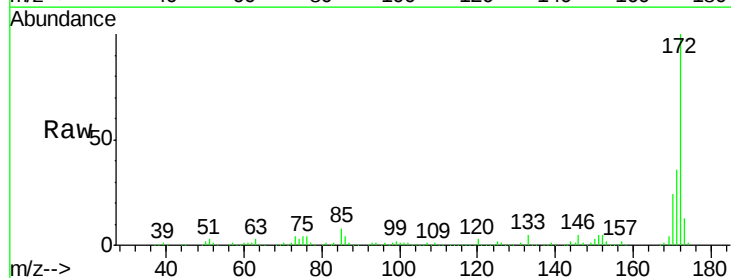

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

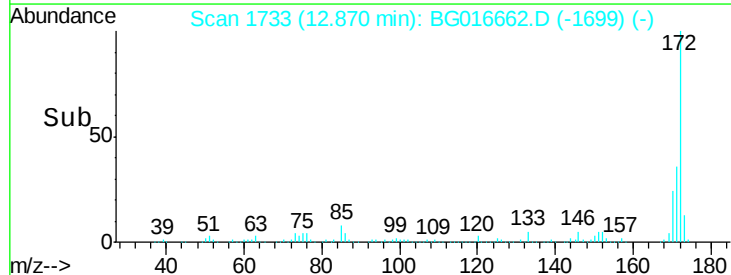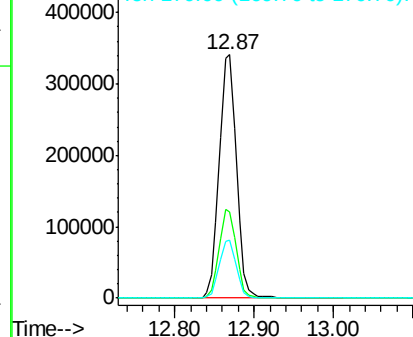


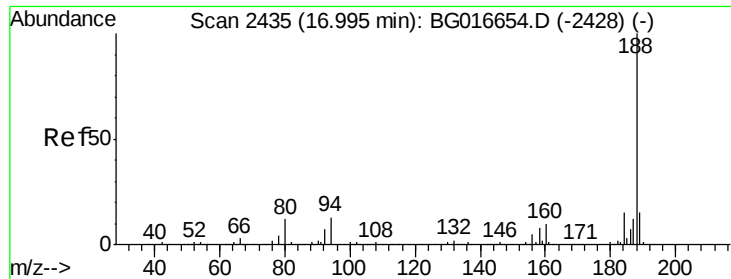




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.99 min Scan# 2435
Delta R.T. -0.00 min
Lab File: BG016662.D
Acq: 23 Apr 2015 20:53

Instrument :
BNA_G
ClientSampled :
PB82956BL

Tot Ion:188 Resp: 281375
Ion Ratio Lower Upper
188 100
94 12.7 10.7 16.1
80 12.1 9.9 14.9

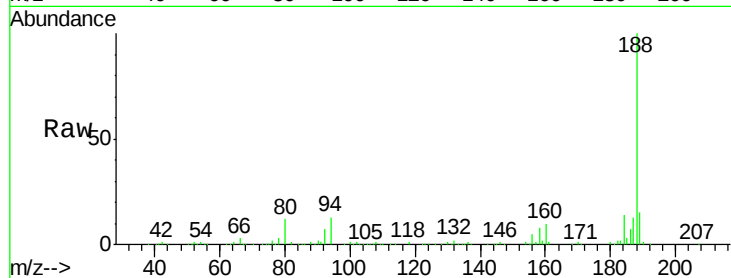


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): B
Ion 80.00 (79.70 to 80.70): B

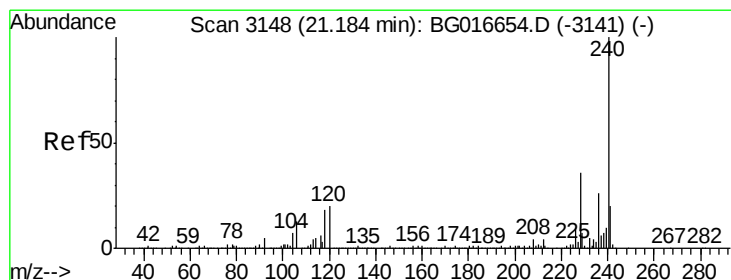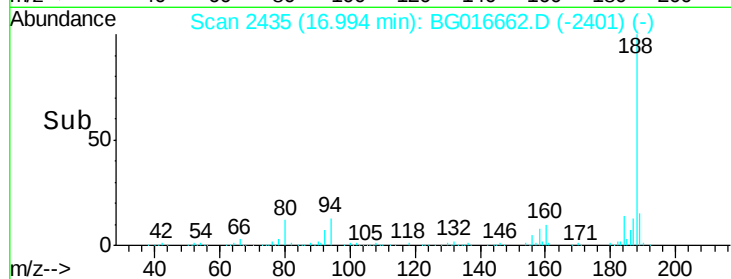
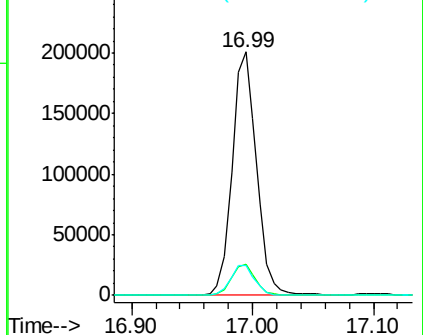



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.18 min Scan# 3147
Delta R.T. -0.01 min
Lab File: BG016662.D
Acq: 23 Apr 2015 20:53

Tgt Ion:240 Resp: 284770
Ion Ratio Lower Upper
240 100
120 20.1 16.3 24.5
236 26.6 21.1 31.7

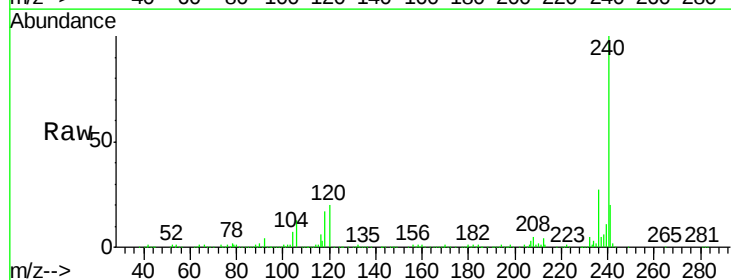

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

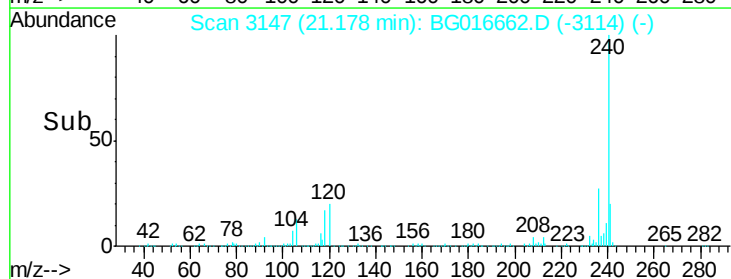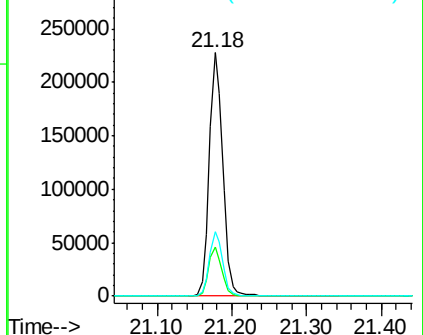

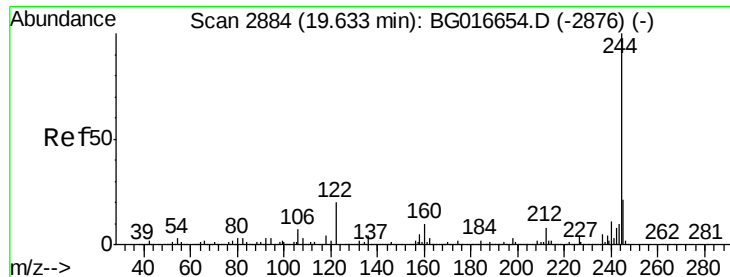

#78

Terphenyl-d14

Concen: 62.74 ng

RT: 19.63 min Scan# 2883

Delta R.T. -0.01 min

Lab File: BG016662.D

Acq: 23 Apr 2015 20:53

Instrument :

BNA_G

ClientSampleId :

PB82956BL


Tot Ion:244 Resp: 775652

Ion Ratio Lower Upper

244 100

212 8.4 6.4 9.6




122 20.9 15.9 23.9

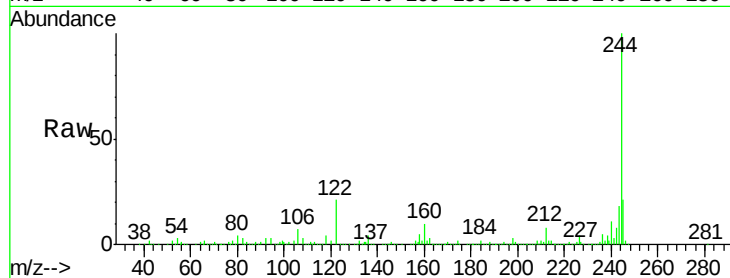

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

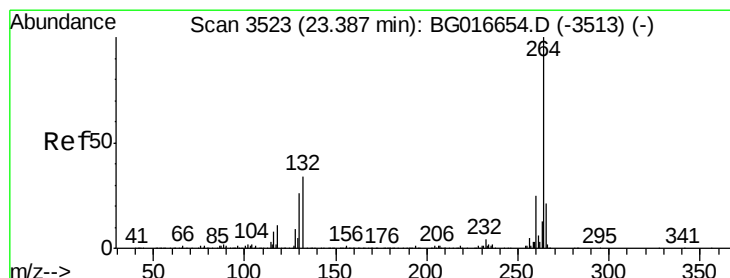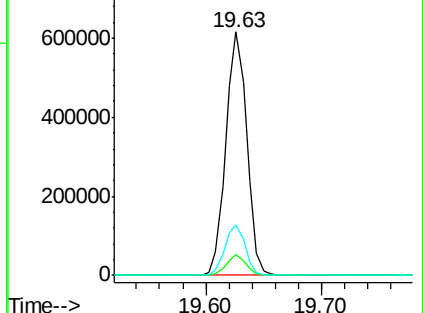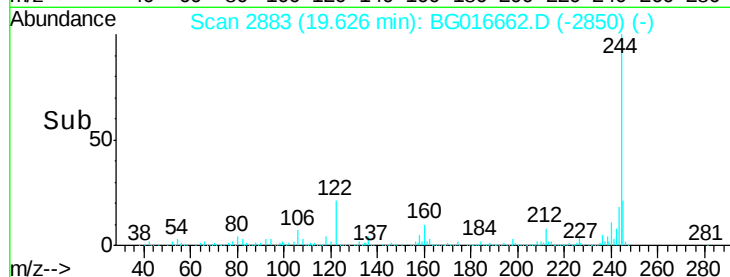

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.39 min Scan# 3523

Delta R.T. -0.00 min

Lab File: BG016662.D

Acq: 23 Apr 2015 20:53


Tgt Ion:264 Resp: 258478

Ion Ratio Lower Upper

264 100

260 24.4 20.0 30.0

265 20.8 16.8 25.2

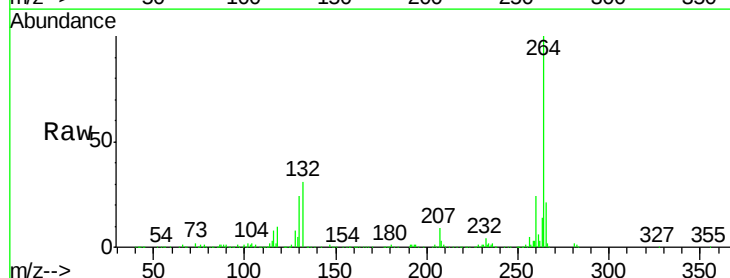

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

