
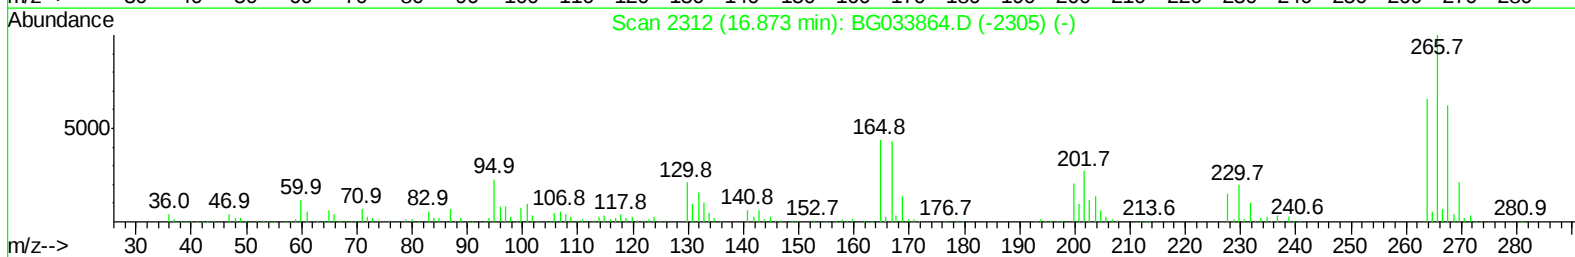
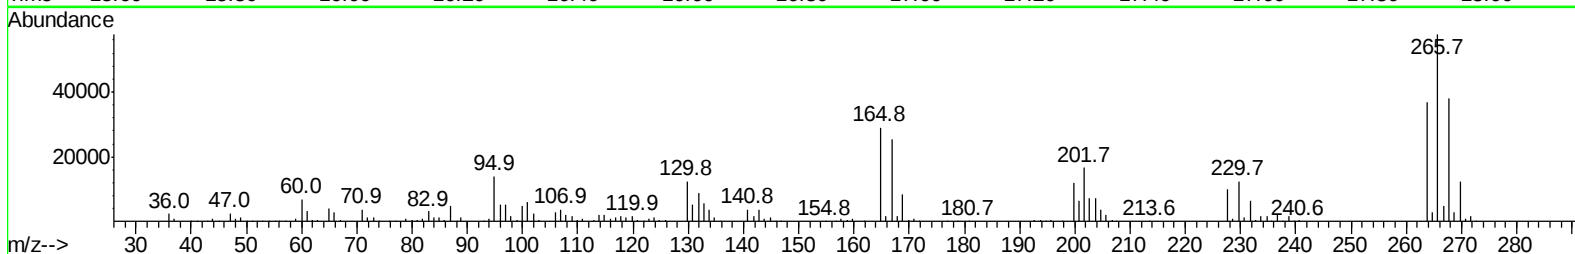


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042318\
Data File : BG033914.D
Acq On : 23 Apr 2018 10:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 05:08:01 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

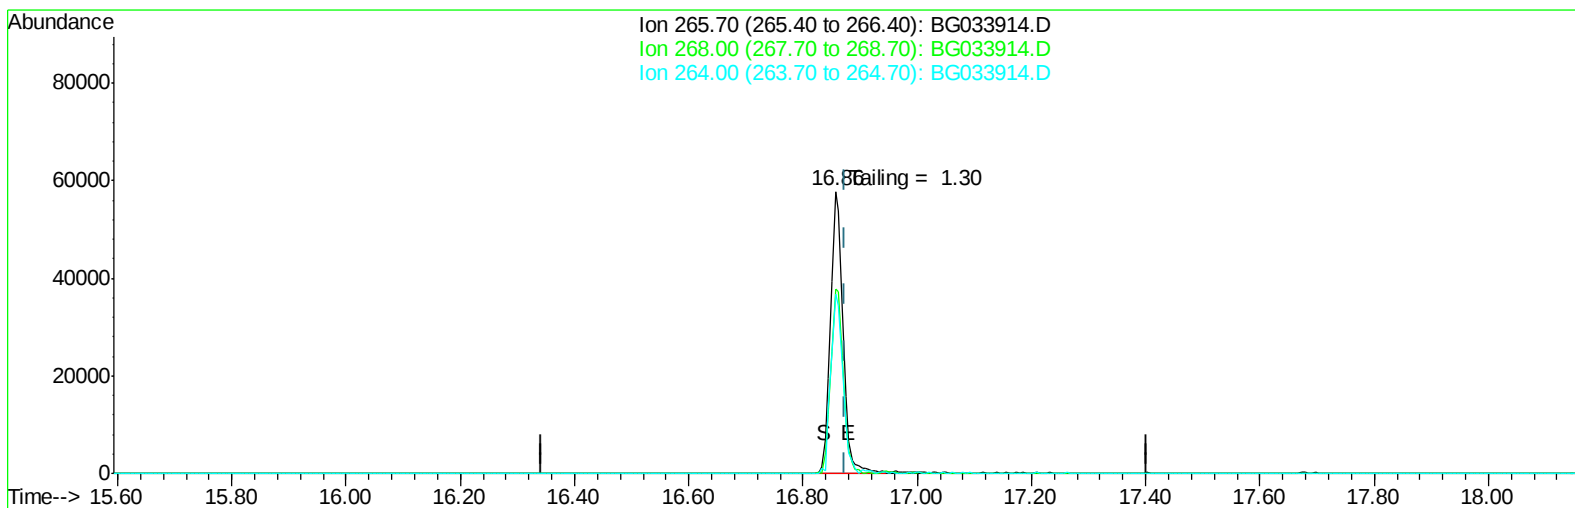

TIC: BG033914.D

(69) Pentachlorophenol (C)




16.856min (-0.017) 174494.08ng

response 87034

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.45
264.00	62.00	68.38
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042318\
Data File : BG033914.D
Acq On : 23 Apr 2018 10:01
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 05:08:01 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

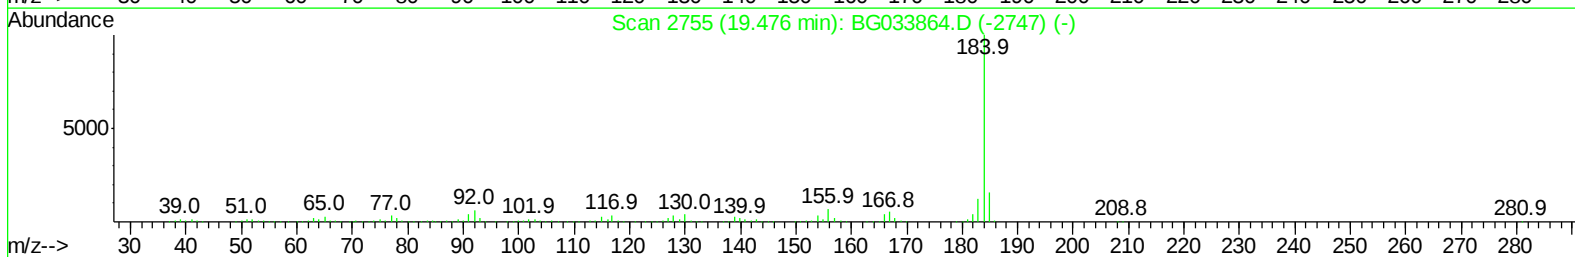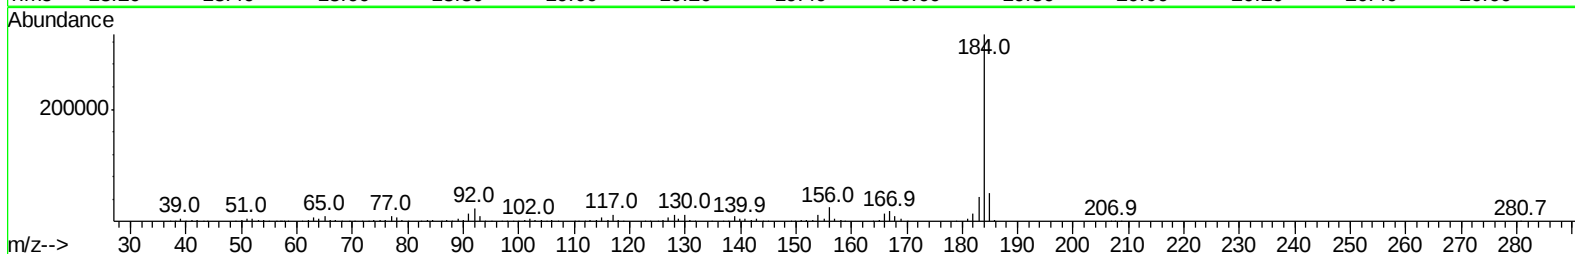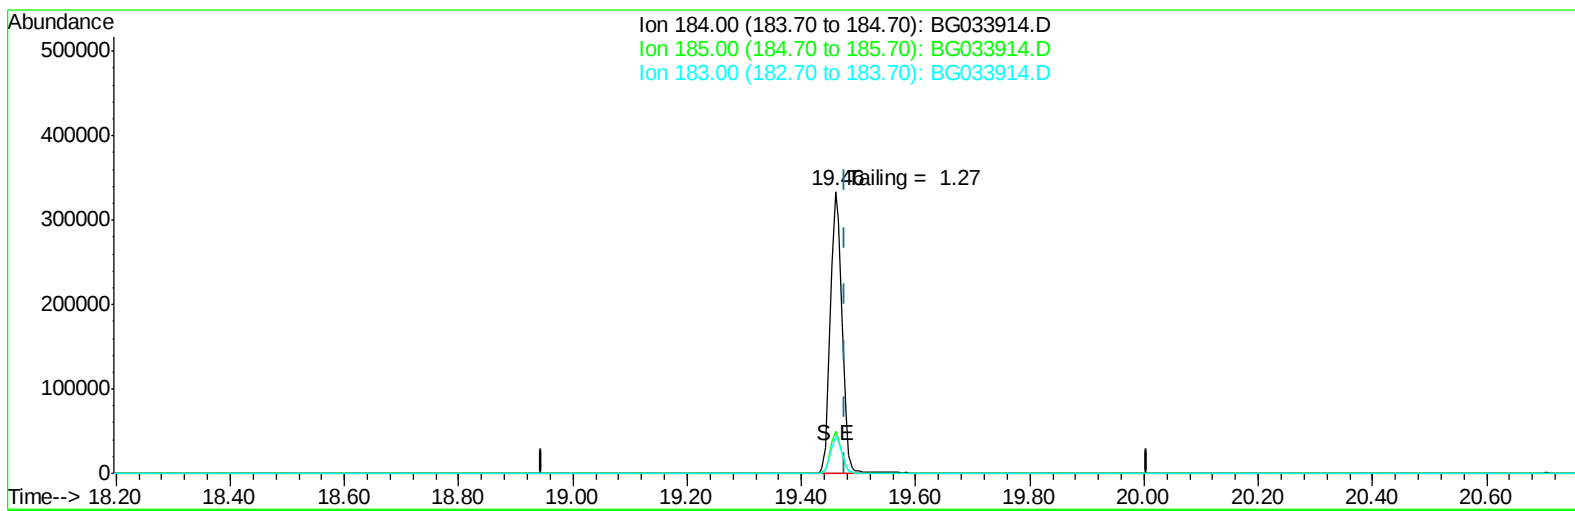

TIC: BG033914.D

(76) Benzidine

19.459min (-0.017) 0.00ng

response 470100

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.99
183.00	13.30	13.18
0.00	0.00	0.00