
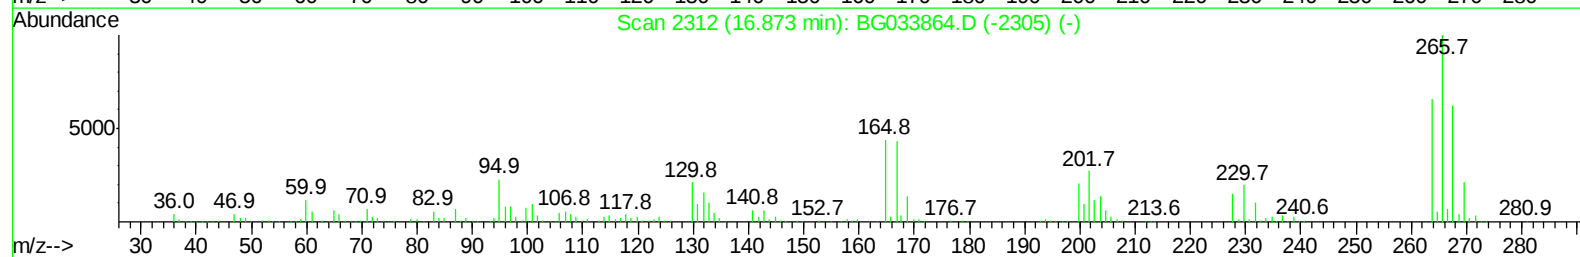
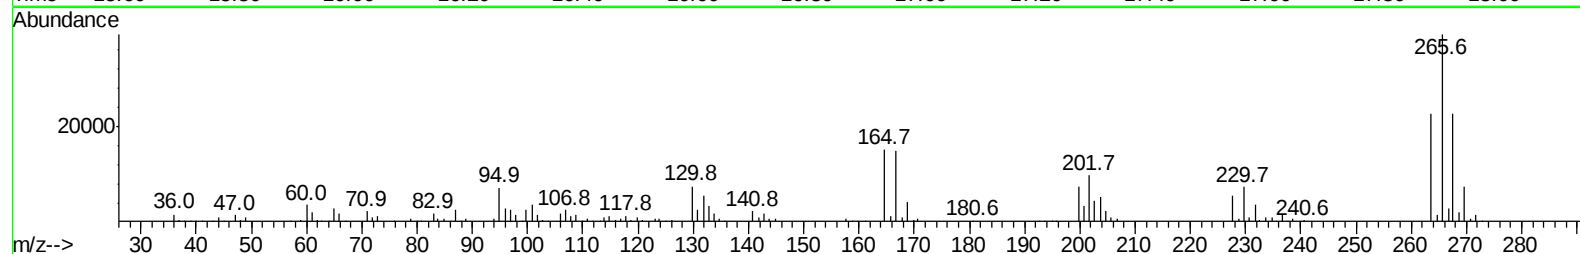


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042318\
Data File : BG033932.D
Acq On : 23 Apr 2018 22:54
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 05:09:05 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

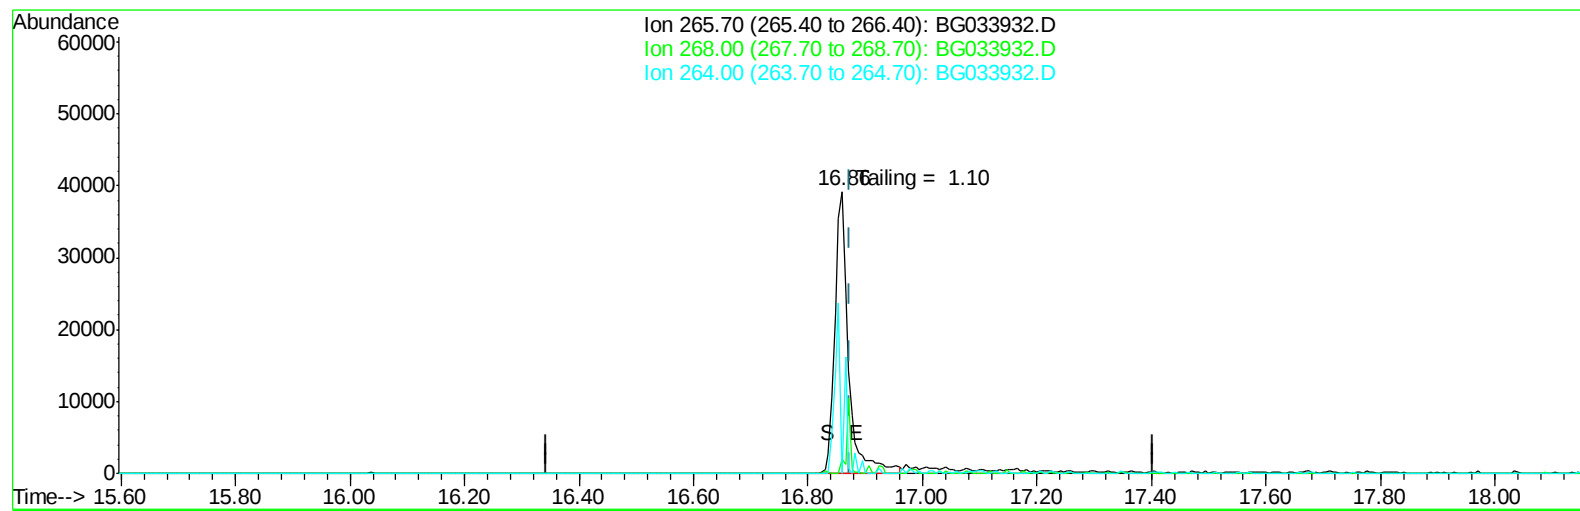

TIC: BG033932.D

(69) Pentachlorophenol (C)




16.859min (-0.014) 24444.59ng

response 64502

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	4.94#
264.00	62.00	4.08#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042318\
 Data File : BG033932.D
 Acq On : 23 Apr 2018 22:54
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 24 05:09:05 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 19 13:56:22 2018
 Response via : Initial Calibration

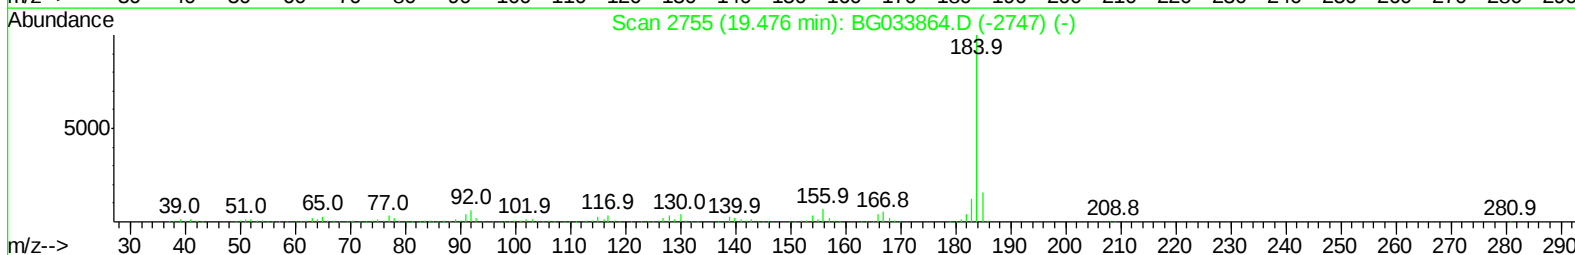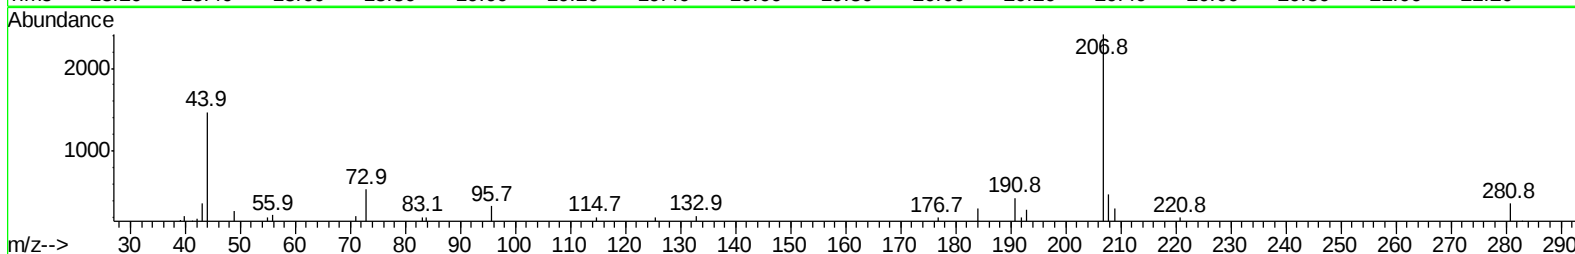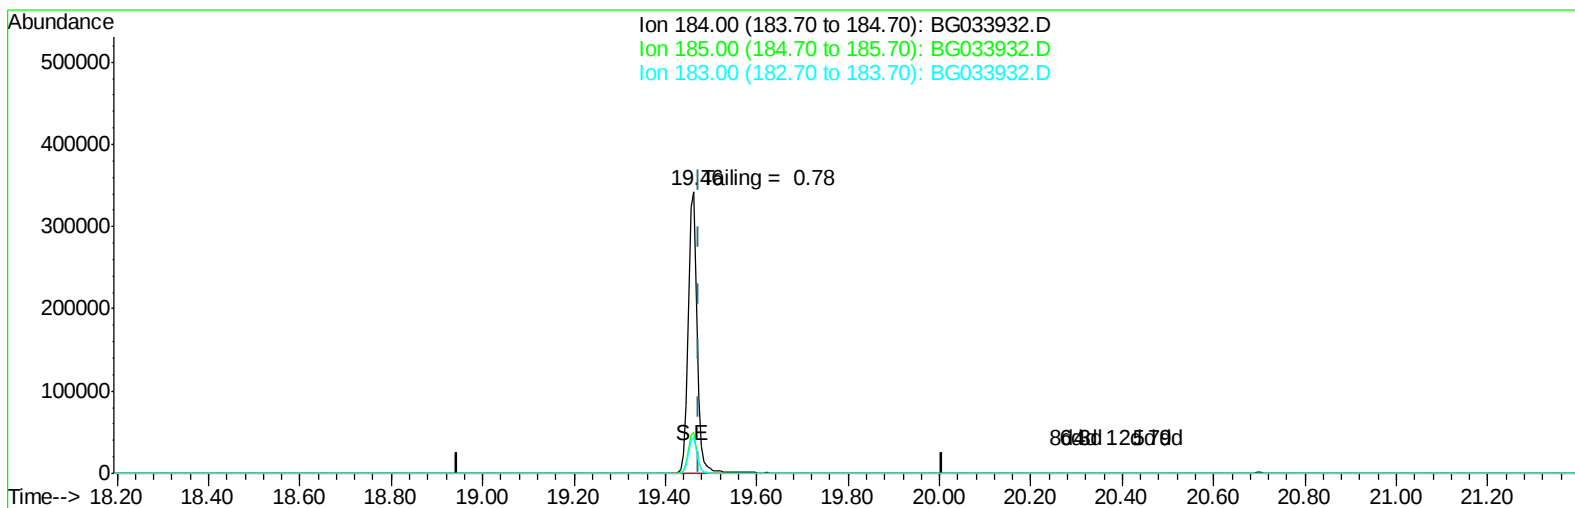

TIC: BG033932.D

(76) Benzidine

20.379min (+0.903) 170.35ng

response 299

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	0.00#
183.00	13.30	0.00#
0.00	0.00	0.00