

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042318\
 Data File : BG033941.D
 Acq On : 24 Apr 2018 4:52
 Operator : SJ/JU
 Sample : J2495-04
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RS-RO-1-7-B

Quant Time: Apr 24 08:13:52 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 19 13:56:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	58602	20.00	ng	0.00
21) Naphthalene-d8	10.61	136	257450	20.00	ng	-0.02
38) Acenaphthene-d10	14.46	164	172710	20.00	ng	-0.02
63) Phenanthrene-d10	17.21	188	479373	20.00	ng	-0.01
75) Chrysene-d12	21.47	240	512201	20.00	ng	-0.03
86) Perylene-d12	24.52	264	492331	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	565045	153.94	ng	0.00
7) Phenol-d6	7.00	99	702572	131.23	ng	0.00
23) Nitrobenzene-d5	8.97	82	510713	112.89	ng	-0.01
41) 2,4,6-Tribromophenol	15.95	330	358012	177.68	ng	-0.02
44) 2-Fluorobiphenyl	13.08	172	1267585	107.82	ng	-0.02
78) Terphenyl-d14	19.85	244	2346257	102.91	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042318\
Data File : BG033941.D
Acq On : 24 Apr 2018 4:52
Operator : SJ/JU
Sample : J2495-04
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RS-RO-1-7-B

Quant Time: Apr 24 08:13:52 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

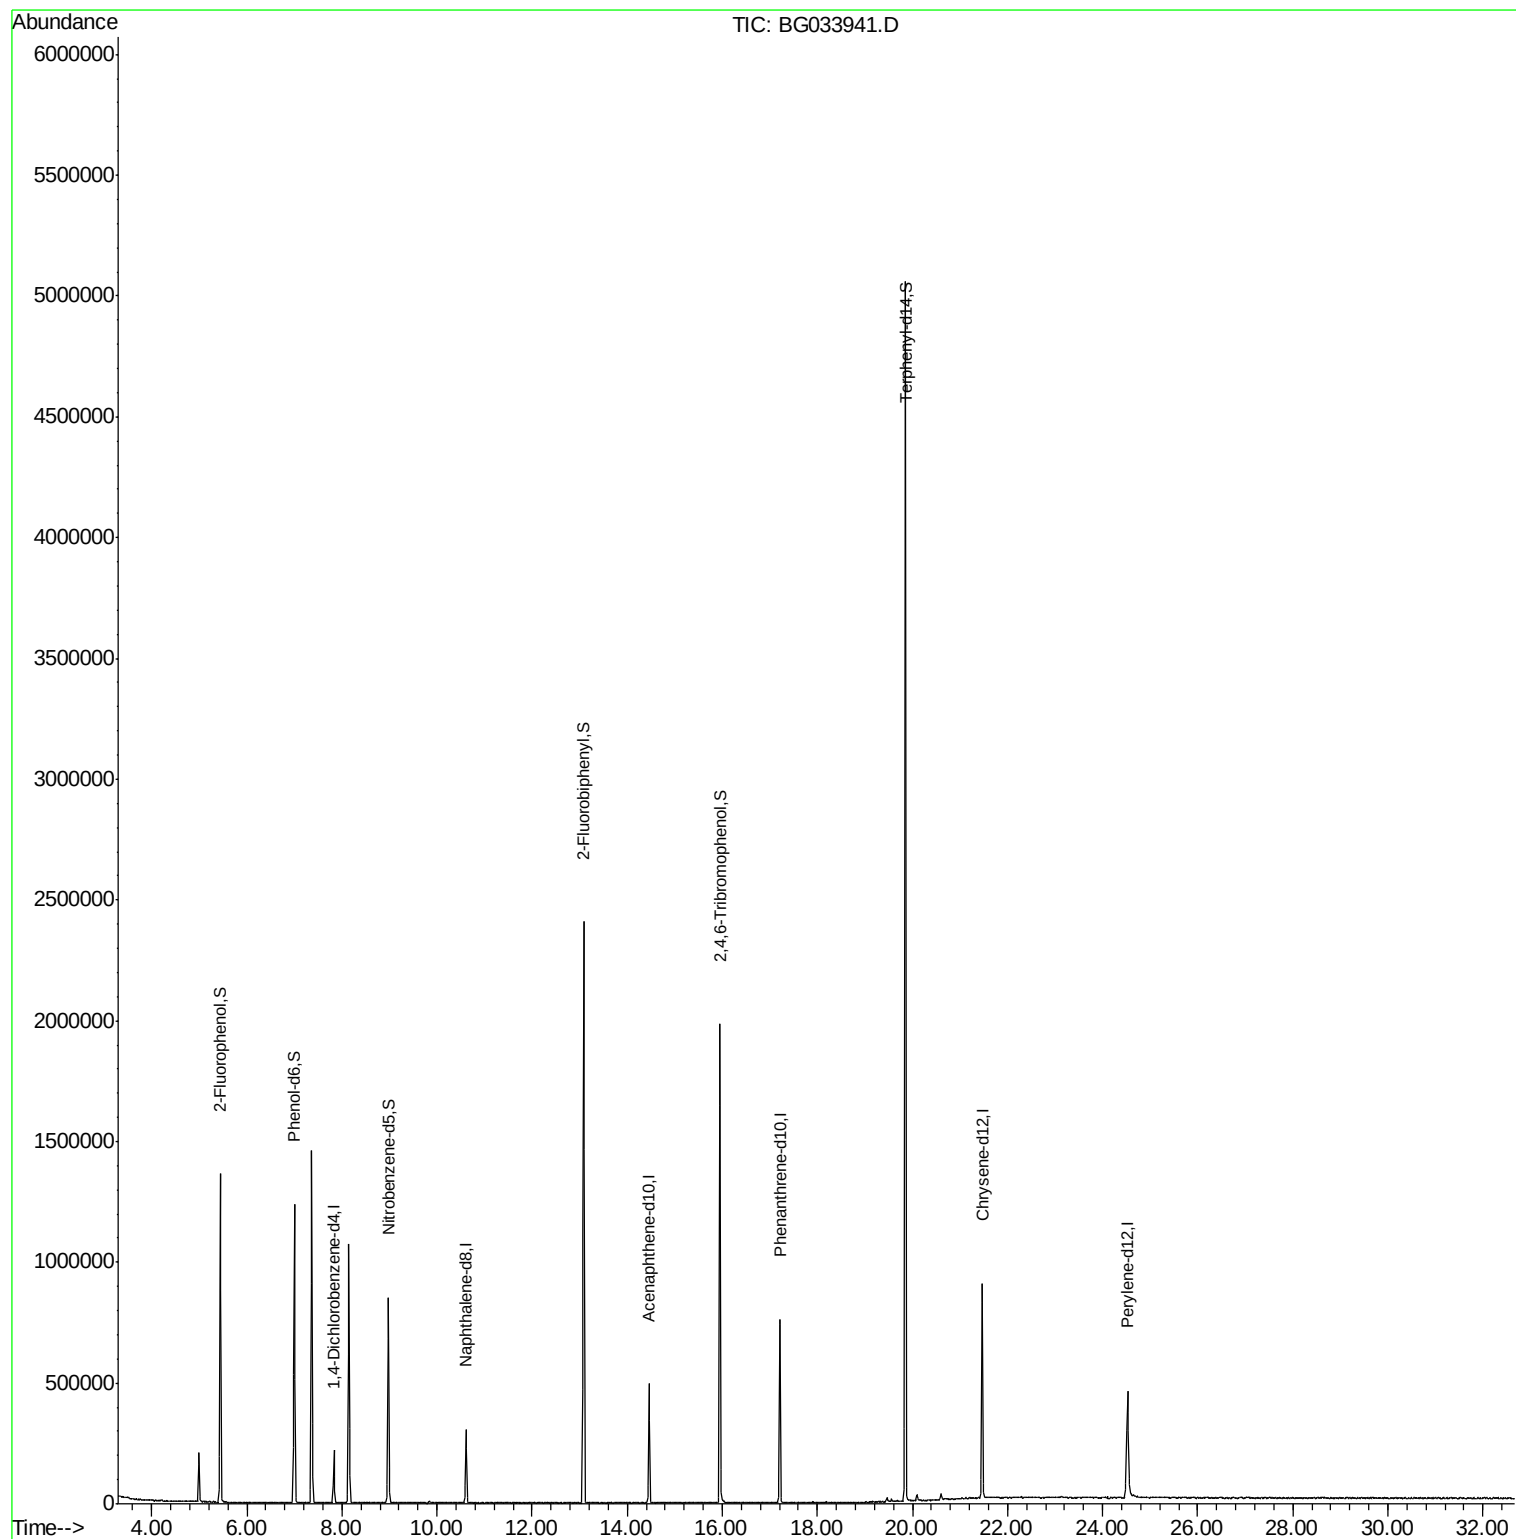

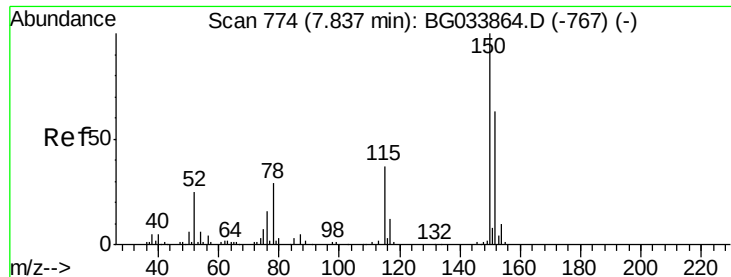


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.83 min Scan# 773
Delta R.T. -0.01 min
Lab File: BG033941.D
Acq: 24 Apr 2018 4:52

Instrument :
BNA_G
ClientSampleId :
RS-RO-1-7-B

Tot Ion	152	Resp	58602
Ion Ratio	Lower	Upper	
152	100		
150	157.2	126.6	189.8
115	60.0	53.0	79.4

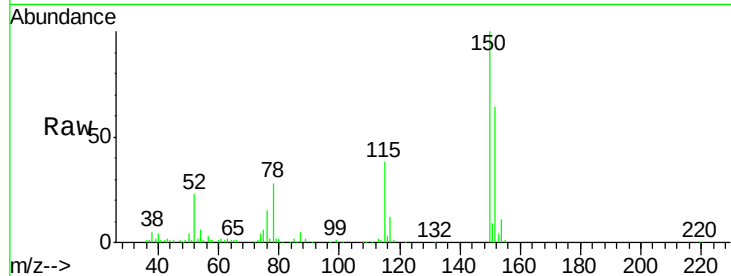


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

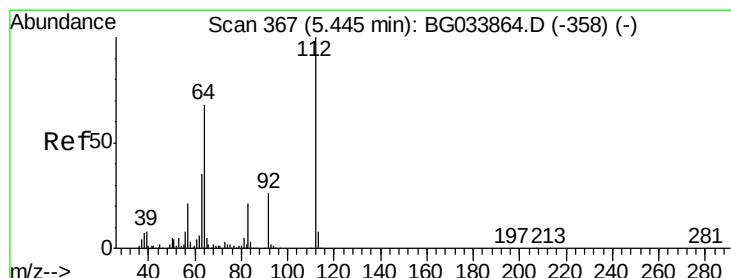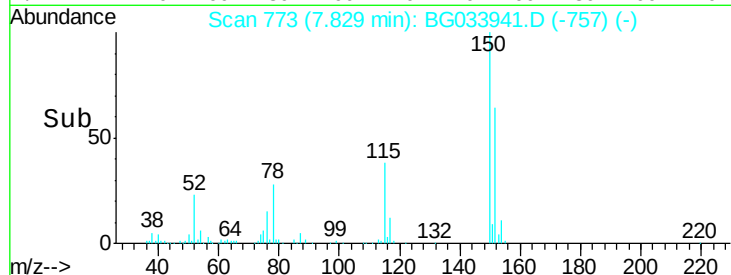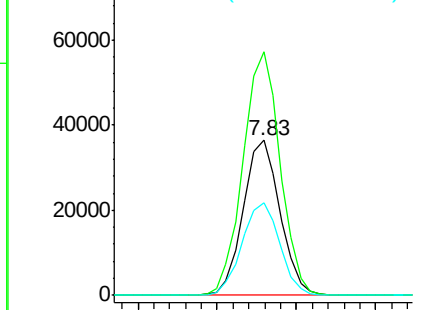



#5


2-Fluorophenol
Concen: 153.939 ng
RT: 5.44 min Scan# 367
Delta R.T. -0.00 min
Lab File: BG033941.D
Acq: 24 Apr 2018 4:52

Tgt Ion	112	Resp	565045
Ion Ratio	Lower	Upper	
112	100		
64	65.5	56.3	84.5
63	33.7	30.1	45.1

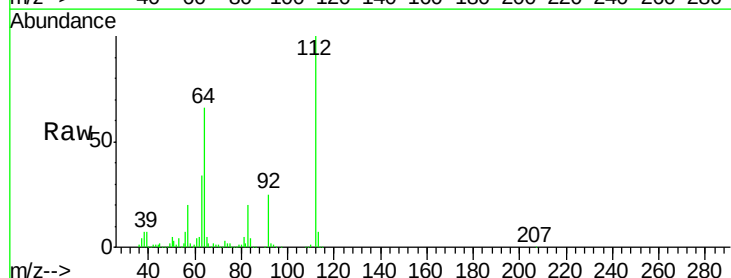

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

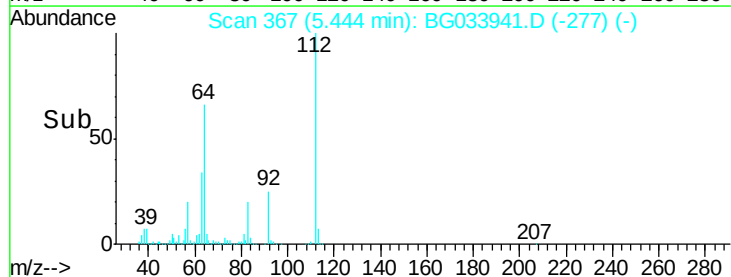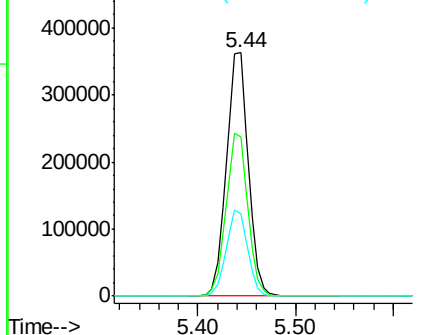

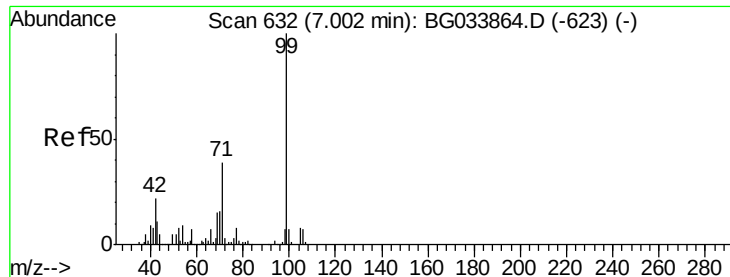

#7

Phenol-d6

Concen: 131.230 ng

RT: 7.00 min Scan# 632

Delta R.T. -0.00 min

Lab File: BG033941.D

Acq: 24 Apr 2018 4:52

Instrument :

BNA_G

ClientSampleId :

RS-RO-1-7-B


Tot Ion: 99 Resp: 702572

Ion Ratio Lower Upper




99 100

42 20.3 14.1 21.1

71 37.2 26.1 39.1

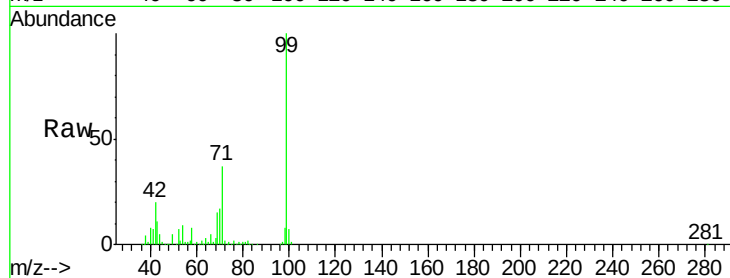

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

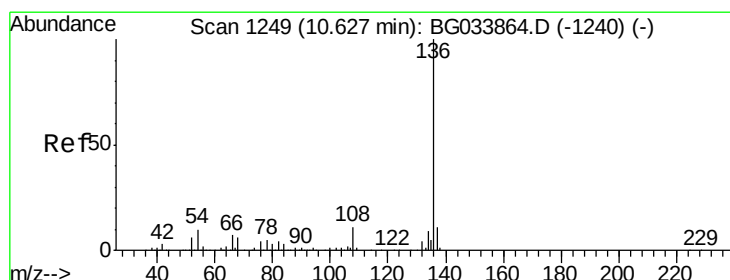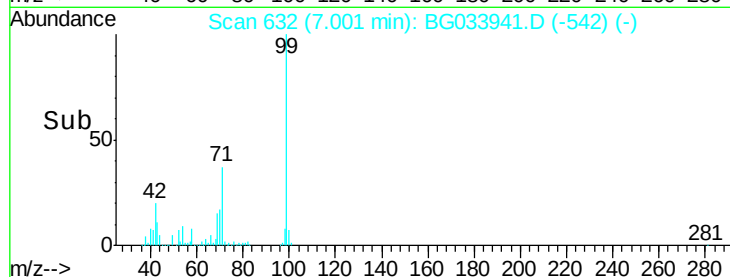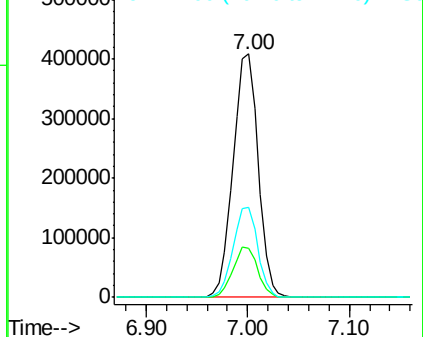

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.61 min Scan# 1246

Delta R.T. -0.02 min

Lab File: BG033941.D

Acq: 24 Apr 2018 4:52

Tgt Ion: 136 Resp: 257450


Ion Ratio Lower Upper

136 100



137 12.2 9.2 13.8


54 8.9 10.3 15.5#

68 6.1 4.5 6.7

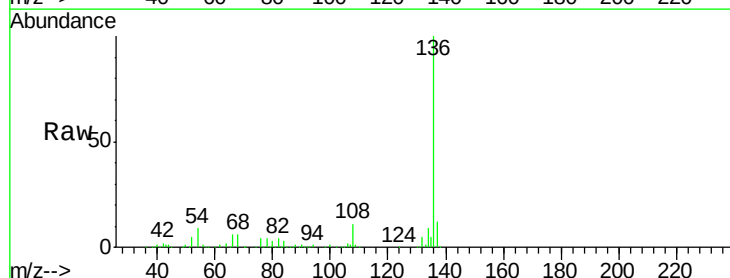

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



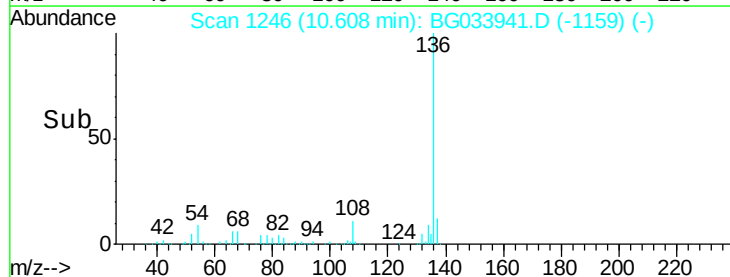
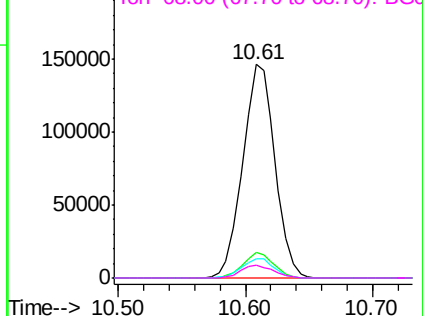


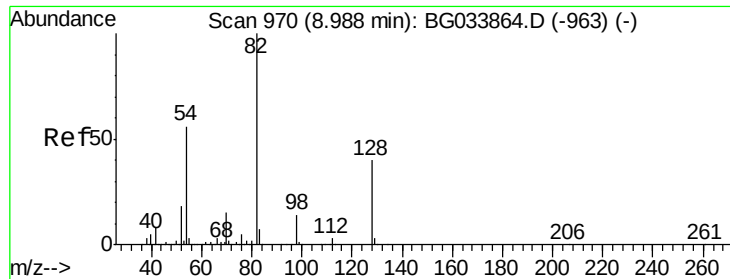

#23
 Nitrobenzene-d5
 Concen: 112.894 ng
 RT: 8.97 min Scan# 968
 Delta R.T. -0.01 min
 Lab File: BG033941.D
 Acq: 24 Apr 2018 4:52




Instrument :
 BNA_G
 ClientSampleId :
 RS-RO-1-7-B


Tot Ion	82	Resp	510713
Ion	Ratio	Lower	Upper
82	100		
128	40.4	29.7	44.5
54	54.1	43.1	64.7

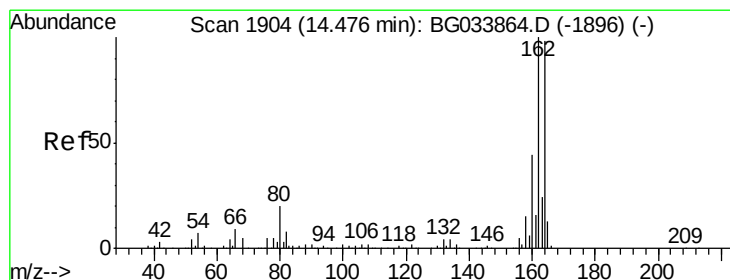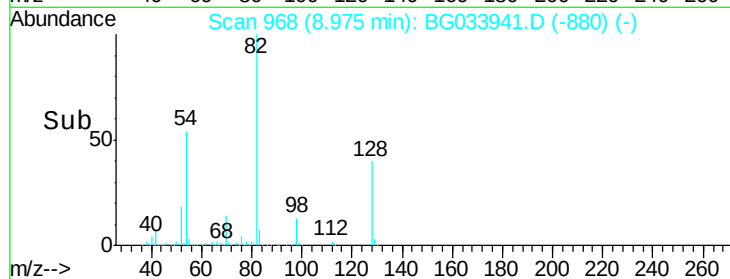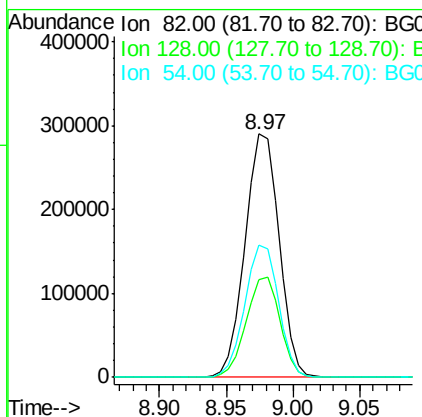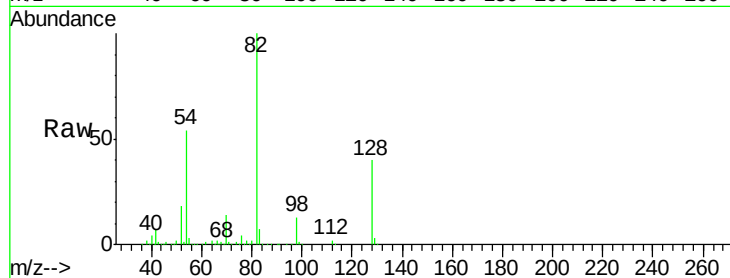

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.46 min Scan# 1901
 Delta R.T. -0.02 min
 Lab File: BG033941.D
 Acq: 24 Apr 2018 4:52

Tgt Ion	164	Resp	172710
Ion	Ratio	Lower	Upper
164	100		
162	103.0	78.8	118.2
160	42.2	35.4	53.0

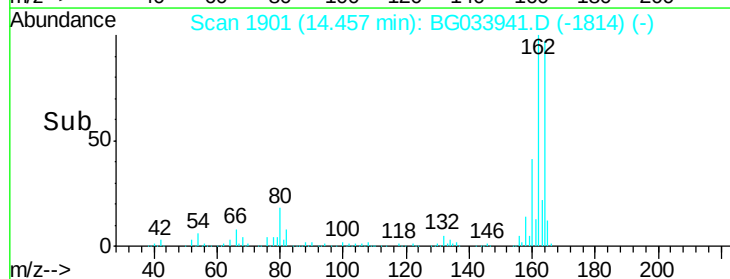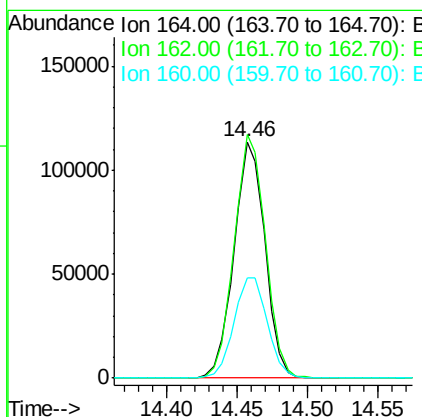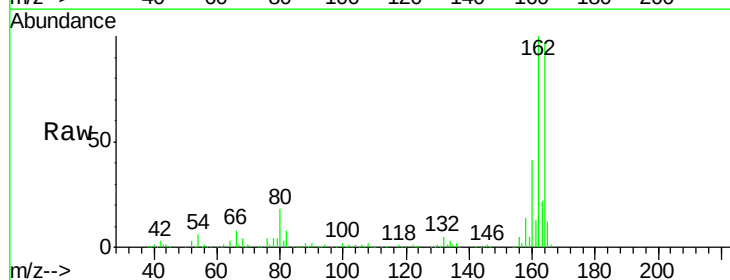


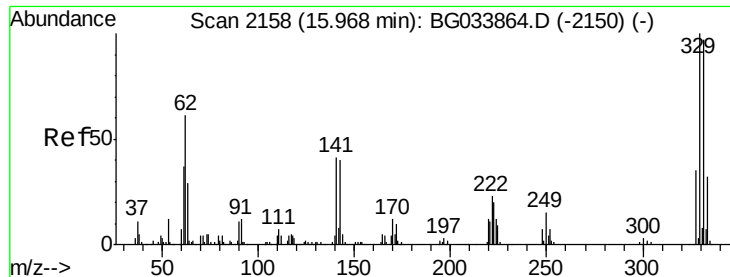




#41
 2,4,6-Tribromophenol
 Concen: 177.679 ng
 RT: 15.95 min Scan# 2155
 Delta R.T. -0.02 min
 Lab File: BG033941.D
 Acq: 24 Apr 2018 4:52

Instrument :
 BNA_G
 ClientSampleId :
 RS-RO-1-7-B

Tot Ion:330 Resp: 358012
 Ion Ratio Lower Upper
 330 100
 332 95.8 77.0 115.6
 141 39.1 25.2 37.8#

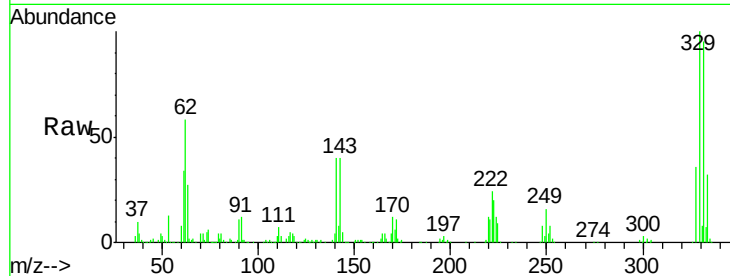


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

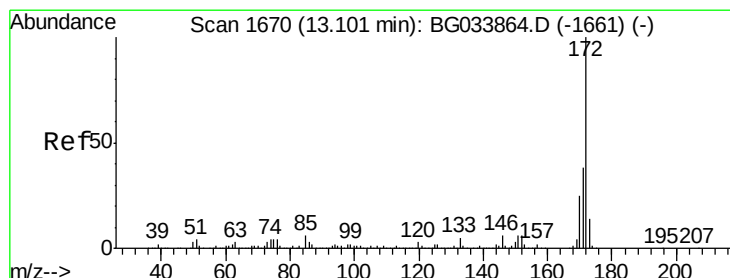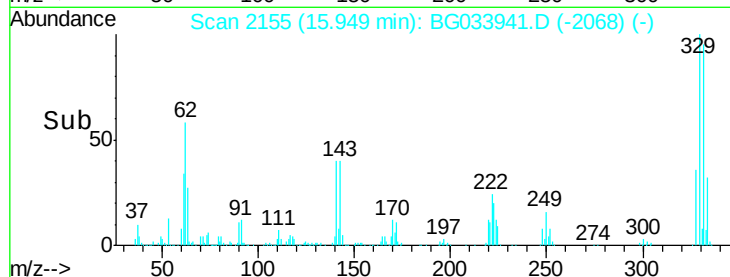
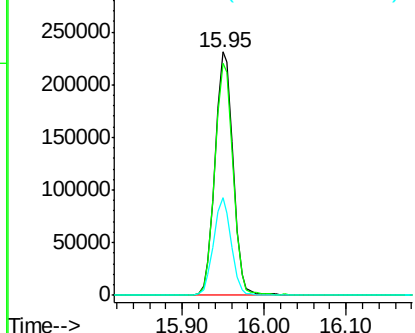



#44
 2-Fluorobiphenyl
 Concen: 107.817 ng
 RT: 13.08 min Scan# 1667
 Delta R.T. -0.02 min
 Lab File: BG033941.D
 Acq: 24 Apr 2018 4:52

Tgt Ion:172 Resp: 1267585
 Ion Ratio Lower Upper
 172 100
 171 38.3 30.0 45.0
 170 26.1 19.5 29.3

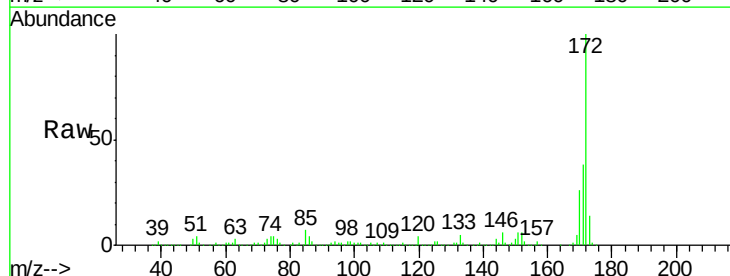

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

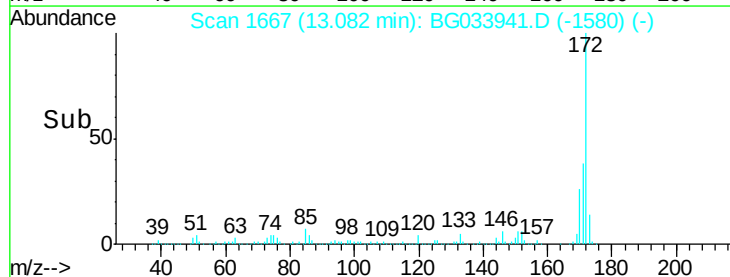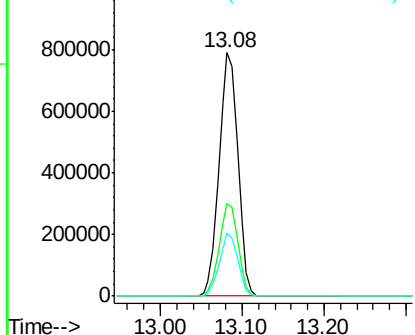


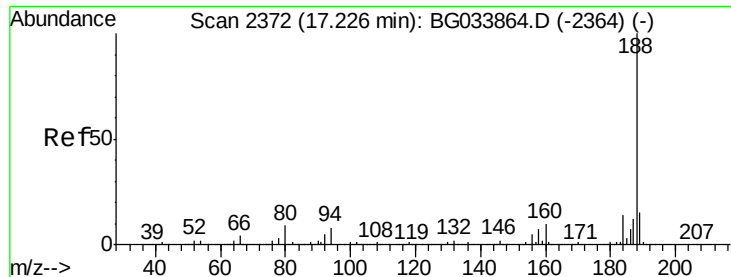




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.21 min Scan# 2370
Delta R.T. -0.01 min
Lab File: BG033941.D
Acq: 24 Apr 2018 4:52

Instrument :
BNA_G
ClientSampleId :
RS-RO-1-7-B

Tot Ion:188 Resp: 479373
Ion Ratio Lower Upper
188 100
94 7.5 6.9 10.3
80 8.8 7.7 11.5

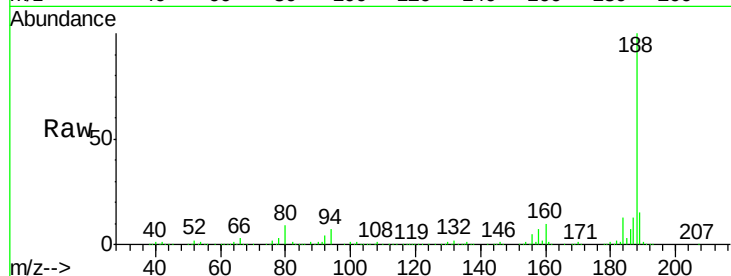


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

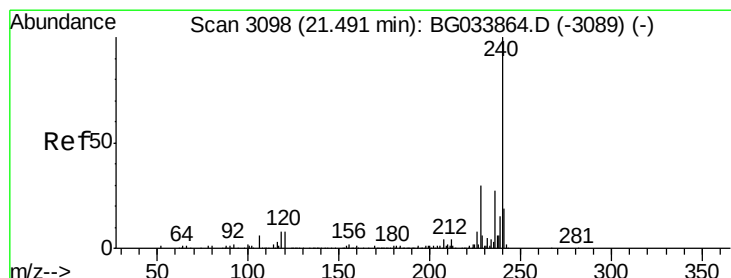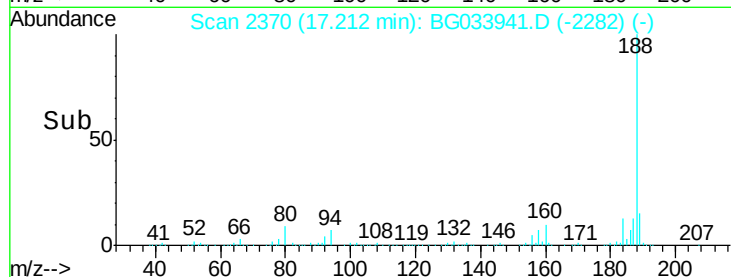
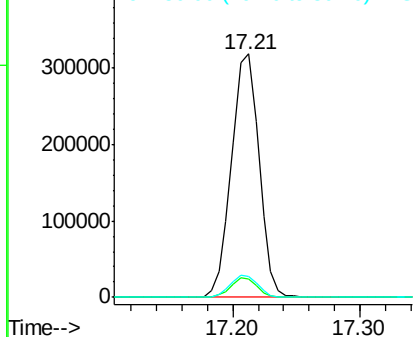



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.47 min Scan# 3094
Delta R.T. -0.03 min
Lab File: BG033941.D
Acq: 24 Apr 2018 4:52

Tgt Ion:240 Resp: 512201
Ion Ratio Lower Upper
240 100
120 8.8 6.8 10.2
236 26.6 20.9 31.3

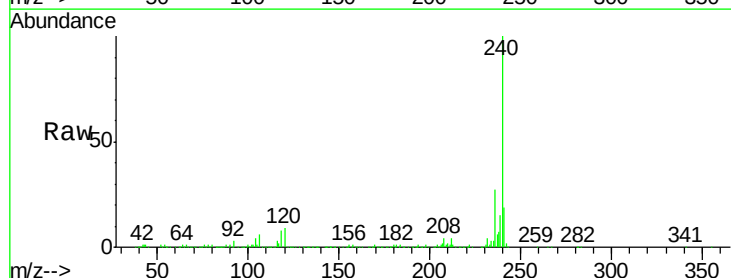

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

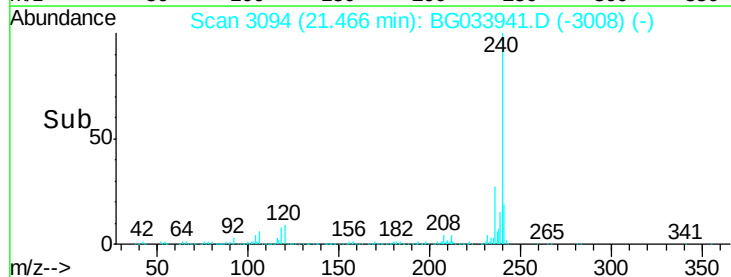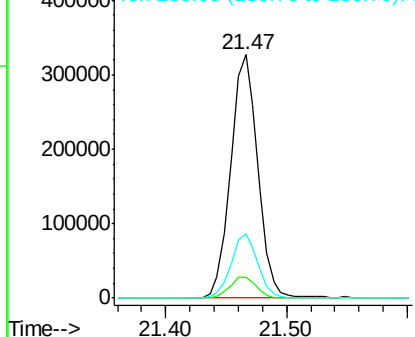

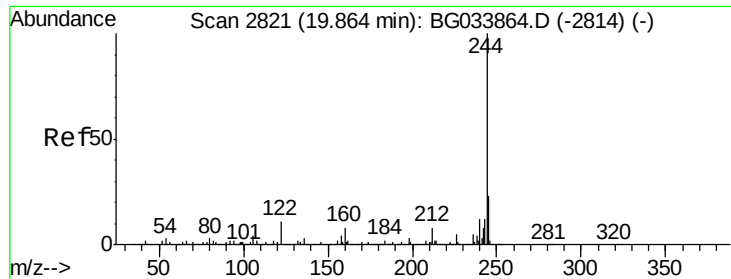

#78

Terphenyl-d14

Concen: 102.911 ng

RT: 19.85 min Scan# 2819

Delta R.T. -0.01 min

Lab File: BG033941.D

Acq: 24 Apr 2018 4:52

Instrument :

BNA_G

ClientSampleId :

RS-RO-1-7-B


Tot Ion:244 Resp: 2346257

Ion Ratio Lower Upper

244 100

212 9.5 5.8 8.8#




122 10.9 7.0 10.4#

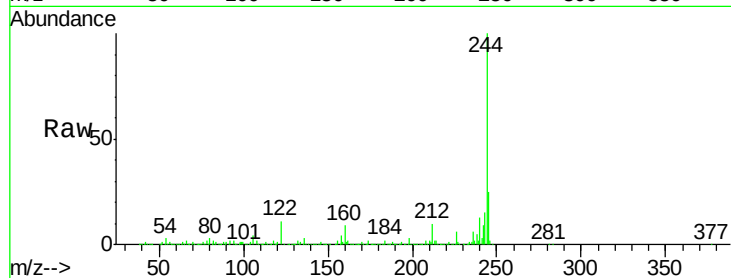

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

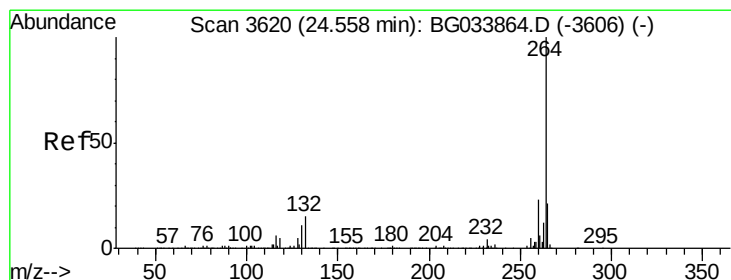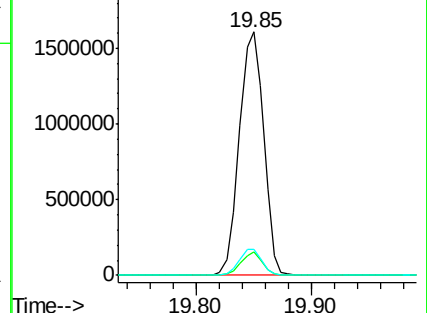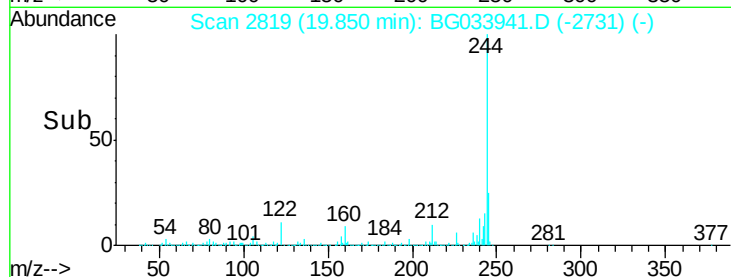

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.52 min Scan# 3614

Delta R.T. -0.04 min

Lab File: BG033941.D

Acq: 24 Apr 2018 4:52


Tgt Ion:264 Resp: 492331

Ion Ratio Lower Upper

264 100

260 23.9 17.4 26.0

265 21.5 17.7 26.5

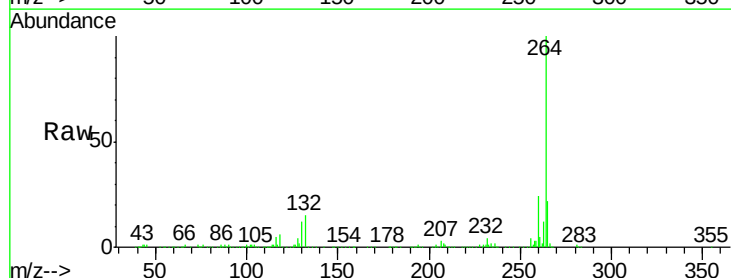

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

