

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042318\
 Data File : BG033942.D
 Acq On : 24 Apr 2018 5:29
 Operator : SJ/JU
 Sample : J2496-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RS-RO-1-3

Quant Time: Apr 24 08:15:29 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 19 13:56:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	63756	20.00	ng	0.00
21) Naphthalene-d8	10.61	136	274799	20.00	ng	-0.01
38) Acenaphthene-d10	14.46	164	184836	20.00	ng	-0.01
63) Phenanthrene-d10	17.21	188	519889	20.00	ng	-0.02
75) Chrysene-d12	21.46	240	564711	20.00	ng	-0.03
86) Perylene-d12	24.53	264	546375	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	554503	138.85	ng	0.00
7) Phenol-d6	7.00	99	680156	116.77	ng	0.00
23) Nitrobenzene-d5	8.98	82	497598	103.05	ng	0.00
41) 2,4,6-Tribromophenol	15.95	330	353816	164.08	ng	-0.01
44) 2-Fluorobiphenyl	13.09	172	1230466	97.79	ng	-0.01
78) Terphenyl-d14	19.85	244	2334848	92.89	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042318\
Data File : BG033942.D
Acq On : 24 Apr 2018 5:29
Operator : SJ/JU
Sample : J2496-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RS-RO-1-3

Quant Time: Apr 24 08:15:29 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

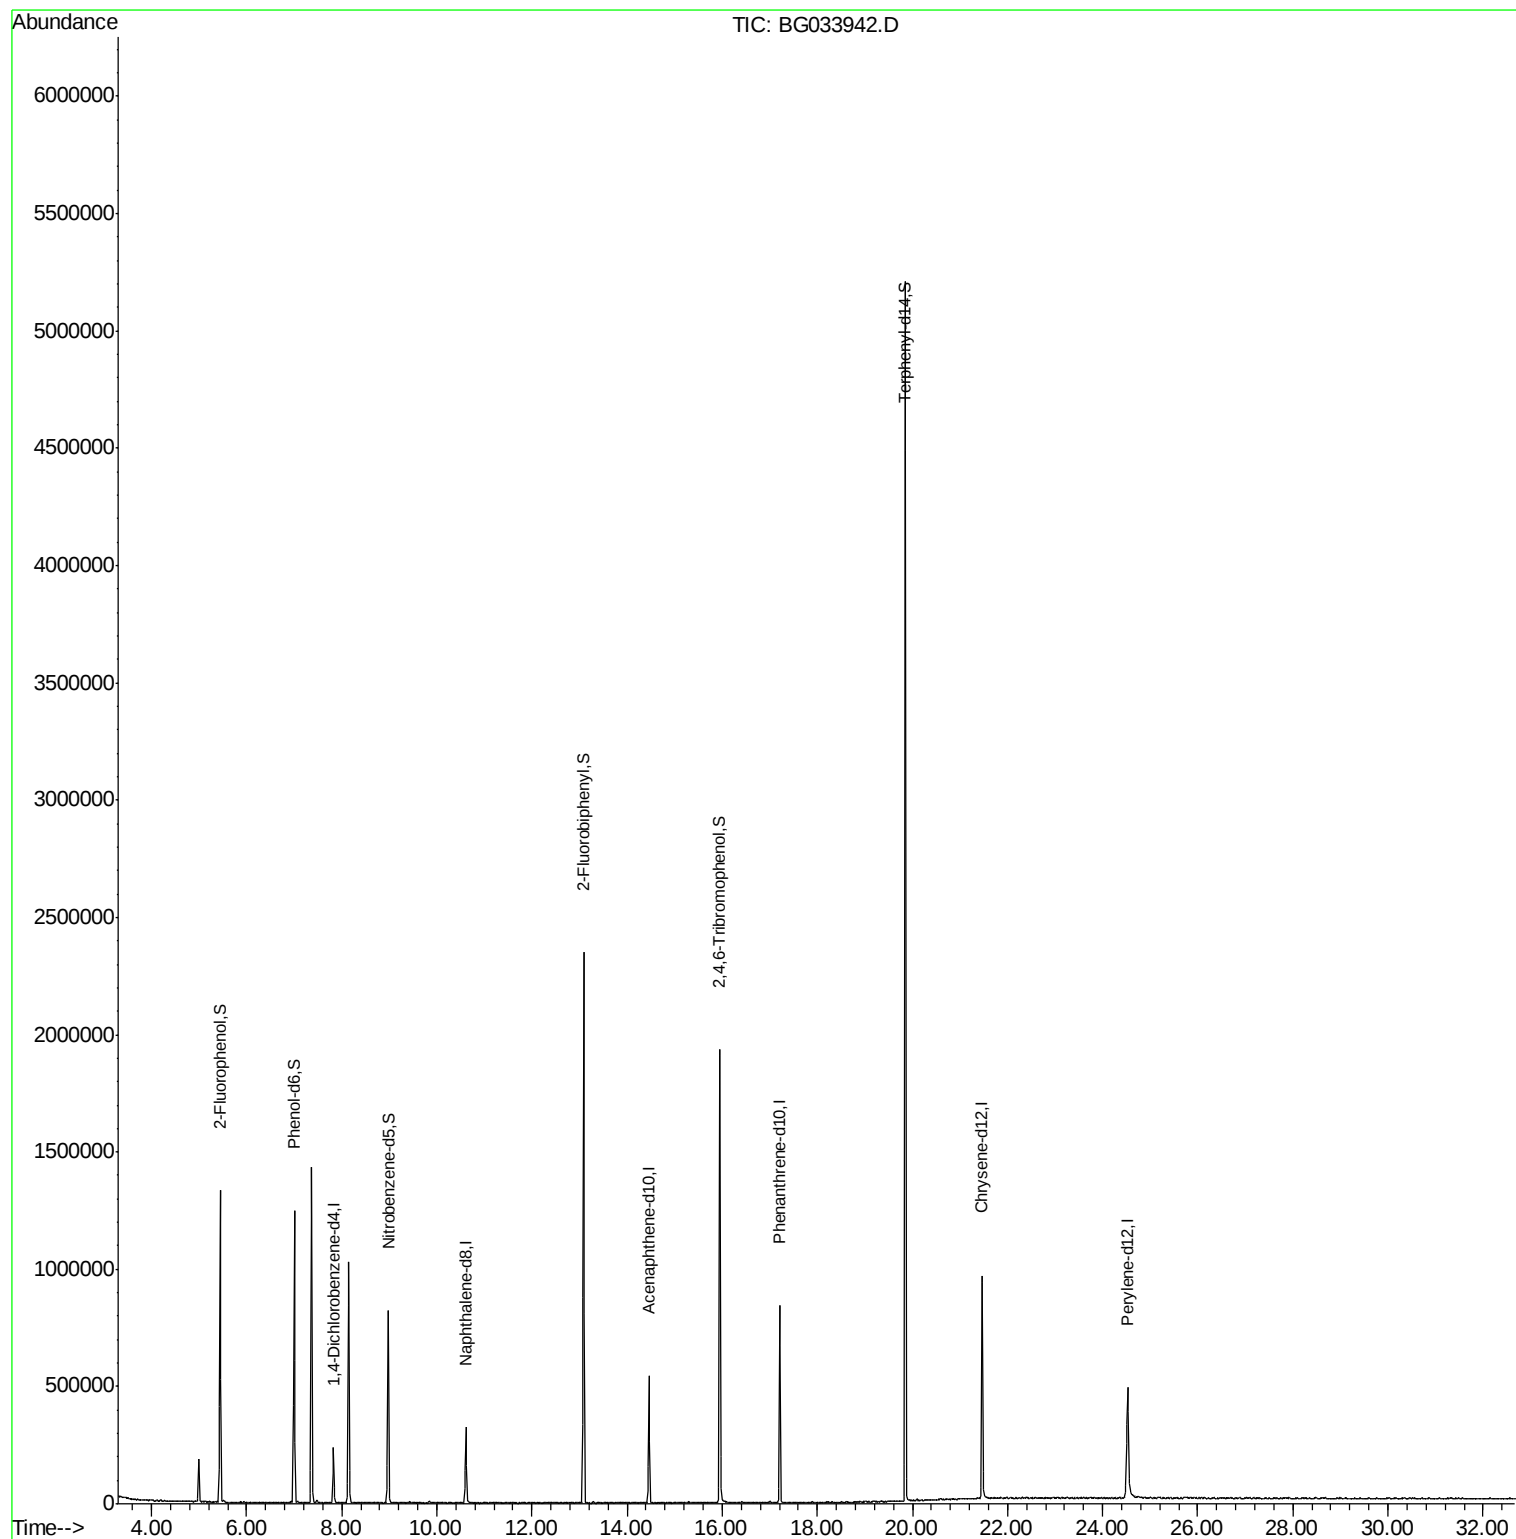

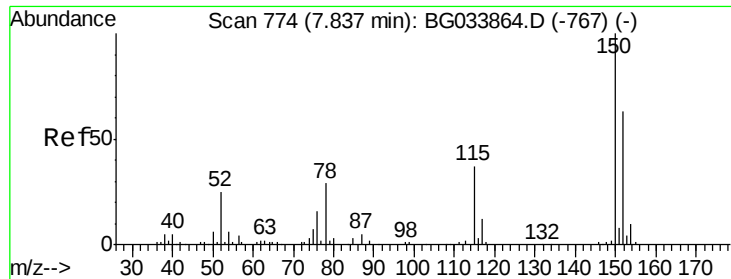


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.83 min Scan# 772
Delta R.T. -0.01 min
Lab File: BG033942.D
Acq: 24 Apr 2018 5:29

Instrument :
BNA_G
ClientSampleId :
RS-RO-1-3

Tot Ion	Ratio	Lower	Upper
152	100		
150	160.4	126.6	189.8
115	60.2	53.0	79.4

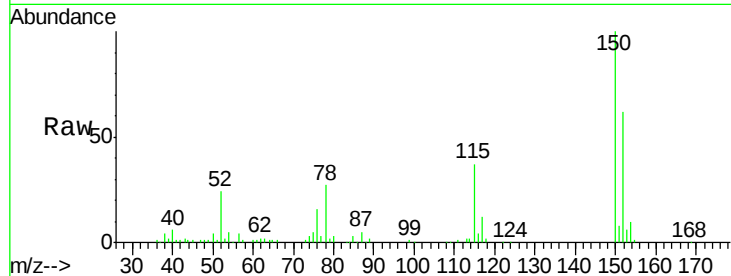


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

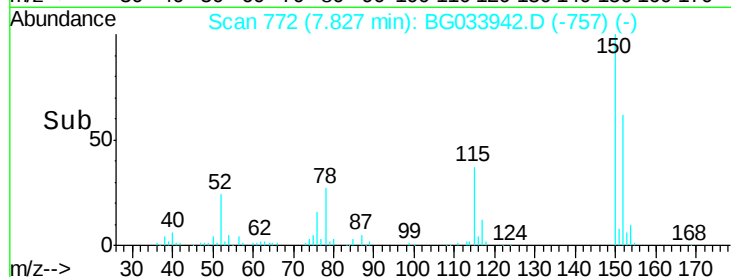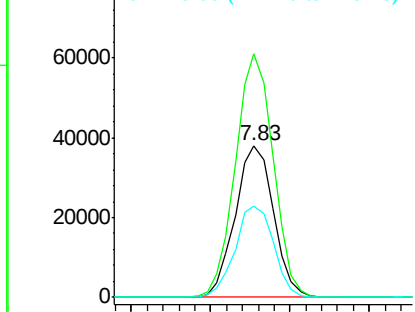



#5


2-Fluorophenol
Concen: 138.855 ng
RT: 5.44 min Scan# 366
Delta R.T. -0.00 min
Lab File: BG033942.D
Acq: 24 Apr 2018 5:29

Tgt Ion	Ratio	Lower	Upper
112	100		
64	65.9	56.3	84.5
63	34.3	30.1	45.1

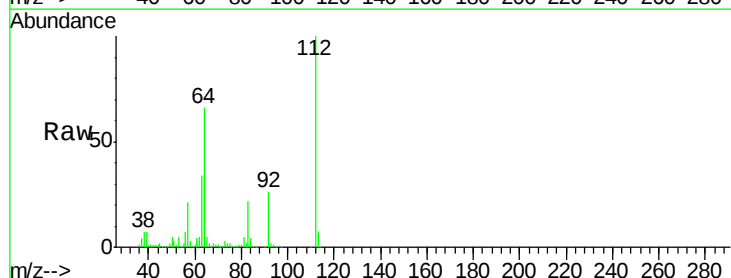

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

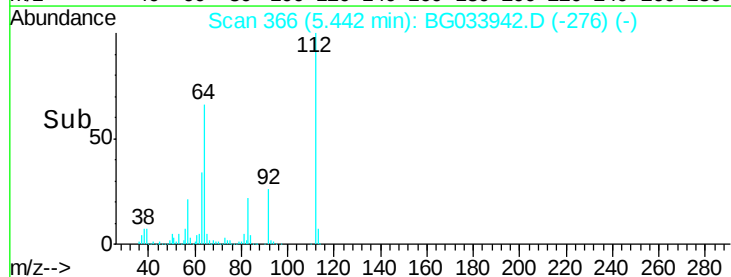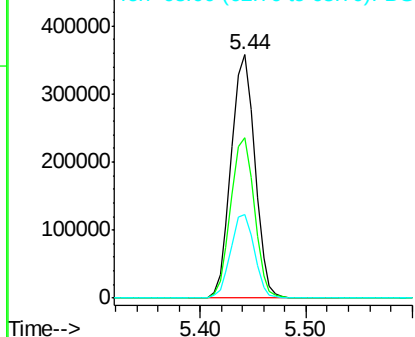

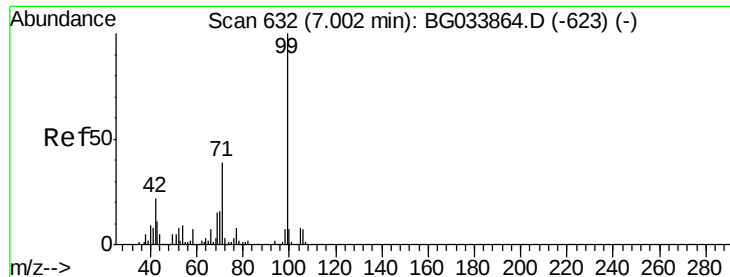

#7

Phenol-d6

Concen: 116.773 ng

RT: 7.00 min Scan# 631

Delta R.T. -0.00 min

Lab File: BG033942.D

Acq: 24 Apr 2018 5:29

Instrument :

BNA_G

ClientSampled :

RS-RO-1-3


Tot Ion: 99 Resp: 680156

Ion Ratio Lower Upper




99 100

42 20.2 14.1 21.1

71 37.0 26.1 39.1

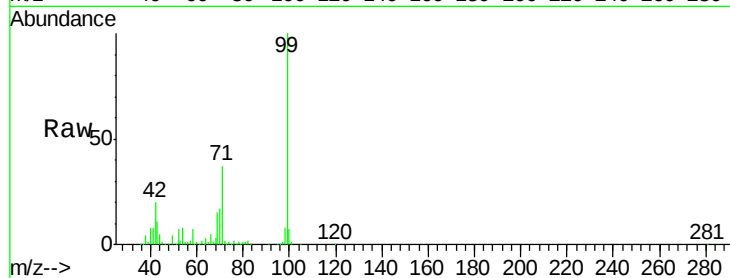

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

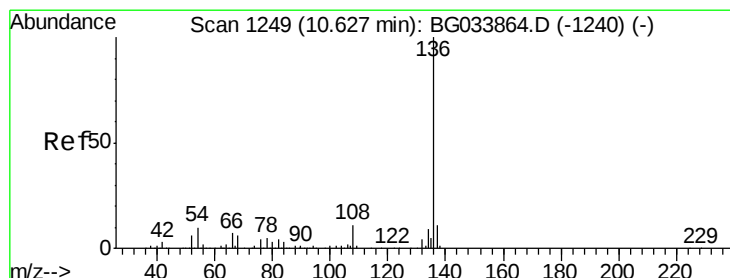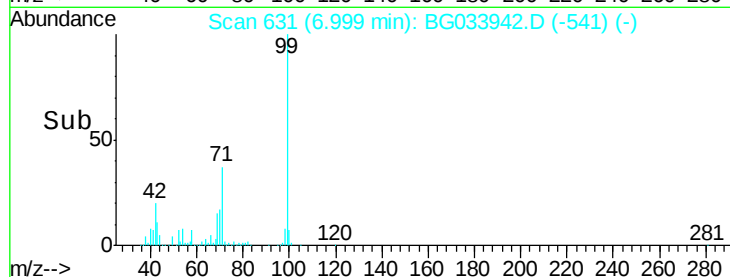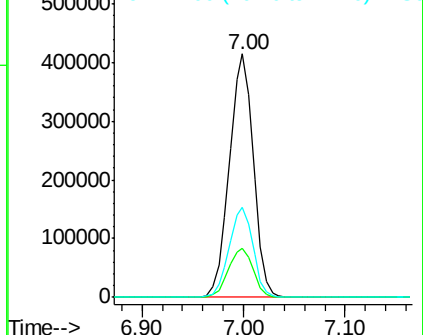

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.61 min Scan# 1246

Delta R.T. -0.01 min

Lab File: BG033942.D

Acq: 24 Apr 2018 5:29

Tgt Ion: 136 Resp: 274799


Ion Ratio Lower Upper

136 100



137 11.5 9.2 13.8


54 8.5 10.3 15.5#

68 5.8 4.5 6.7

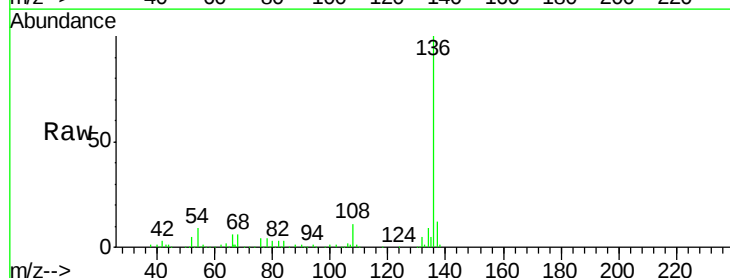

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



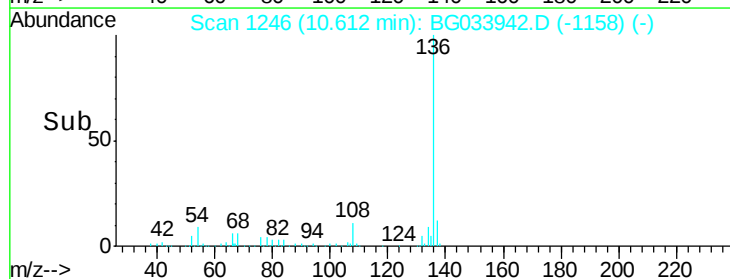
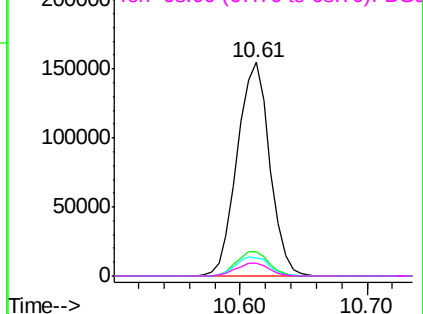


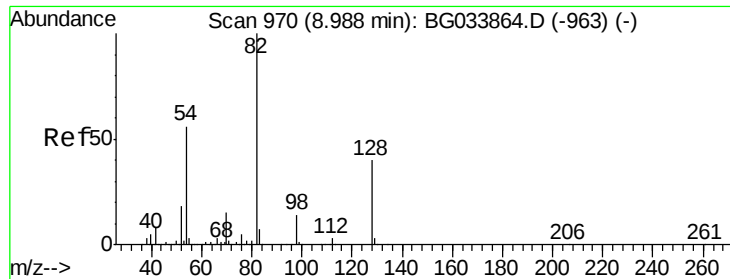

#23
 Nitrobenzene-d5
 Concen: 103.050 ng
 RT: 8.98 min Scan# 968
 Delta R.T. -0.01 min
 Lab File: BG033942.D
 Acq: 24 Apr 2018 5:29




Instrument :
 BNA_G
 ClientSampleId :
 RS-RO-1-3


Tot Ion	82	Resp	497598
Ion Ratio	Lower	Upper	
82	100		
128	41.1	29.7	44.5
54	54.3	43.1	64.7

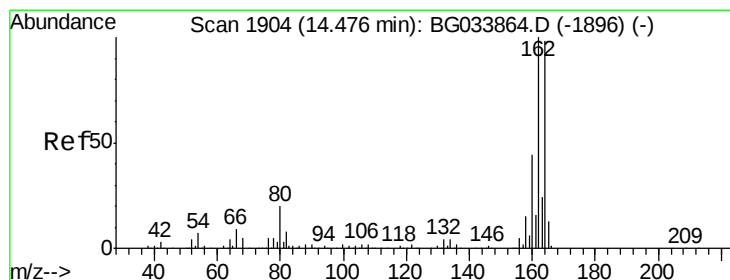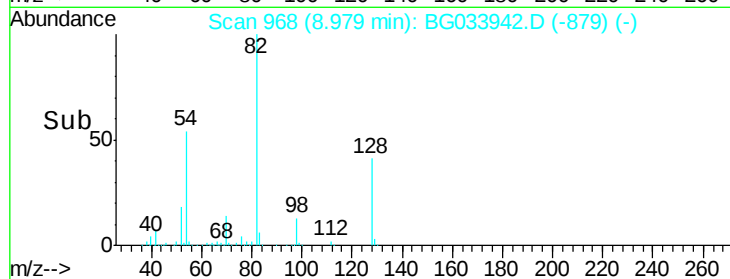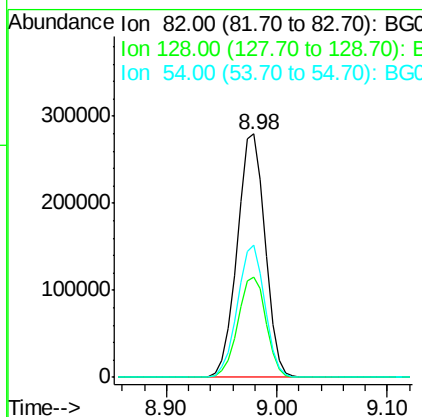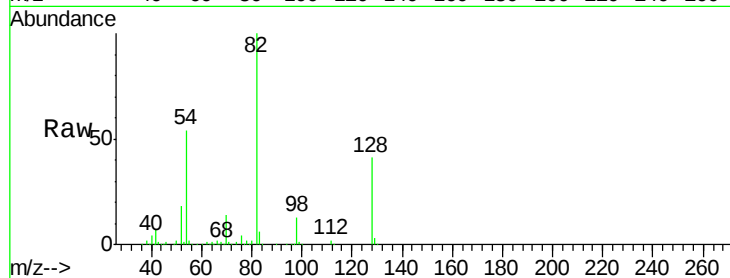

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.46 min Scan# 1901
 Delta R.T. -0.01 min
 Lab File: BG033942.D
 Acq: 24 Apr 2018 5:29

Tgt Ion	164	Resp	184836
Ion Ratio	Lower	Upper	
164	100		
162	100.6	78.8	118.2
160	42.3	35.4	53.0

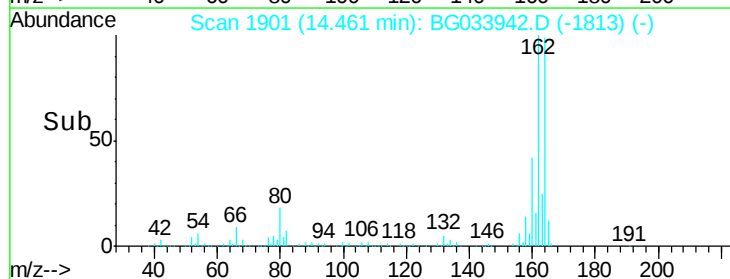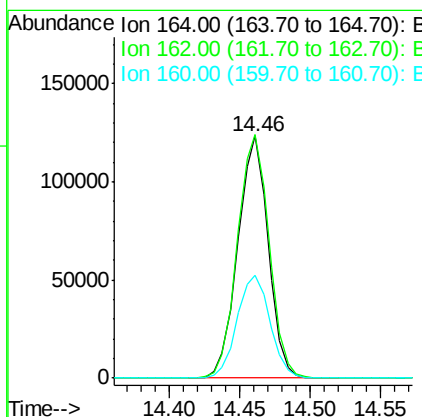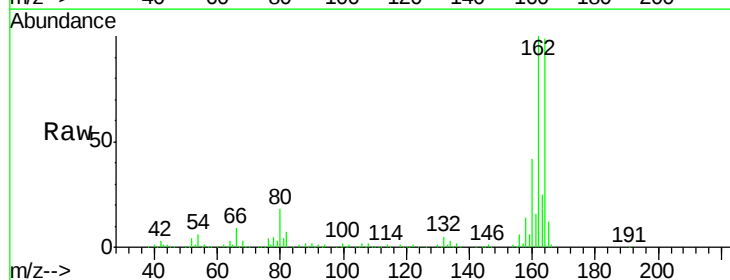


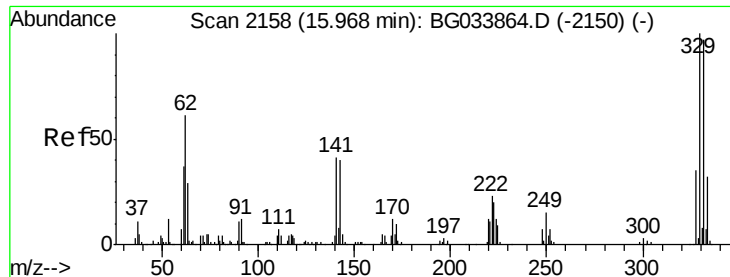




#41
 2,4,6-Tribromophenol
 Concen: 164.077 ng
 RT: 15.95 min Scan# 2155
 Delta R.T. -0.01 min
 Lab File: BG033942.D
 Acq: 24 Apr 2018 5:29

Instrument :
 BNA_G
 ClientSampleId :
 RS-RO-1-3

Tot Ion:330 Resp: 353816
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.0 115.6
 141 39.5 25.2 37.8#

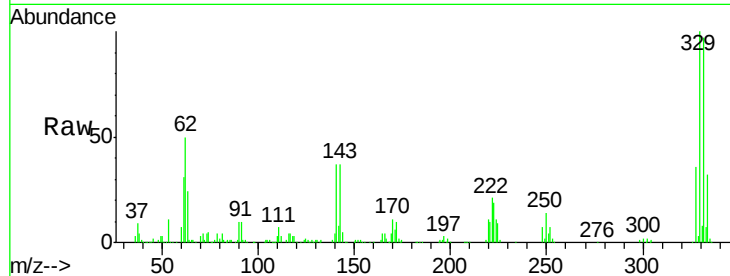


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

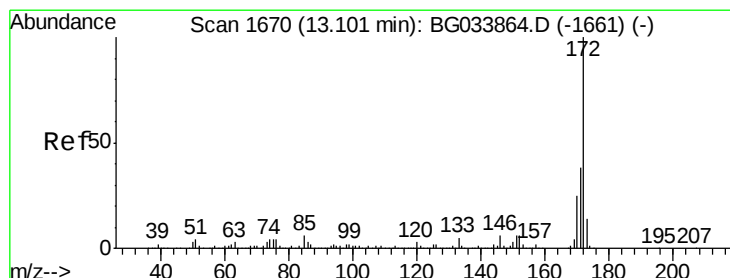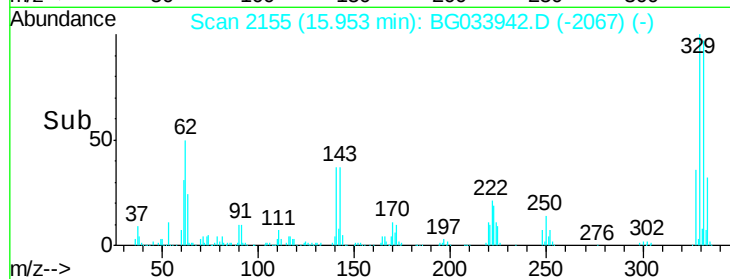
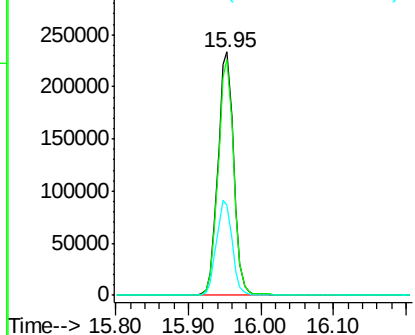



#44
 2-Fluorobiphenyl
 Concen: 97.794 ng
 RT: 13.09 min Scan# 1667
 Delta R.T. -0.01 min
 Lab File: BG033942.D
 Acq: 24 Apr 2018 5:29

Tgt Ion:172 Resp: 1230466
 Ion Ratio Lower Upper
 172 100
 171 38.2 30.0 45.0
 170 25.3 19.5 29.3

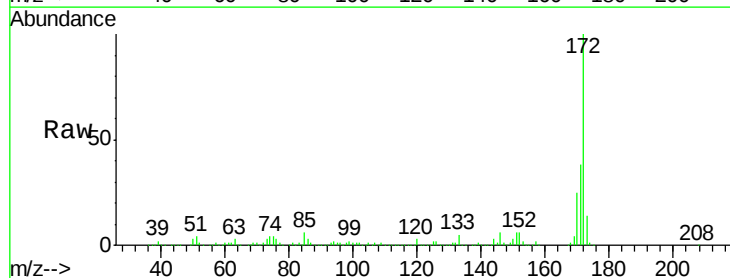

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



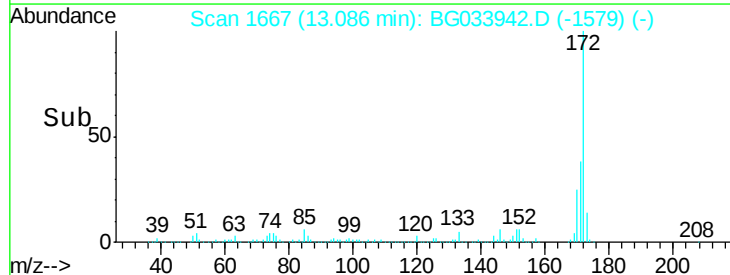
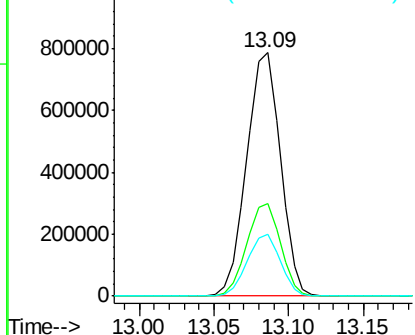


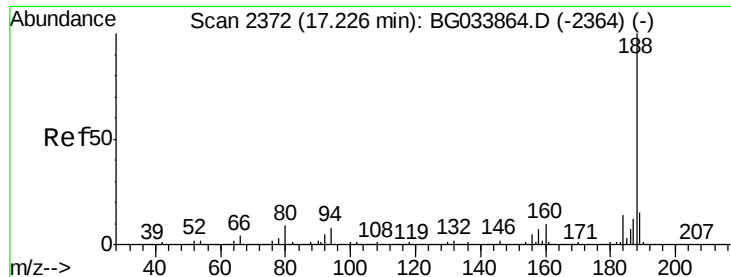

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.21 min Scan# 2369
Delta R.T. -0.02 min
Lab File: BG033942.D
Acq: 24 Apr 2018 5:29




Instrument :
BNA_G
ClientSampleId :
RS-RO-1-3


Tot Ion	Ratio	Lower	Upper
188	100		
94	7.7	6.9	10.3
80	8.9	7.7	11.5

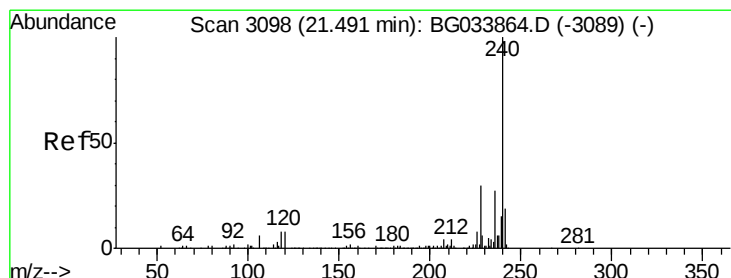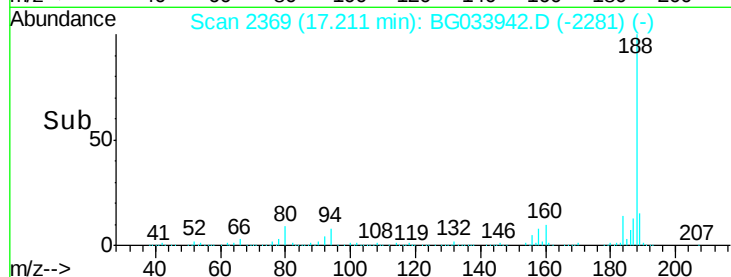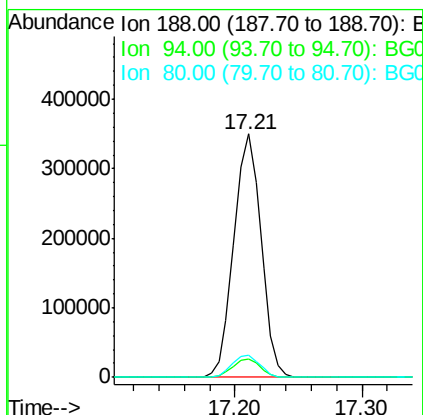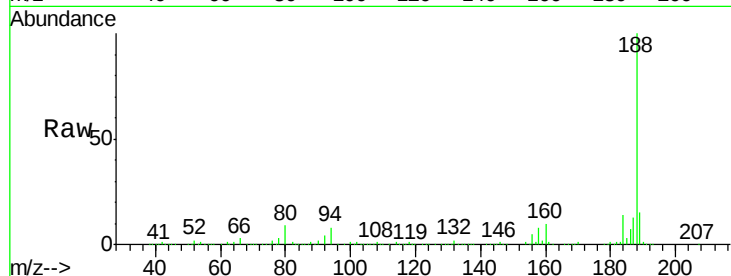

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.46 min Scan# 3093
Delta R.T. -0.03 min
Lab File: BG033942.D
Acq: 24 Apr 2018 5:29

Tgt Ion	Ratio	Lower	Upper
240	100		
120	8.9	6.8	10.2
236	26.1	20.9	31.3

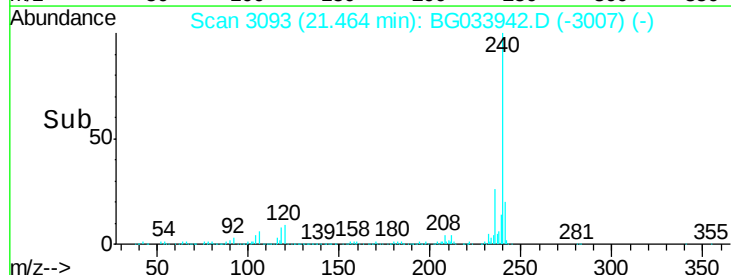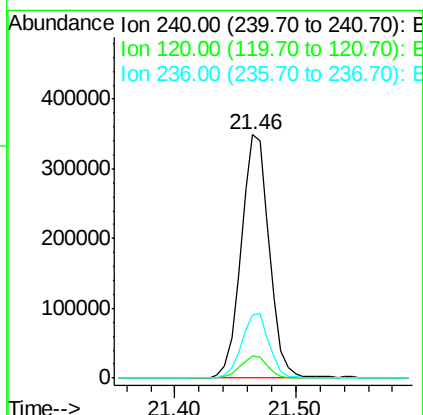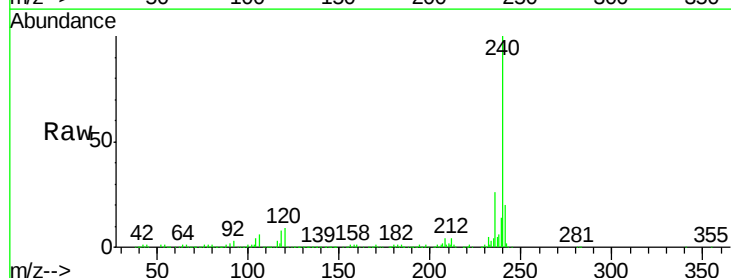

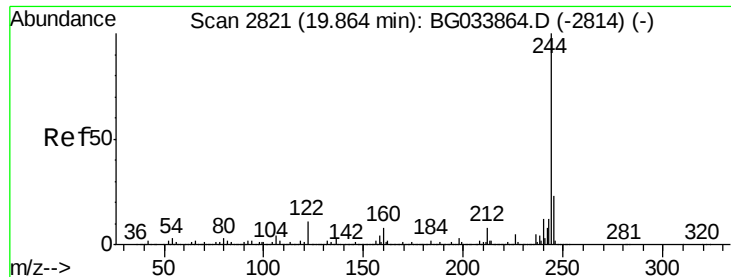

#78

Terphenyl-d14

Concen: 92.888 ng

RT: 19.85 min Scan# 2818

Delta R.T. -0.01 min

Lab File: BG033942.D

Acq: 24 Apr 2018 5:29

Instrument :

BNA_G

ClientSampleId :

RS-RO-1-3


Tot Ion:244 Resp: 2334848

Ion Ratio Lower Upper

244 100

212 9.3 5.8 8.8#




122 11.2 7.0 10.4#

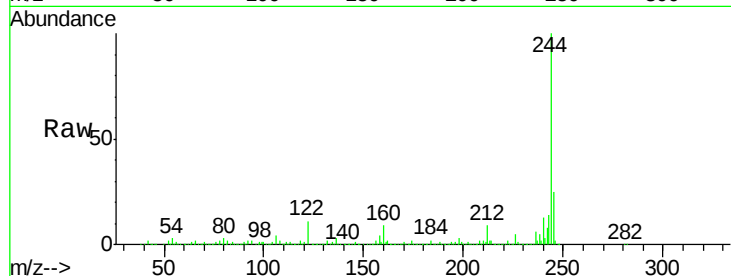

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

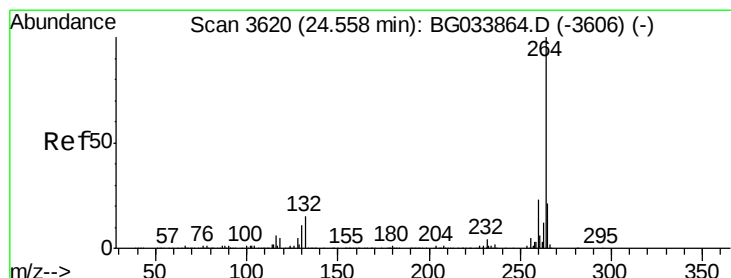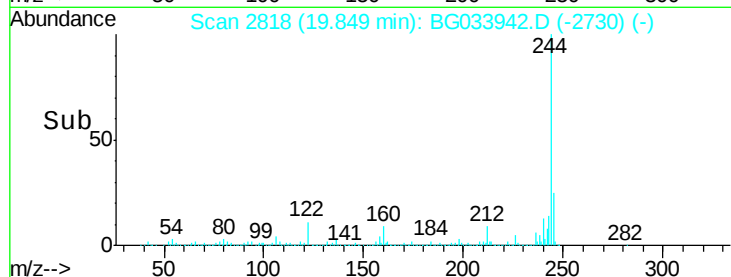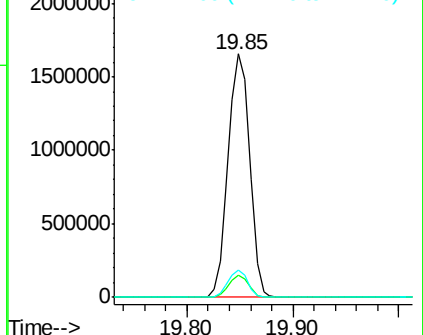

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.53 min Scan# 3614

Delta R.T. -0.03 min

Lab File: BG033942.D

Acq: 24 Apr 2018 5:29


Tgt Ion:264 Resp: 546375

Ion Ratio Lower Upper

264 100

260 23.7 17.4 26.0

265 22.0 17.7 26.5

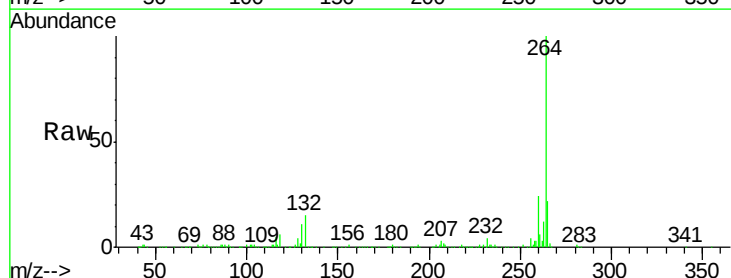

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

