


Data Path : Z:\HPCHEM1\BNA G\Data\BG042318\
 Data File : BG033914.D
 Acq On : 23 Apr 2018 10:01
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

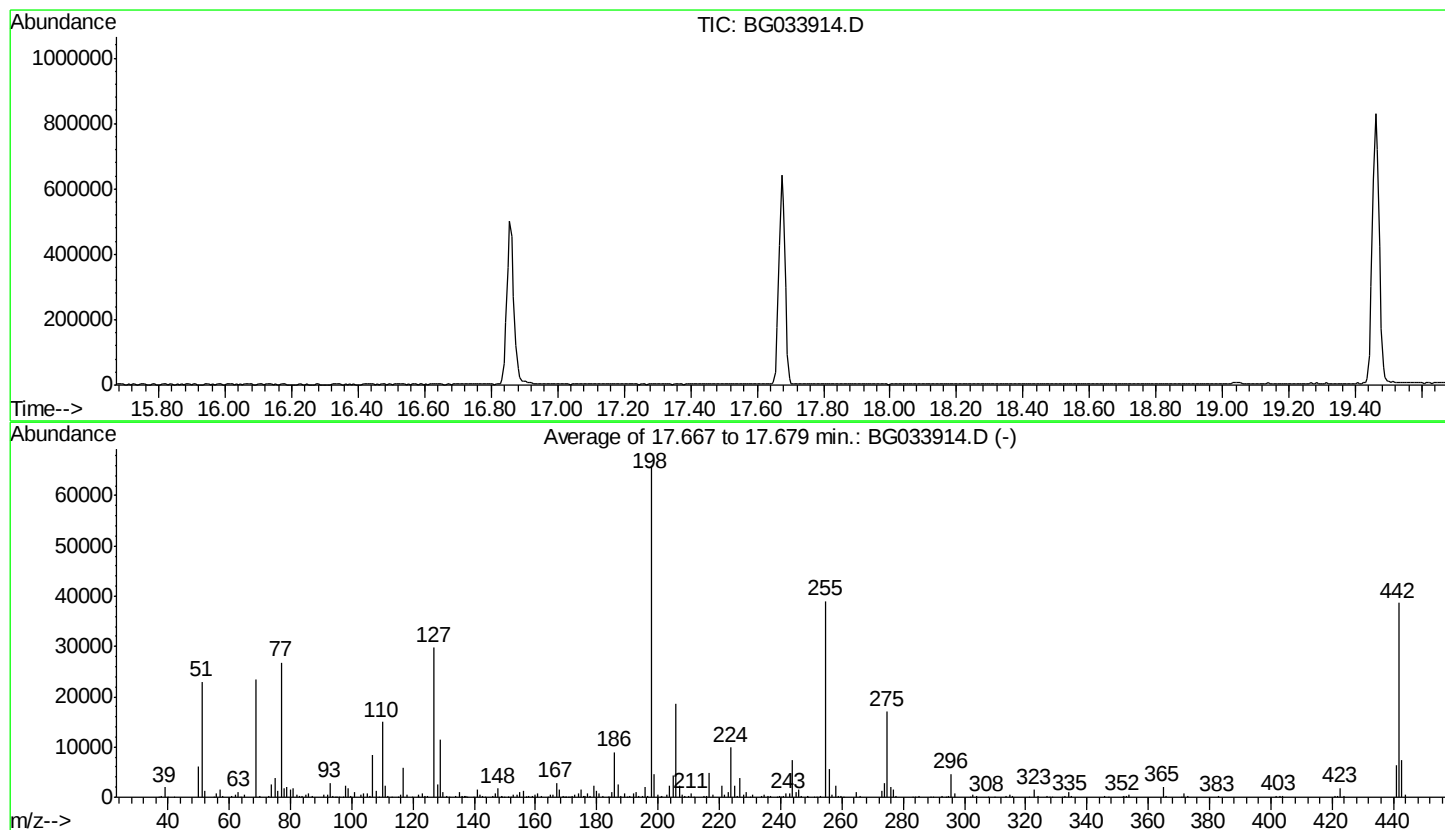

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	22941	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.3	23322	PASS
70	69	0.00	2	0.6	146	PASS
127	198	10	80	45.0	29685	PASS
197	198	0.00	2	0.5	300	PASS
198	198	100	100	100.0	65986	PASS
199	198	5	9	6.8	4512	PASS
275	198	10	60	25.8	17057	PASS
365	198	1	100	3.2	2119	PASS
441	443	0.01	100	87.9	6459	PASS
442	198	50	100	58.5	38600	PASS
443	442	15	24	19.0	7351	PASS