


Data Path : Z:\HPCHEM1\BNA G\Data\BG042318\
Data File : BG033932.D
Acq On : 23 Apr 2018 22:54
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 19 13:56:22 2018

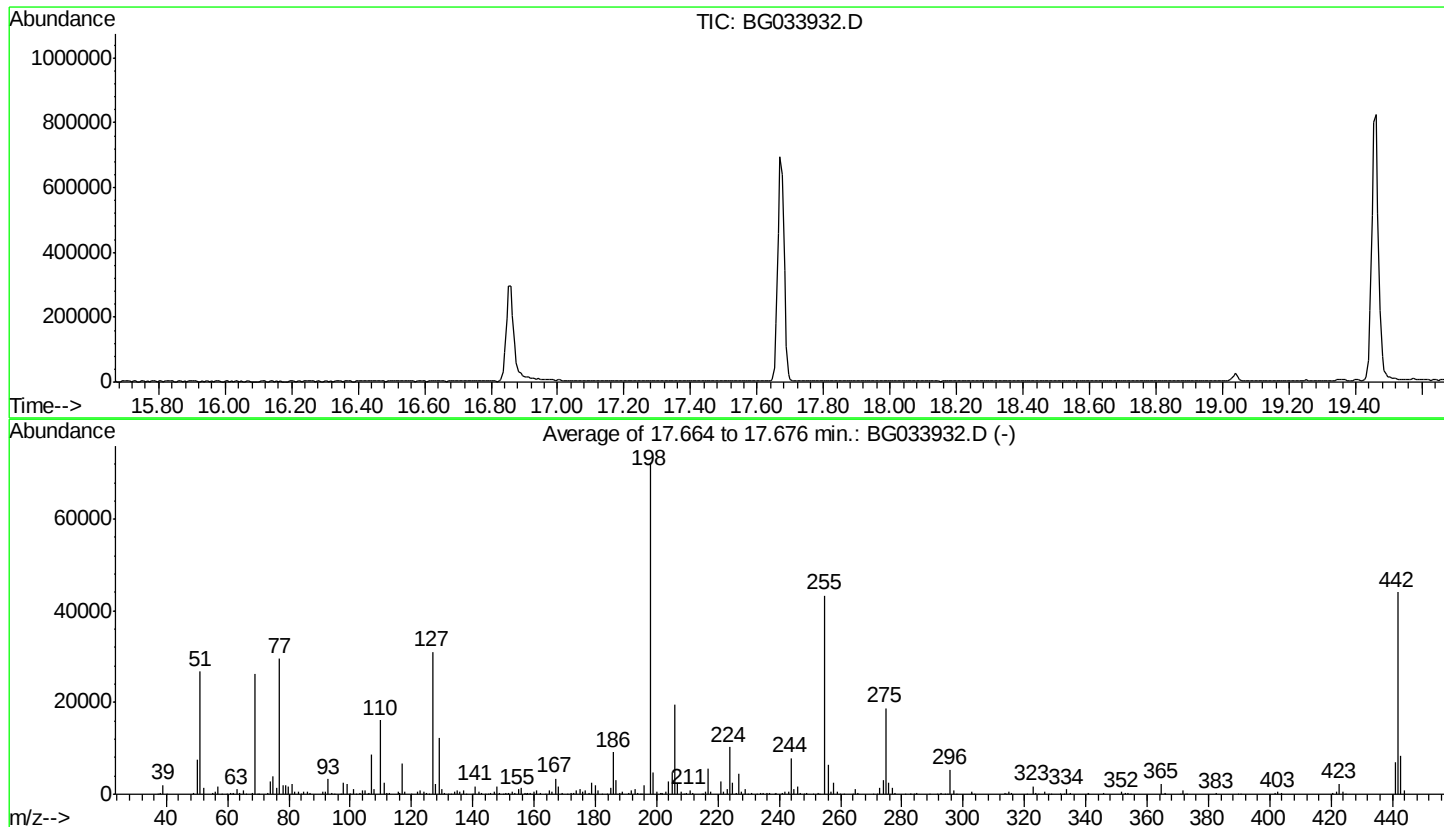

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.0	26786	PASS
68	69	0.00	2	1.4	374	PASS
69	198	0.00	100	36.3	26232	PASS
70	69	0.00	2	0.3	81	PASS
127	198	10	80	42.9	31056	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72338	PASS
199	198	5	9	6.5	4686	PASS
275	198	10	60	26.0	18835	PASS
365	198	1	100	3.2	2290	PASS
441	443	0.01	100	84.9	7077	PASS
442	198	50	100	60.9	44061	PASS
443	442	15	24	18.9	8332	PASS