


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042319\
 Data File : BG040575.D
 Acq On : 23 Apr 2019 17:31
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

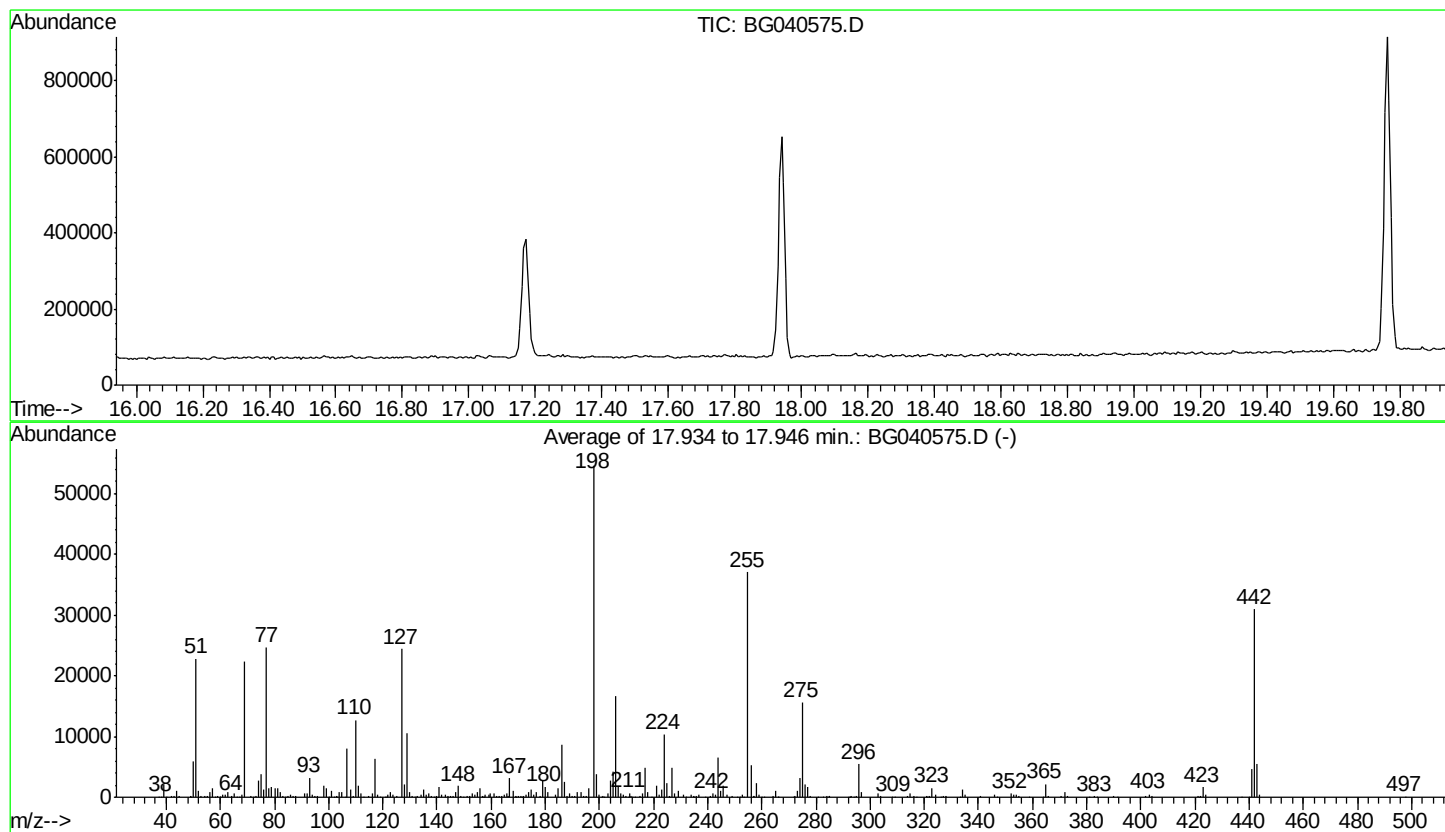

AutoFind: Scans 2527, 2528, 2529; Background Corrected with Scan 2520

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	22816	PASS
68	69	0.00	2	1.7	371	PASS
69	198	0.00	100	40.9	22335	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.7	24411	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54637	PASS
199	198	5	9	6.9	3783	PASS
275	198	10	60	28.5	15558	PASS
365	198	1	100	3.9	2127	PASS
441	198	0.01	100	8.5	4655	PASS
442	198	50	100	56.6	30906	PASS
443	442	15	24	17.9	5539	PASS