
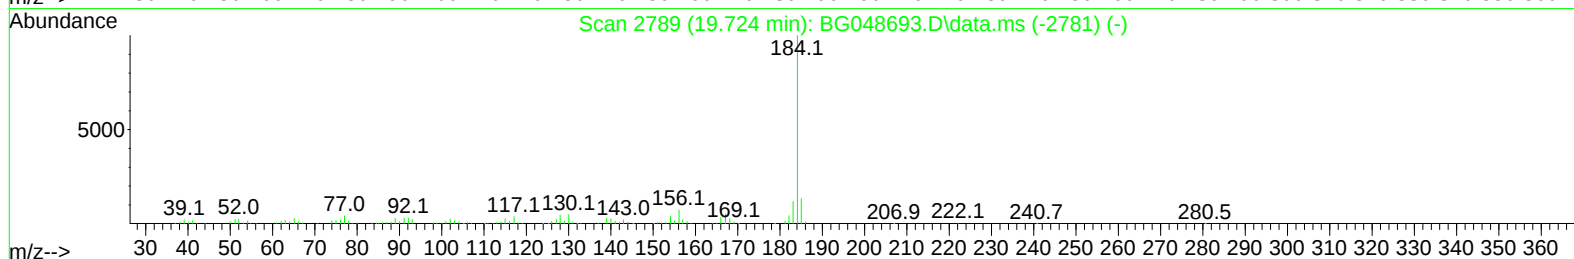
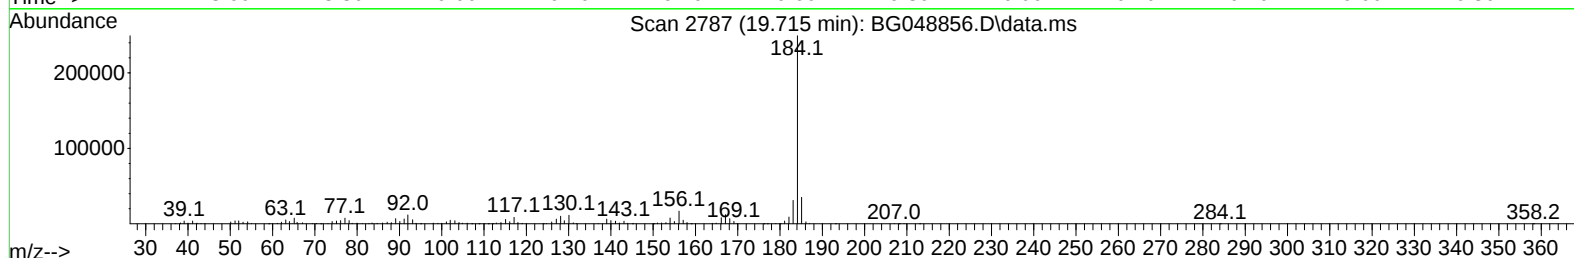


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042321\
 Data File : BG048856.D
 Acq On : 23 Apr 2021 9:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 11:15:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 20 17:33:30 2021
 Response via : Initial Calibration

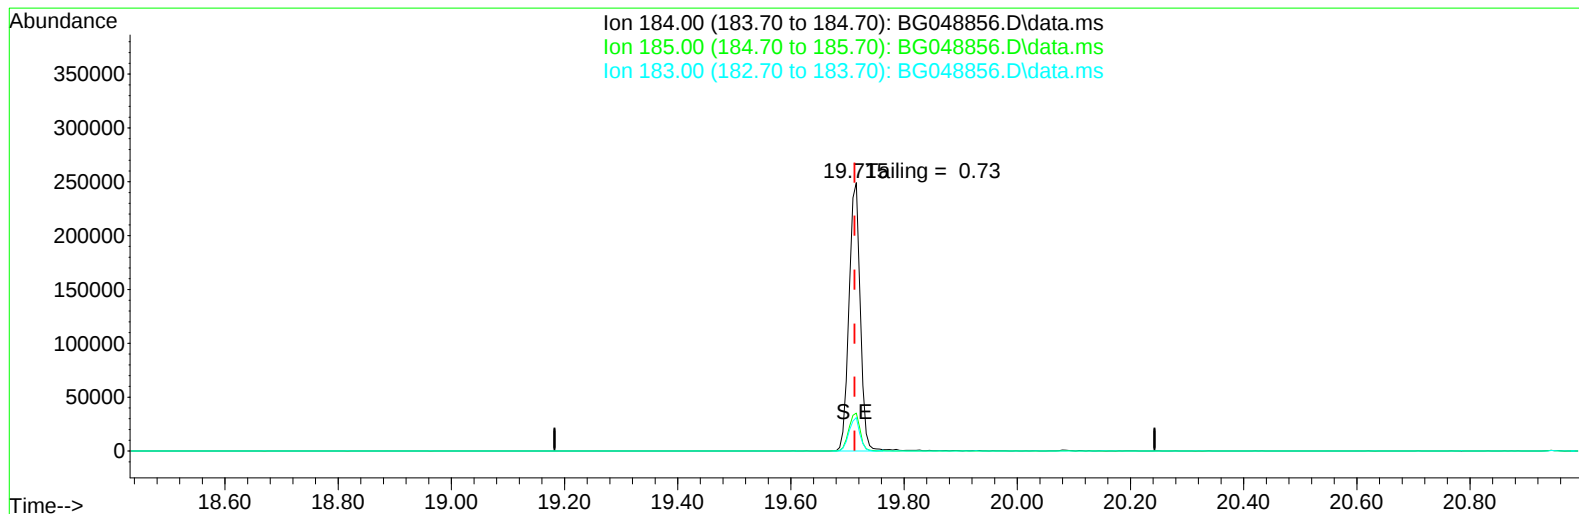




TIC: BG048856.D\data.ms

(77) Benzidine**19.715min (+ 0.003) 62801.46 ng****response 341091**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.11
183.00	11.70	12.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042321\
Data File : BG048856.D
Acq On : 23 Apr 2021 9:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 11:15:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

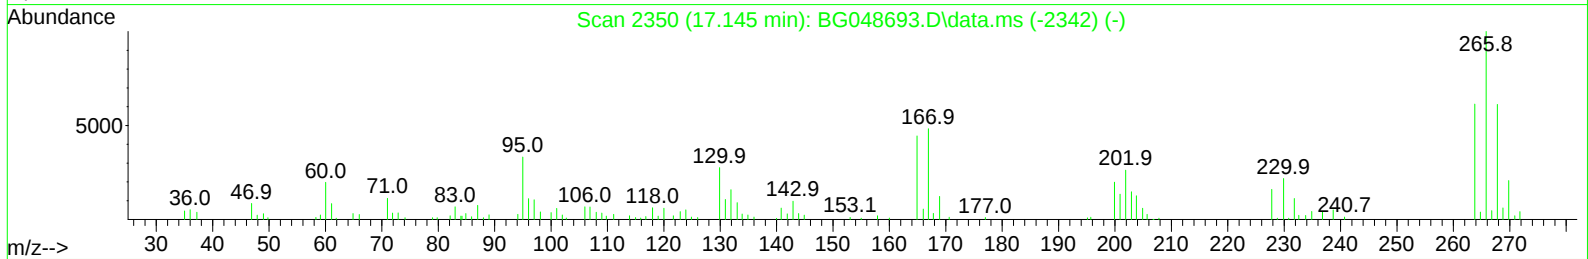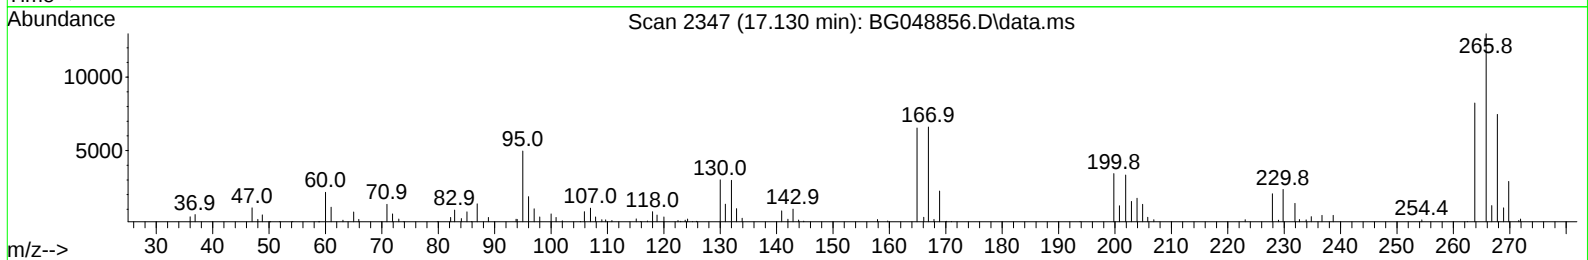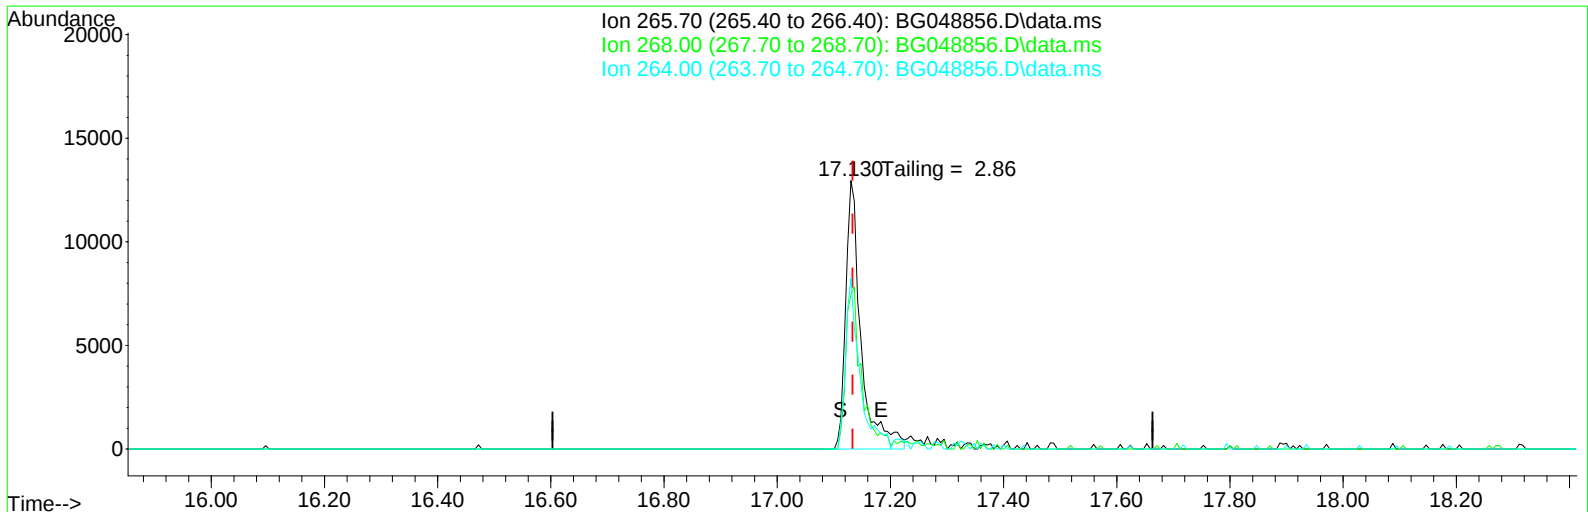

TIC: BG048856.D\data.ms

(70) Pentachlorophenol (C)

17.130min (-0.003) 53068.66 ng

response 24396

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	57.57
264.00	61.30	63.63
0.00	0.00	0.00