
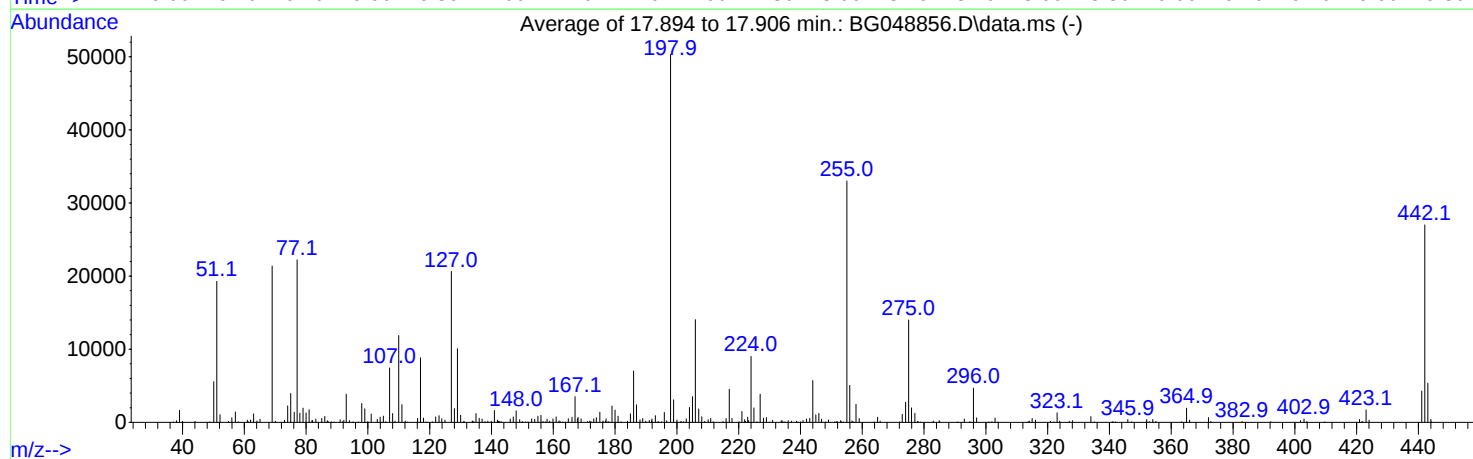


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042321\
 Data File : BG048856.D
 Acq On : 23 Apr 2021 9:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 26 13:36:49 2021

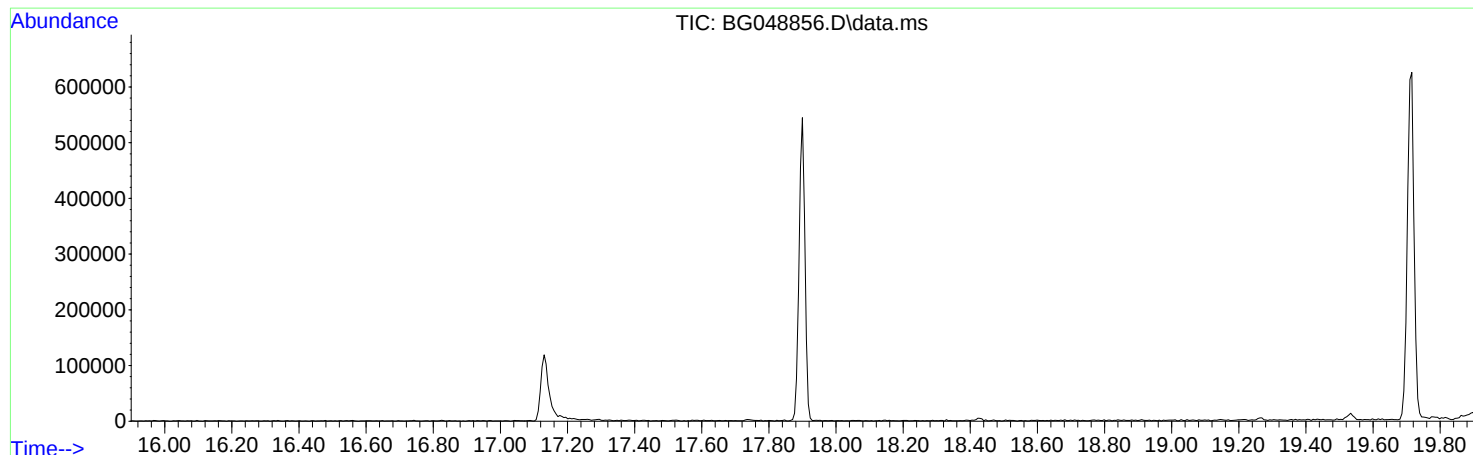




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	19289	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.5	21379	PASS
70	69	0.00	2	0.8	176	PASS
127	198	10	80	41.1	20653	PASS
197	198	0.00	2	0.4	215	PASS
198	198	100	100	100.0	50307	PASS
199	198	5	9	6.1	3076	PASS
275	198	10	60	27.8	14006	PASS
365	198	1	100	3.9	1950	PASS
441	198	0.01	100	8.5	4283	PASS
442	198	50	100	53.7	27013	PASS
443	442	15	24	19.8	5352	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042321\
Data File : BG048856.D
Acq On : 23 Apr 2021 9:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 23 11:15:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

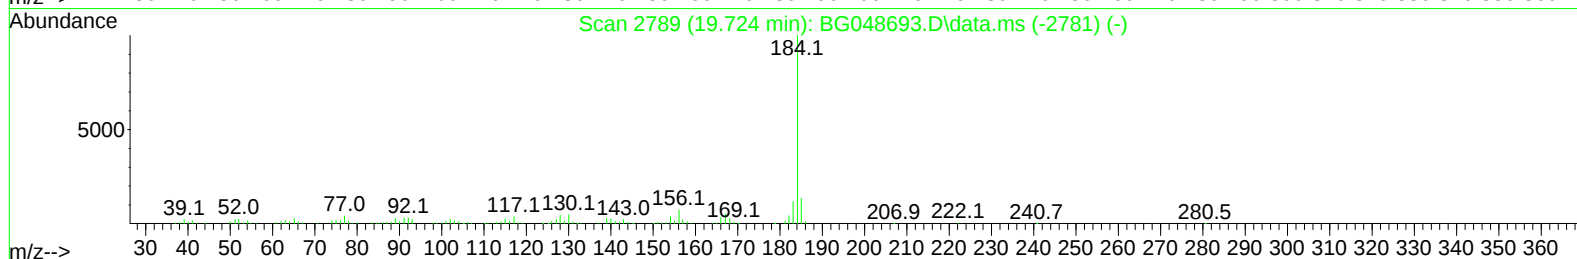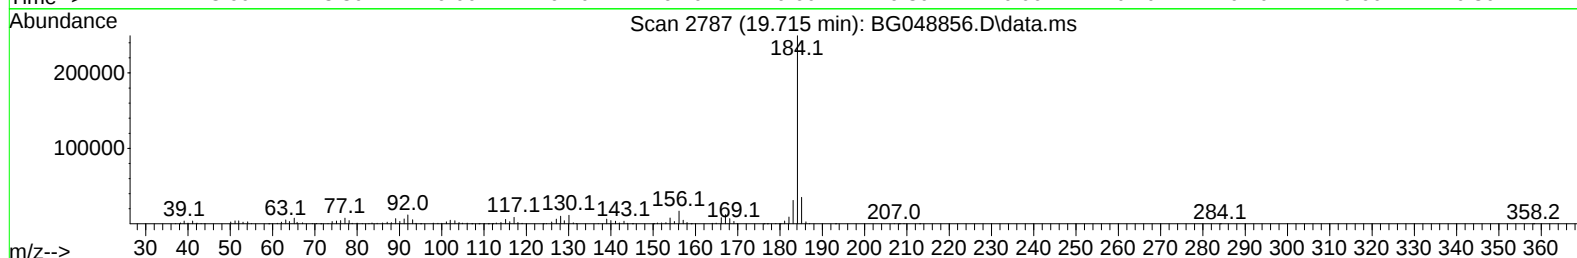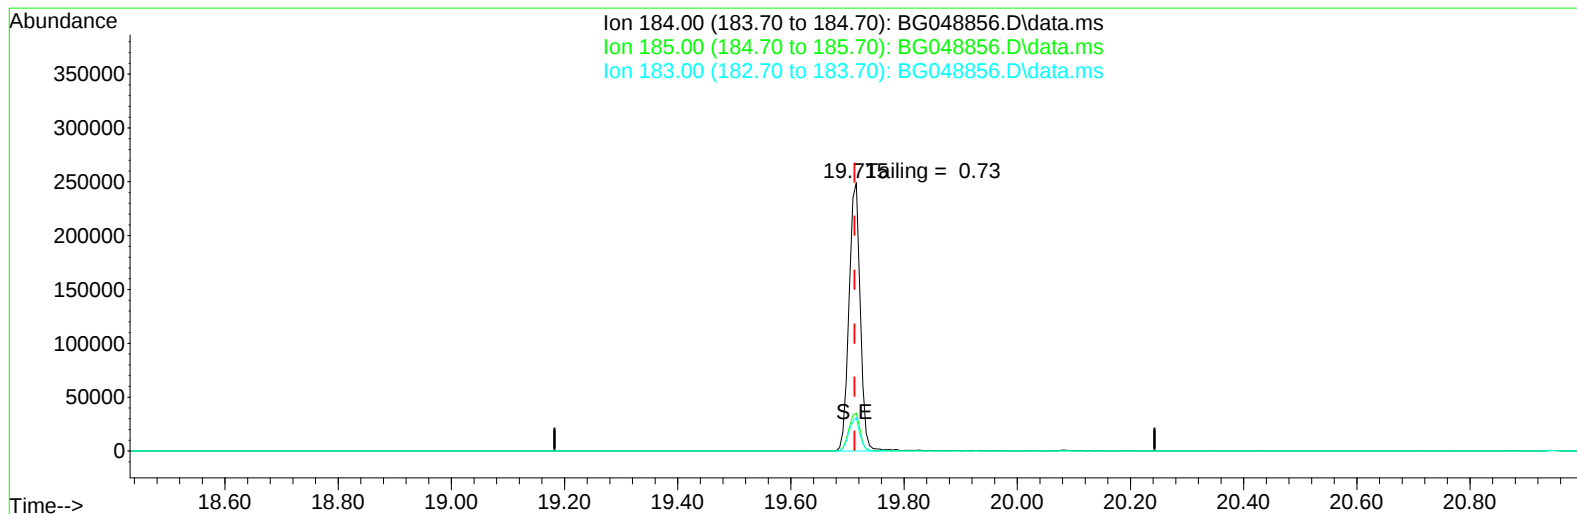

TIC: BG048856.D\data.ms

(77) Benzidine

19.715min (+ 0.003) 62801.46 ng




response 341091

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.11
183.00	11.70	12.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042321\
Data File : BG048856.D
Acq On : 23 Apr 2021 9:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 23 11:15:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG041421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 20 17:33:30 2021
Response via : Initial Calibration

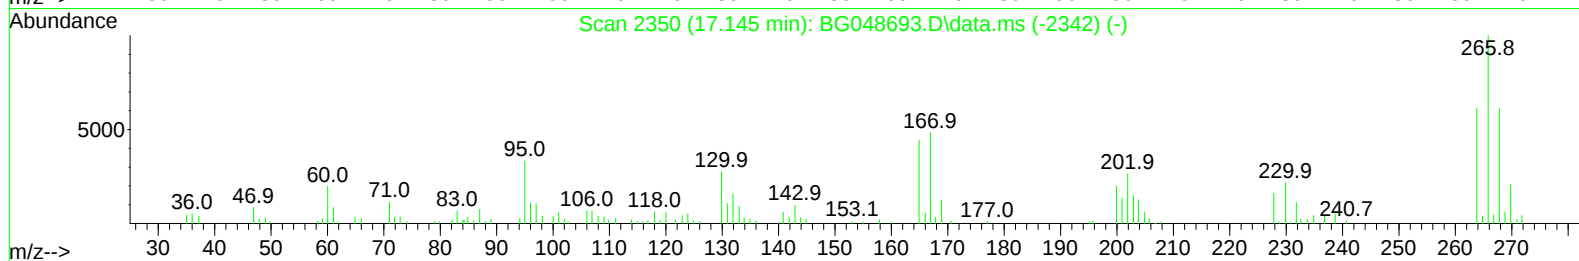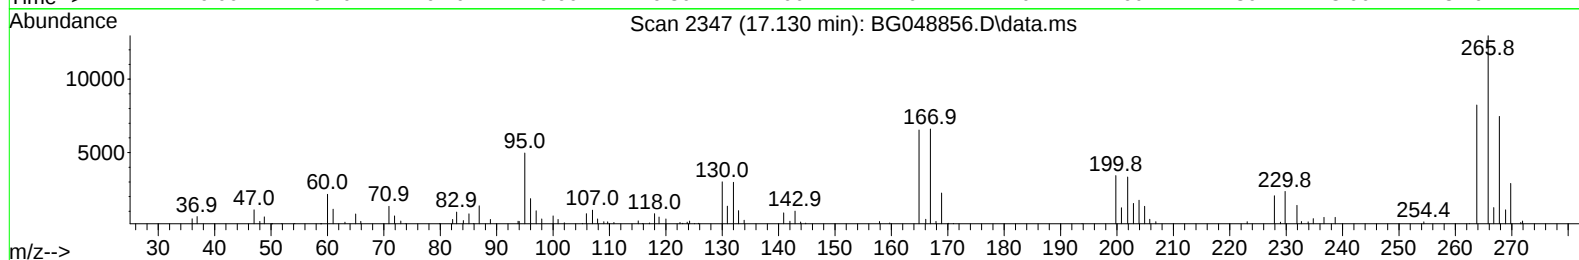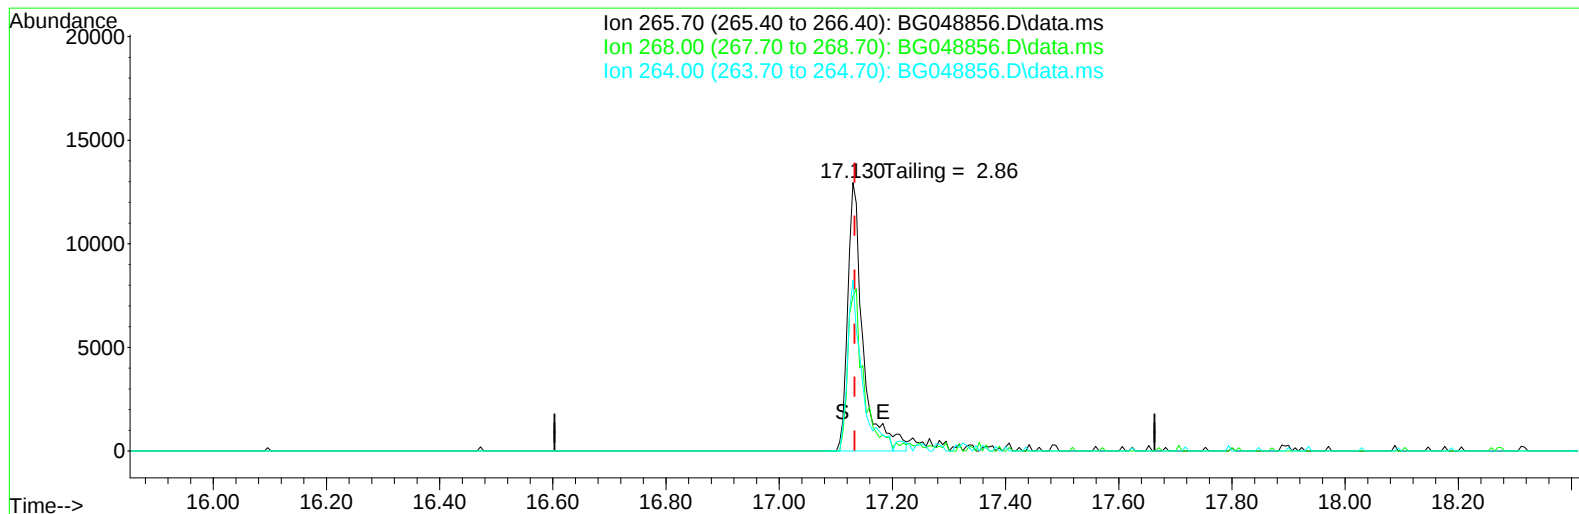

TIC: BG048856.D\data.ms

(70) Pentachlorophenol (C)

17.130min (-0.003) 53068.66 ng

response 24396

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	57.57
264.00	61.30	63.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/23/2021	BNA_G	BG048856.D
Compound Name	Response	Retention Time
DDT	158940	20.94
DDD	5274	20.5
DDE	857	19.99
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6131	165071	3.71