
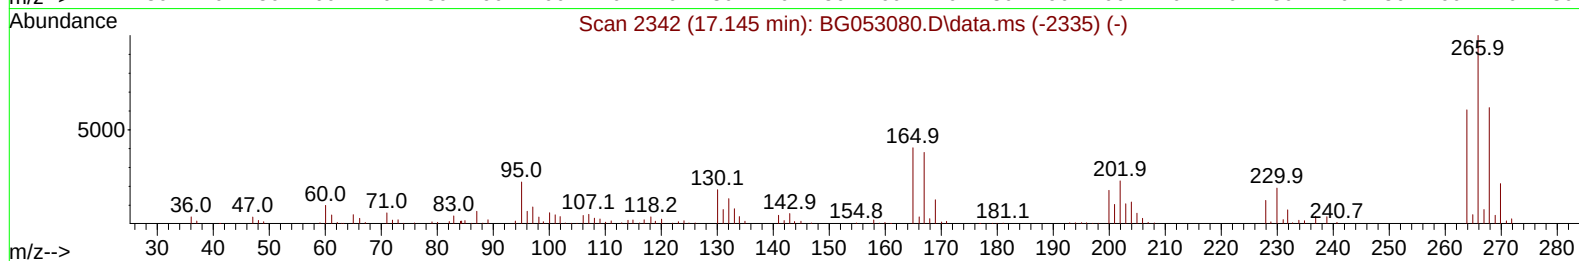
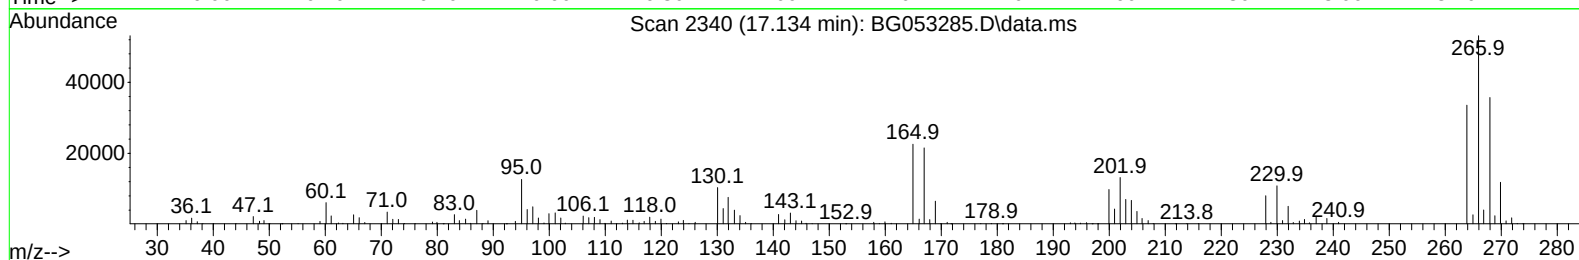


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042322\
Data File : BG053285.D
Acq On : 23 Apr 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 10:26:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

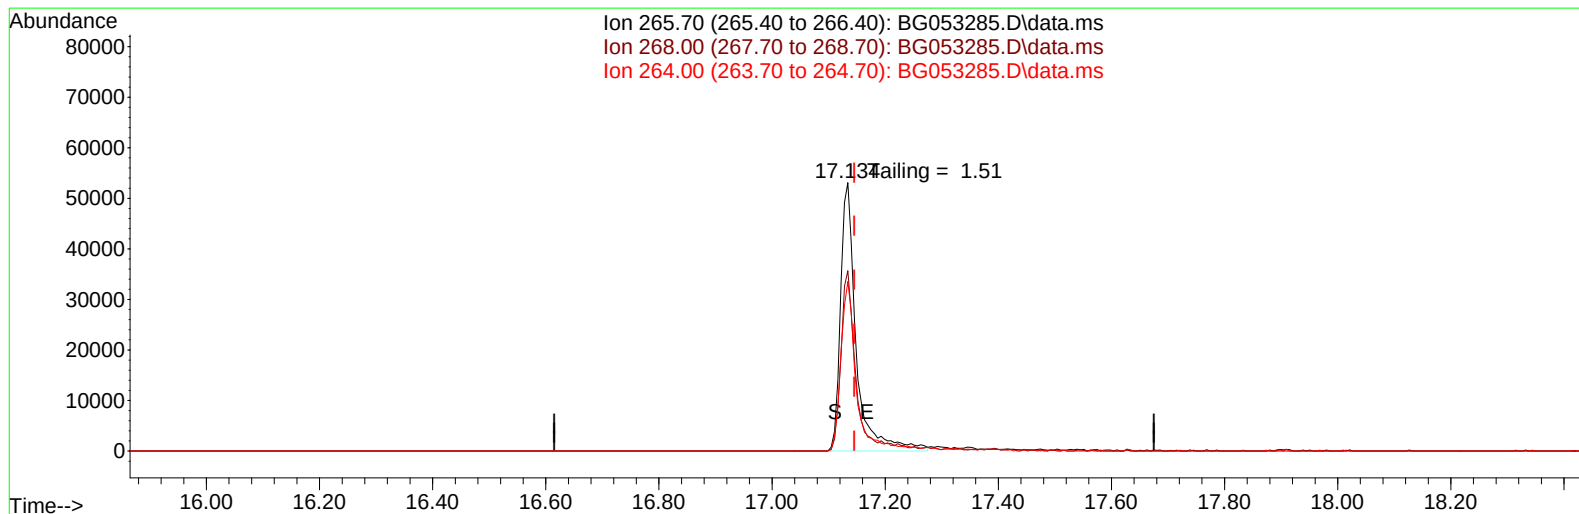

TIC: BG053285.D\data.ms

(70) Pentachlorophenol (C)




17.134min (-0.011) 31561.06 ng

response 102922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	67.20
264.00	56.60	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042322\
Data File : BG053285.D
Acq On : 23 Apr 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 10:26:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

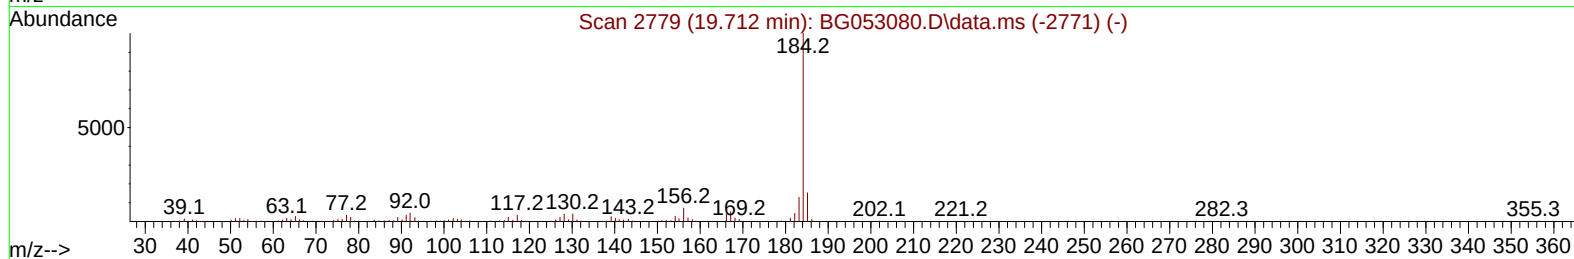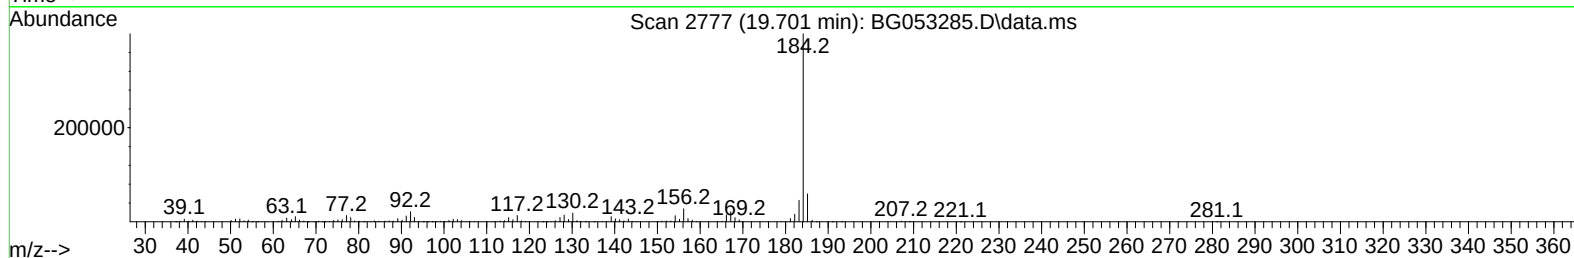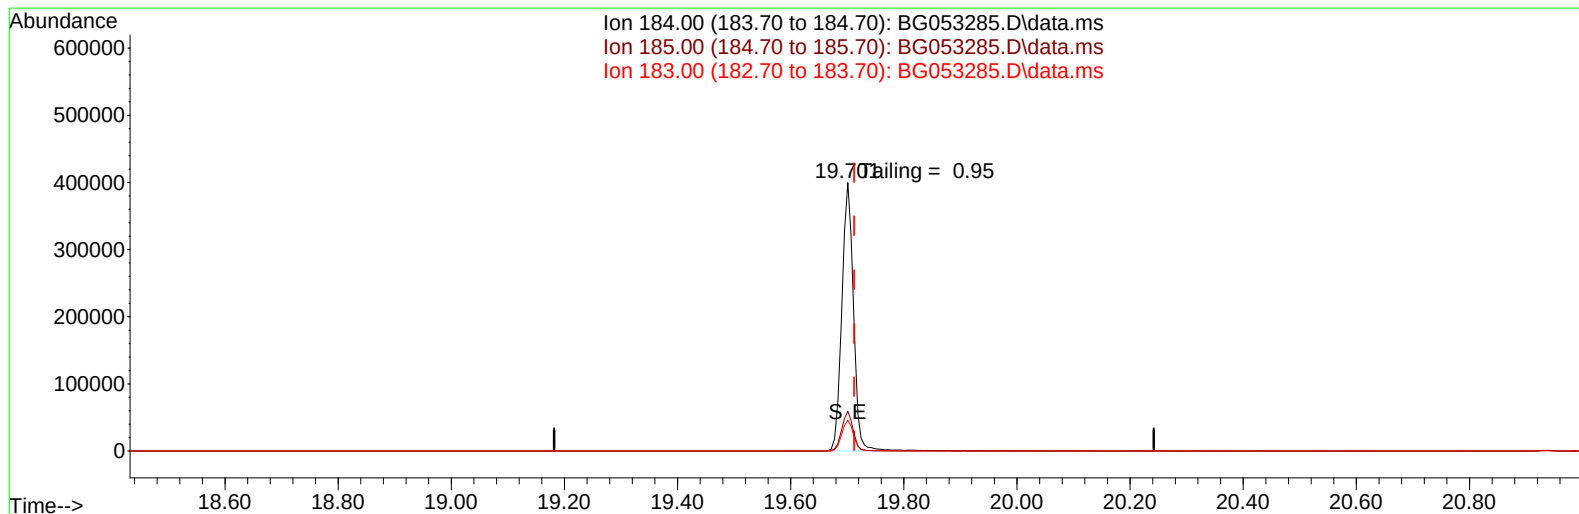

TIC: BG053285.D\data.ms

(77) Benzidine

19.701min (-0.011) 0.00 ng

response 570993

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.82
183.00	11.80	11.45
0.00	0.00	0.00