


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042322\
 Data File : BG053285.D
 Acq On : 23 Apr 2022 9:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 01:13:30 2022

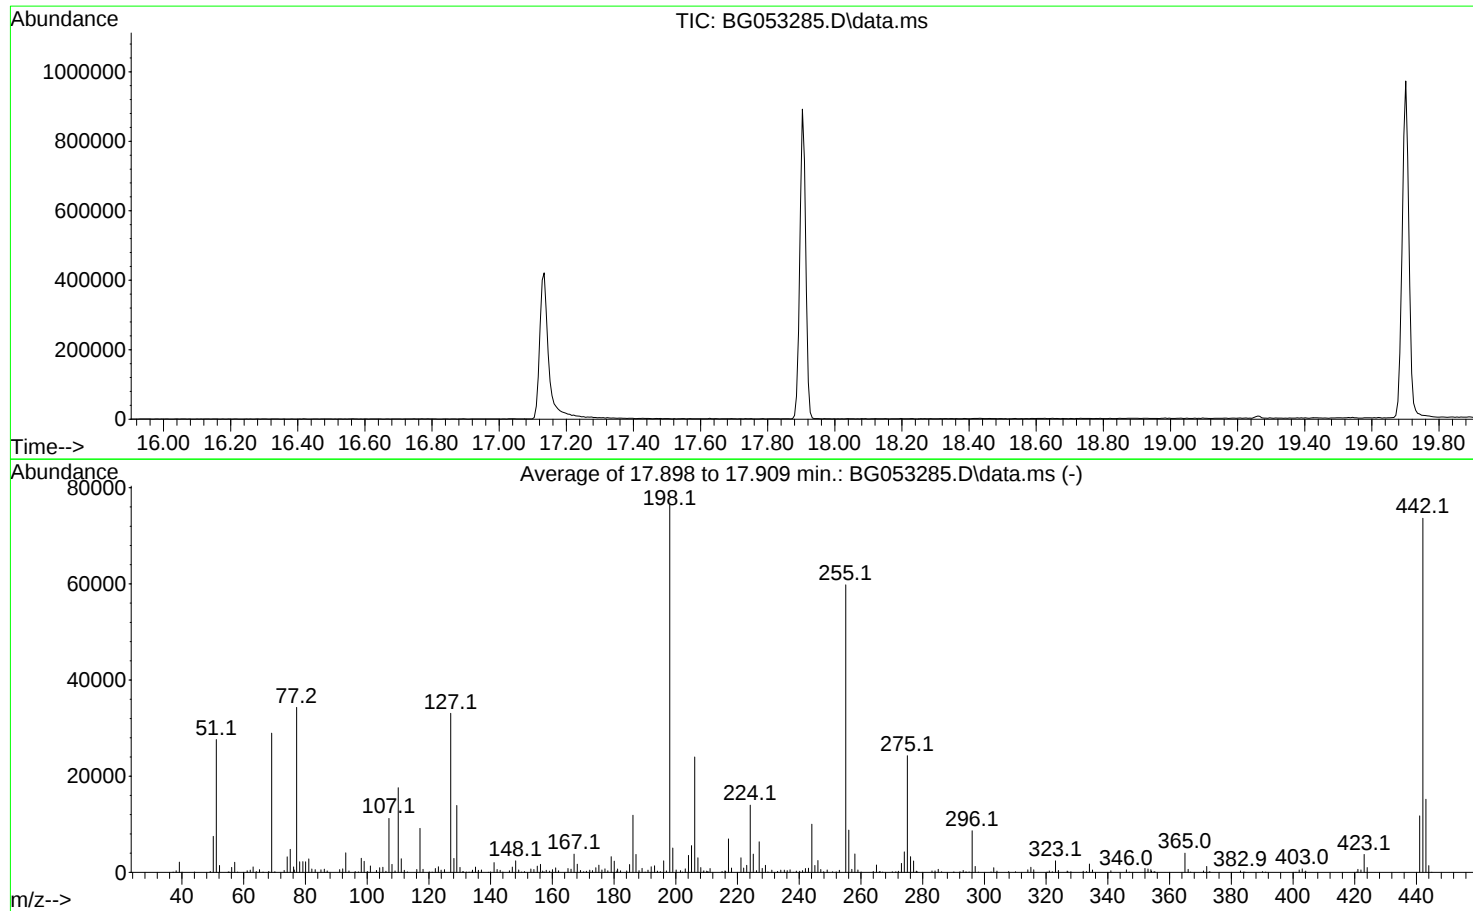

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	27632	PASS
68	69	0.00	2	0.7	196	PASS
69	198	0.00	100	37.8	28941	PASS
70	69	0.00	2	0.5	133	PASS
127	198	10	80	43.2	33083	PASS
197	198	0.00	2	0.4	306	PASS
198	198	100	100	100.0	76517	PASS
199	198	5	9	6.6	5065	PASS
275	198	10	60	31.7	24261	PASS
365	198	1	100	5.2	3980	PASS
441	198	0.01	100	15.4	11746	PASS
442	442	50	100	100.0	73667	PASS
443	442	15	24	20.7	15222	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/23/2022	BNA_G	<u>BG053285.D</u>
Compound Name	Response	Retention Time
DDT	299836	20.935
DDD	2082	20.547
DDE	114	20.001
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2196	302032	0.73

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042322\
Data File : BG053285.D
Acq On : 23 Apr 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 23 10:26:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

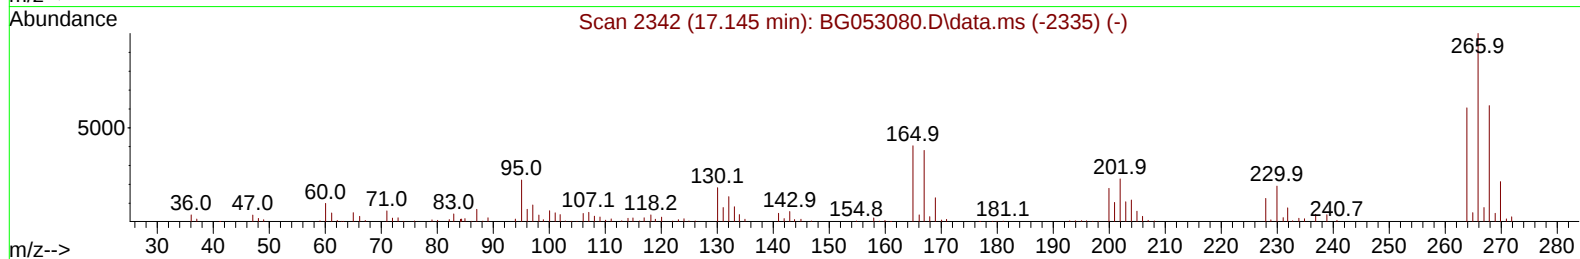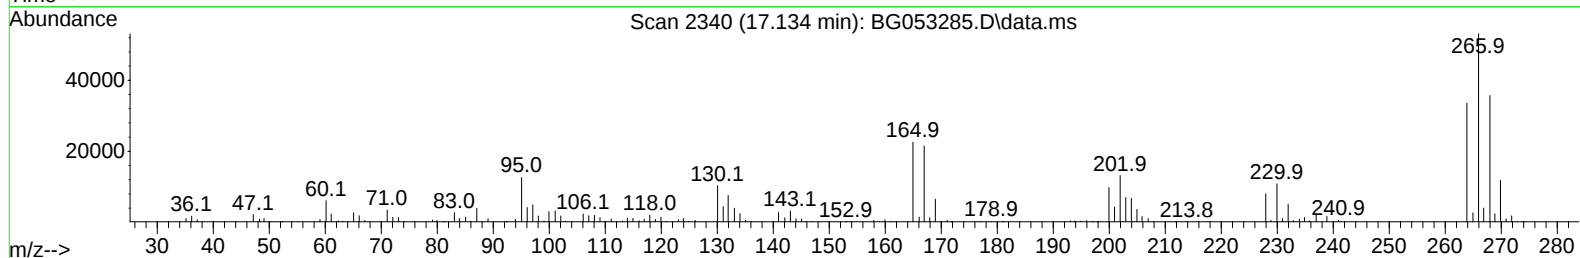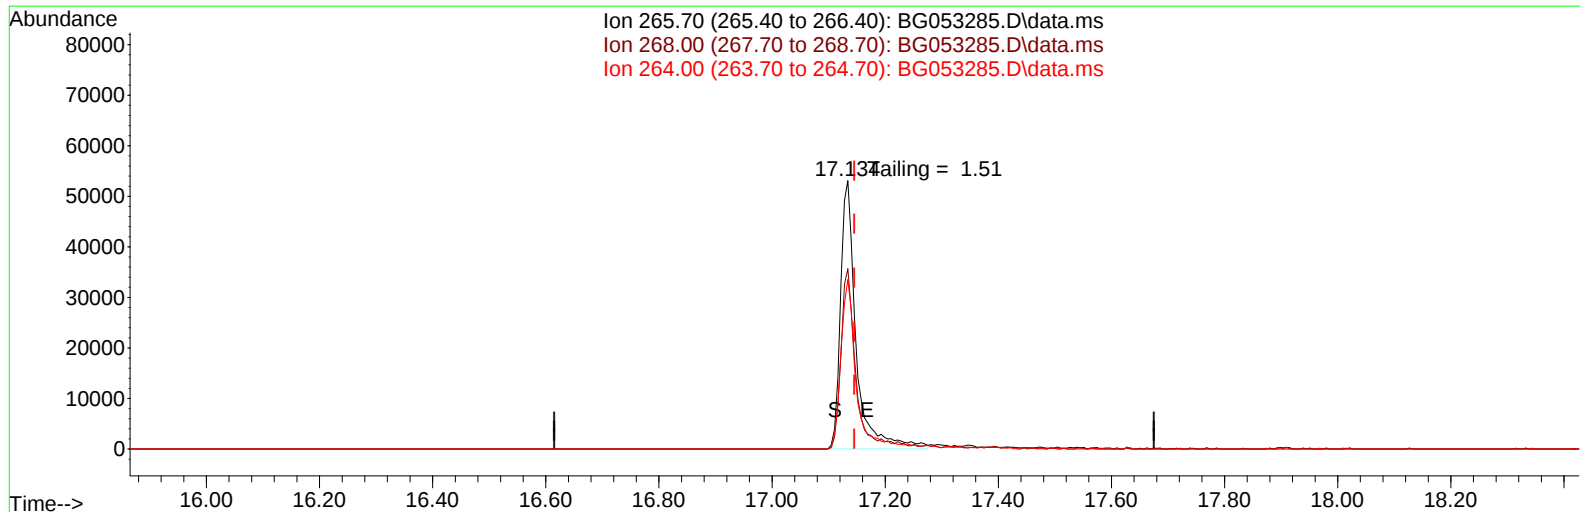

TIC: BG053285.D\data.ms

(70) Pentachlorophenol (C)

17.134min (-0.011) 31561.06 ng




response 102922

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	67.20
264.00	56.60	63.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042322\
Data File : BG053285.D
Acq On : 23 Apr 2022 9:52
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 23 10:26:35 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 08 15:31:24 2022
Response via : Initial Calibration

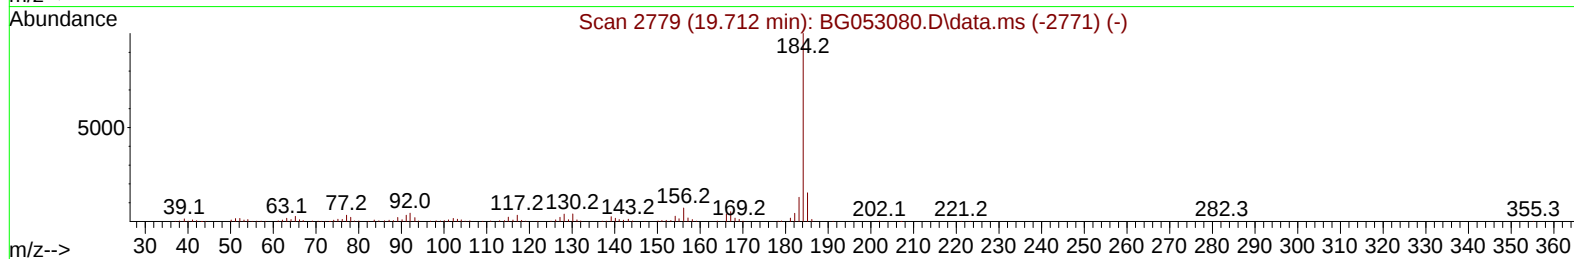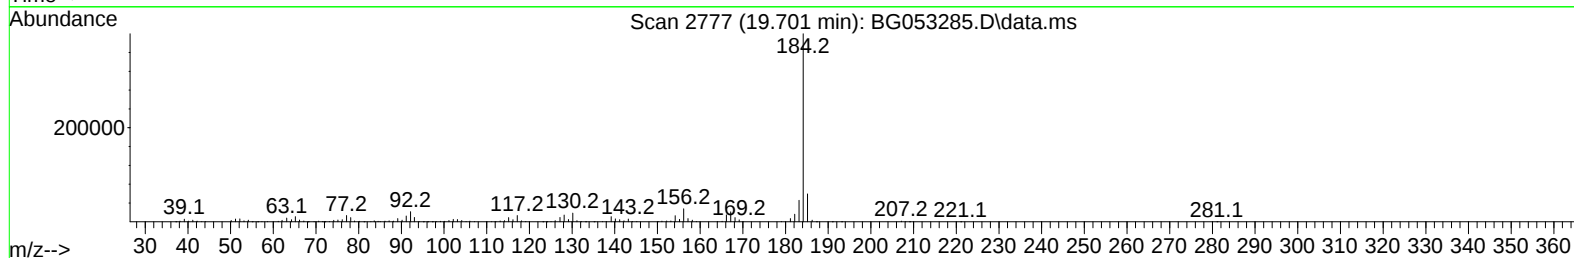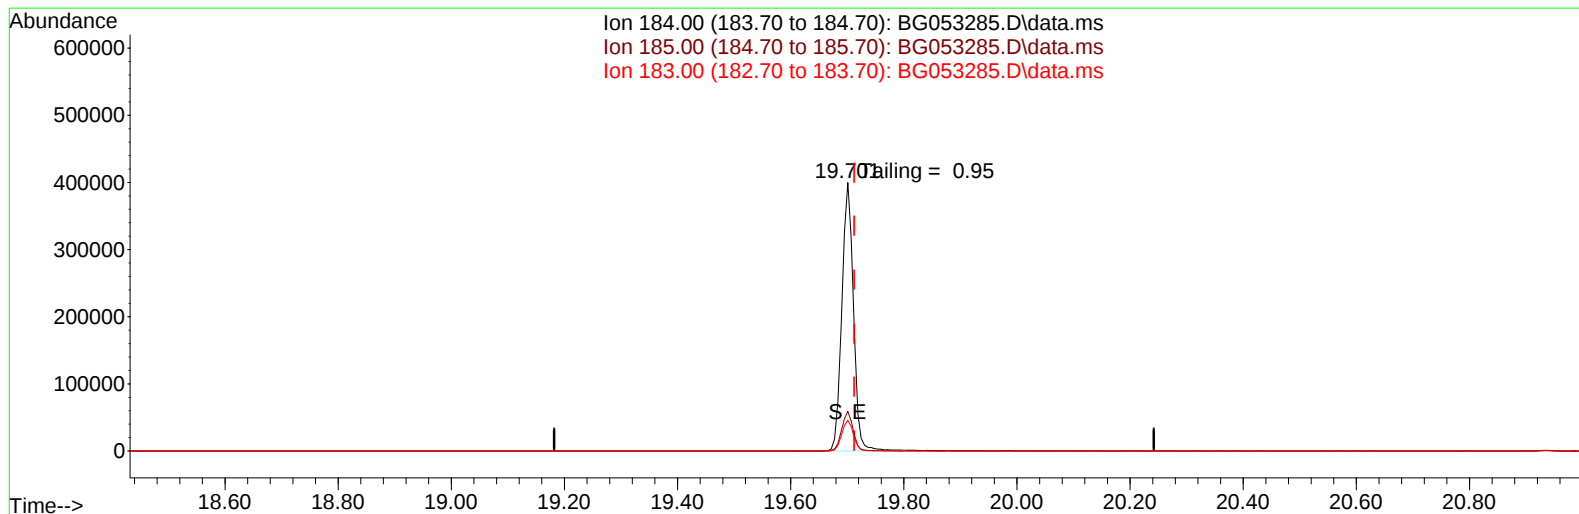

TIC: BG053285.D\data.ms

(77) Benzidine

19.701min (-0.011) 0.00 ng

response 570993

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.82
183.00	11.80	11.45
0.00	0.00	0.00