
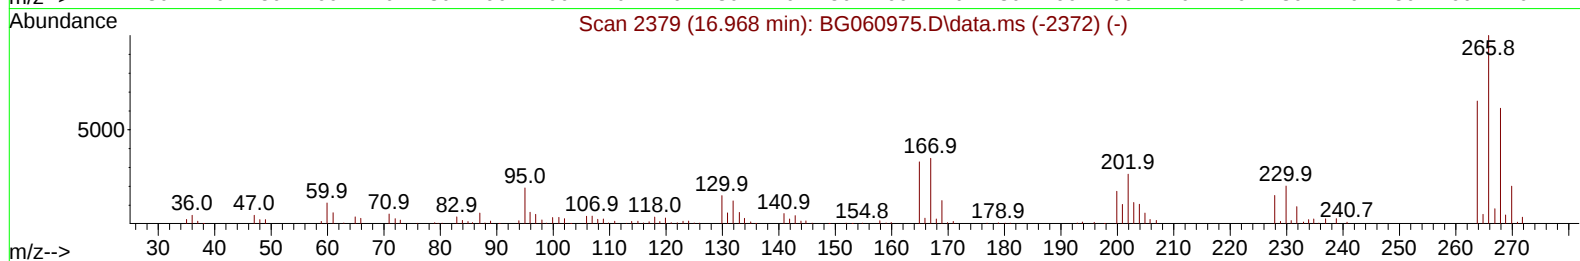
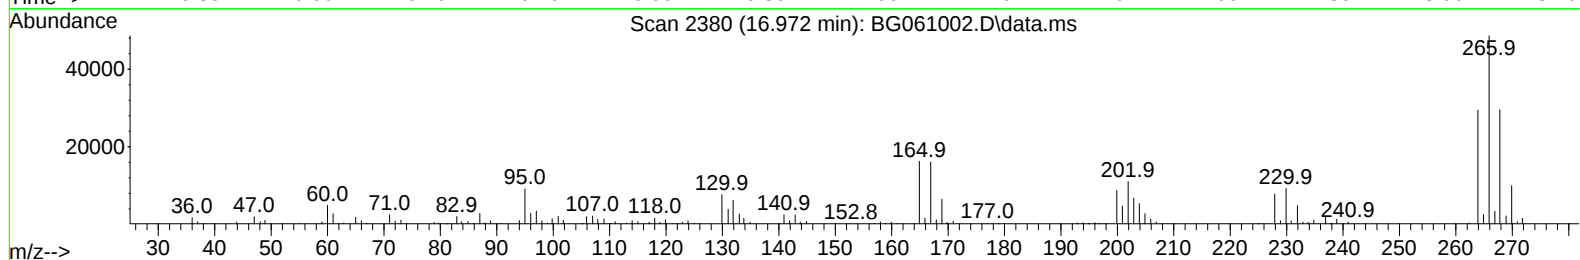


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061002.D
Acq On : 23 Apr 2024 10:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 12:58:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

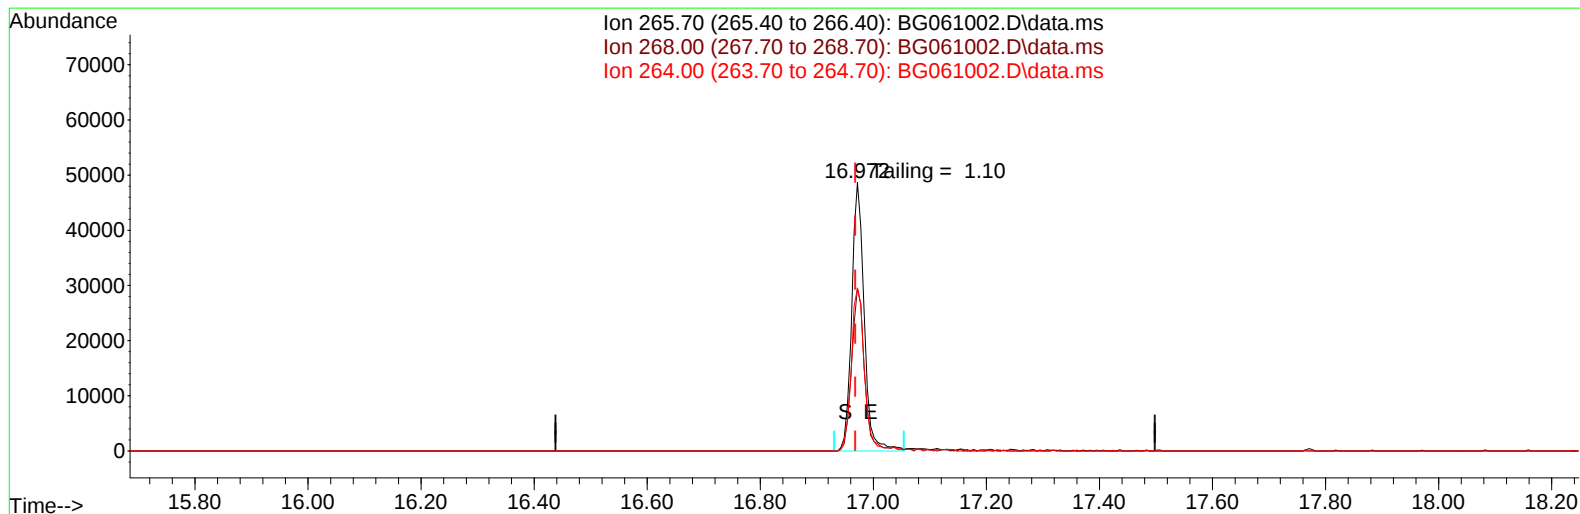

TIC: BG061002.D\data.ms

(70) Pentachlorophenol (C)




16.972min (+ 0.004) 28935.08 ng

response 74679

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	60.73
264.00	65.20	60.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061002.D
Acq On : 23 Apr 2024 10:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 23 12:58:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

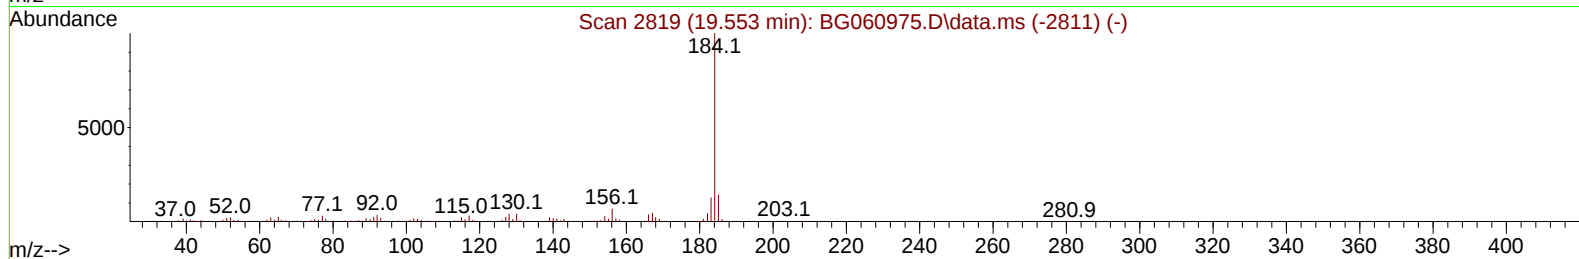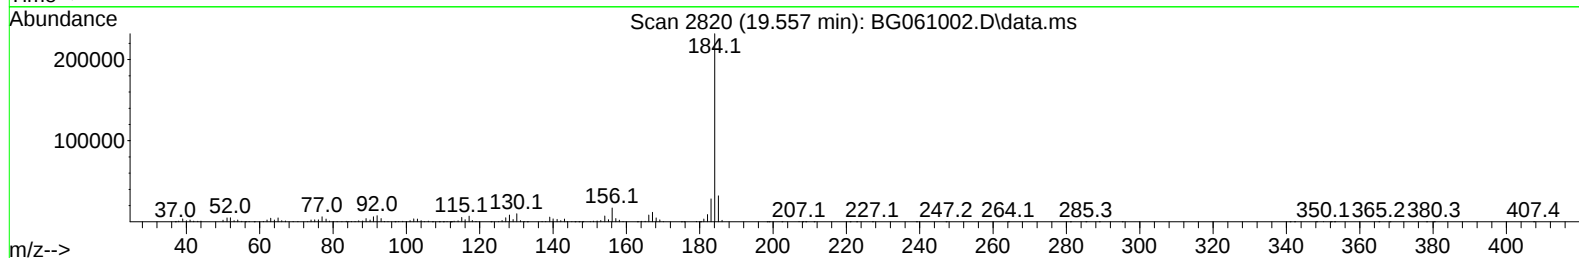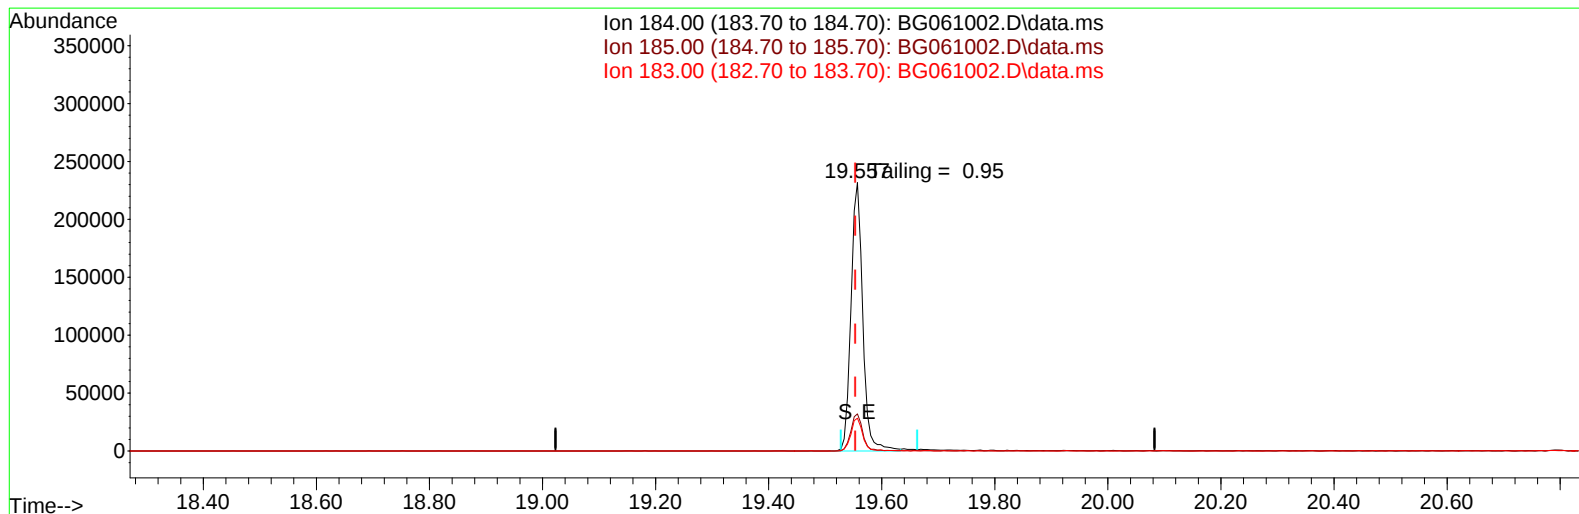

TIC: BG061002.D\data.ms

(77) Benzidine

19.557min (+ 0.004) 72117.87 ng

response 328721

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.87
183.00	12.70	12.24
0.00	0.00	0.00