

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
 Data File : BG061006.D
 Acq On : 23 Apr 2024 13:47
 Operator : MA/JU
 Sample : P2177-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LKWD-BACKFILL-19

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG061006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.526	426	432	440	rVB	200654	316477	20.93%	3.684%
2	7.106	692	701	712	rBV	223875	385392	25.48%	4.486%
3	7.940	837	843	850	rBV	71711	115305	7.62%	1.342%
4	9.092	1032	1039	1047	rBV	148897	251424	16.63%	2.927%
5	10.737	1312	1319	1327	rBV	88027	156965	10.38%	1.827%
6	13.193	1730	1737	1744	rBV	435607	641892	42.45%	7.472%
7	14.568	1966	1971	1978	rBV	154140	244231	16.15%	2.843%
8	14.815	1980	2013	2014	rBV3	358600	1471812	97.33%	17.132%
9	16.060	2218	2225	2231	rVB	449514	668036	44.17%	7.776%
10	17.318	2433	2439	2446	rVB	248349	375433	24.83%	4.370%
11	17.453	2455	2462	2473	rVB8	12450	39067	2.58%	0.455%
12	17.987	2547	2553	2557	rBV8	11594	21940	1.45%	0.255%
13	18.217	2585	2592	2597	rBV4	30419	49295	3.26%	0.574%
14	18.581	2644	2654	2655	rBV9	10936	27130	1.79%	0.316%
15	18.716	2671	2677	2683	rVB3	26453	53406	3.53%	0.622%
16	19.492	2804	2809	2813	rVB6	22206	32495	2.15%	0.378%
17	19.674	2830	2840	2845	rVB2	63259	131356	8.69%	1.529%
18	19.938	2879	2885	2890	rBV	1228180	1512260	100.00%	17.603%
19	19.997	2890	2895	2902	rVB	94911	171328	11.33%	1.994%
20	20.455	2968	2973	2983	rBV	64558	107307	7.10%	1.249%
21	21.166	3088	3094	3100	rBV	63091	117208	7.75%	1.364%
22	21.242	3103	3107	3112	rVV2	59943	91683	6.06%	1.067%
23	21.483	3145	3148	3151	rVB2	17529	21649	1.43%	0.252%
24	21.577	3154	3164	3170	rVB	289908	513157	33.93%	5.973%
25	21.936	3220	3225	3231	rVB2	48709	85233	5.64%	0.992%
26	22.805	3367	3373	3381	rVB4	52746	109377	7.23%	1.273%
27	23.787	3535	3540	3547	rVB3	45755	102773	6.80%	1.196%
28	24.697	3687	3695	3706	rVB2	194312	526196	34.80%	6.125%
29	24.956	3732	3739	3749	rVB5	44280	127093	8.40%	1.479%
30	26.331	3964	3973	3983	rVB5	38909	124215	8.21%	1.446%




Sum of corrected areas: 8591135

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061006.D
Acq On : 23 Apr 2024 13:47
Operator : MA/JU
Sample : P2177-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LKWD-BACKFILL-19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

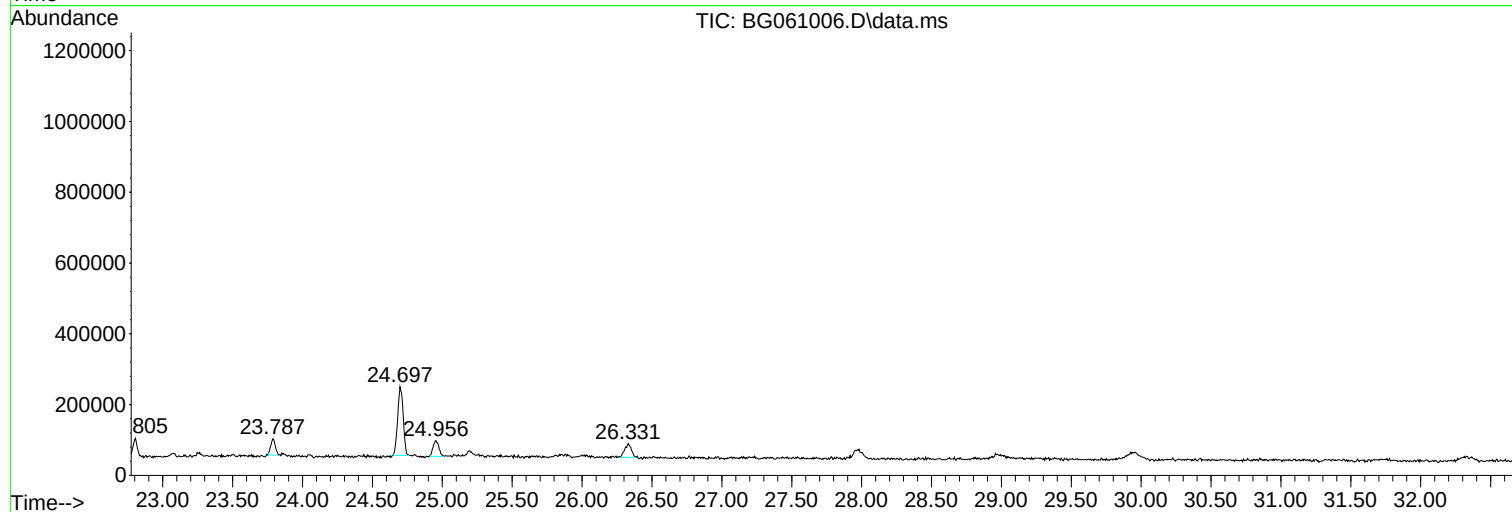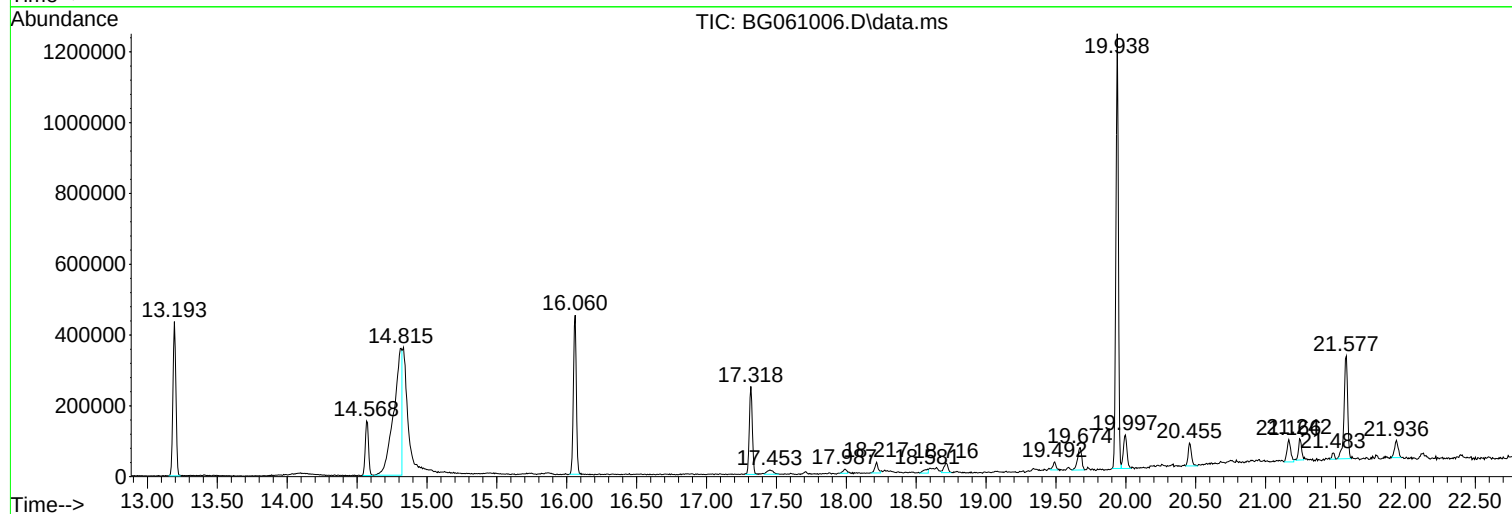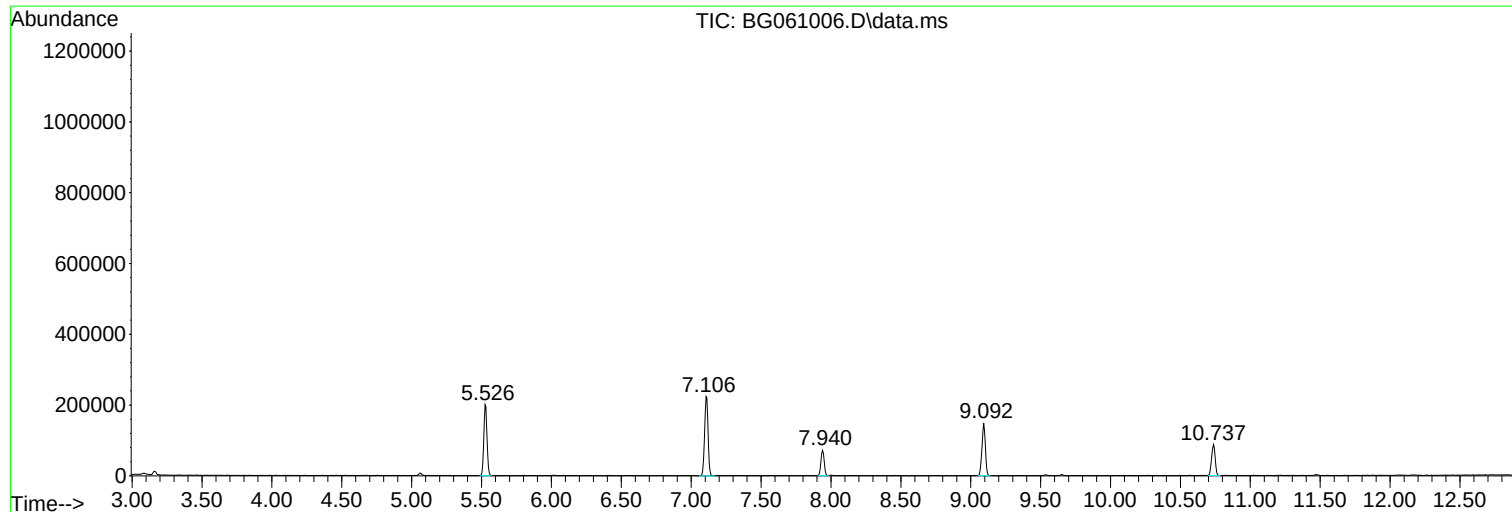

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061006.D
Acq On : 23 Apr 2024 13:47
Operator : MA/JU
Sample : P2177-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LKWD-BACKFILL-19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061006.D
Acq On : 23 Apr 2024 13:47
Operator : MA/JU
Sample : P2177-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LKWD-BACKFILL-19

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------