

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
 Data File : BG061008.D
 Acq On : 23 Apr 2024 15:09
 Operator : MA/JU
 Sample : P2177-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 LKWD-BACKFILL-21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG061008.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	26	30	39	rVB	18672	31863	1.71%	0.449%
2	5.532	427	433	444	rVB	307817	466724	25.11%	6.573%
3	7.112	694	702	710	rVB	315180	519452	27.95%	7.316%
4	7.941	837	843	850	rBV	81758	127344	6.85%	1.793%
5	9.092	1029	1039	1047	rVB	195183	343674	18.49%	4.840%
6	10.737	1309	1319	1326	rBV	94001	161485	8.69%	2.274%
7	13.193	1730	1737	1744	rBV	549620	855736	46.04%	12.052%
8	14.568	1964	1971	1979	rVB	165623	253915	13.66%	3.576%
9	16.061	2218	2225	2233	rBV	602660	928911	49.98%	13.082%
10	17.318	2432	2439	2445	rBV	255485	378251	20.35%	5.327%
11	18.217	2586	2592	2596	rBV3	23324	33072	1.78%	0.466%
12	19.938	2879	2885	2892	rBV	1479683	1858684	100.00%	26.177%
13	21.243	3104	3107	3112	rBV3	38472	56965	3.06%	0.802%
14	21.578	3156	3164	3170	rBV	286371	477837	25.71%	6.730%
15	23.258	3442	3450	3459	rBV3	43056	100087	5.38%	1.410%
16	24.697	3686	3695	3705	rBV2	180619	506425	27.25%	7.132%




Sum of corrected areas: 7100425

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061008.D
Acq On : 23 Apr 2024 15:09
Operator : MA/JU
Sample : P2177-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LKWD-BACKFILL-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

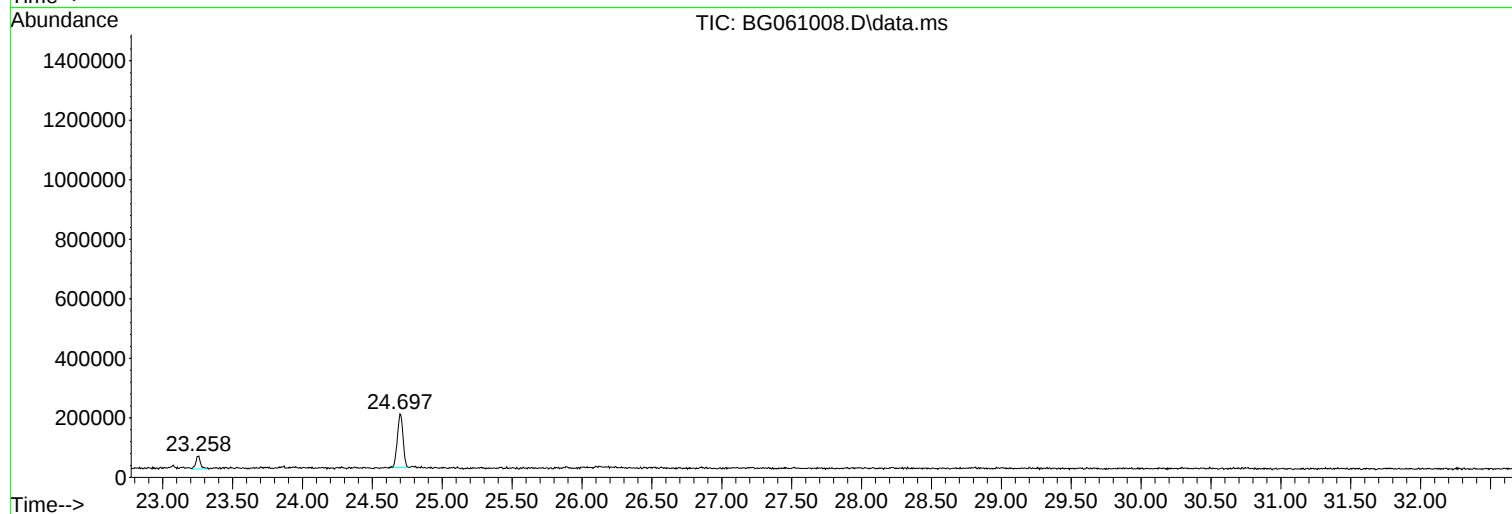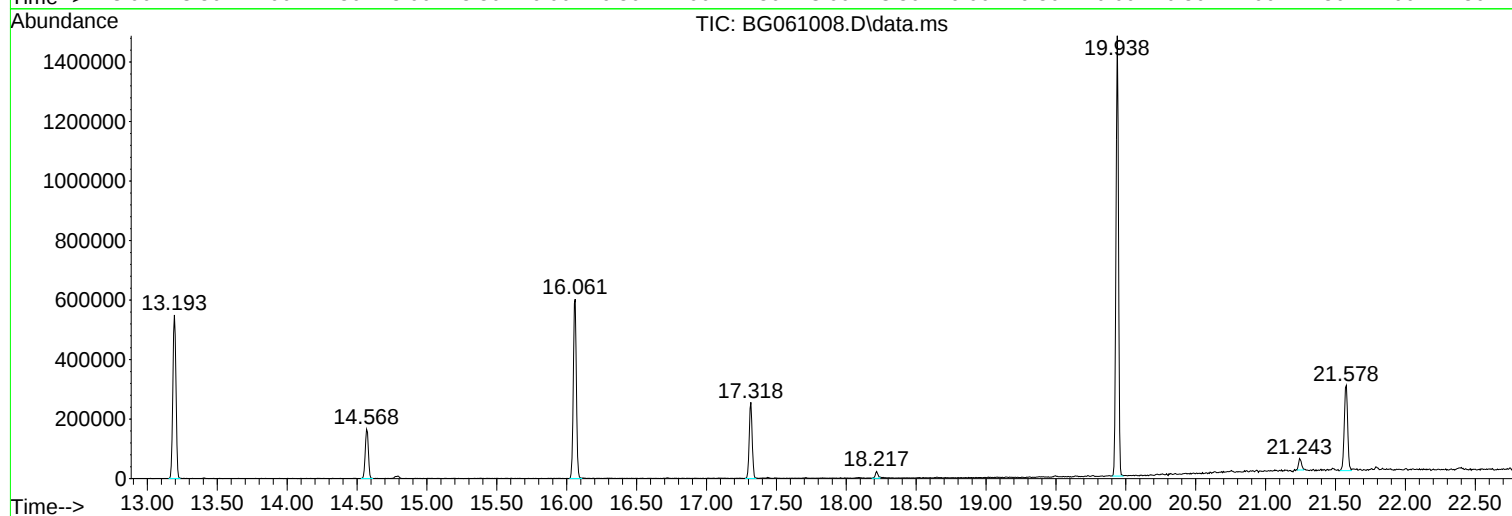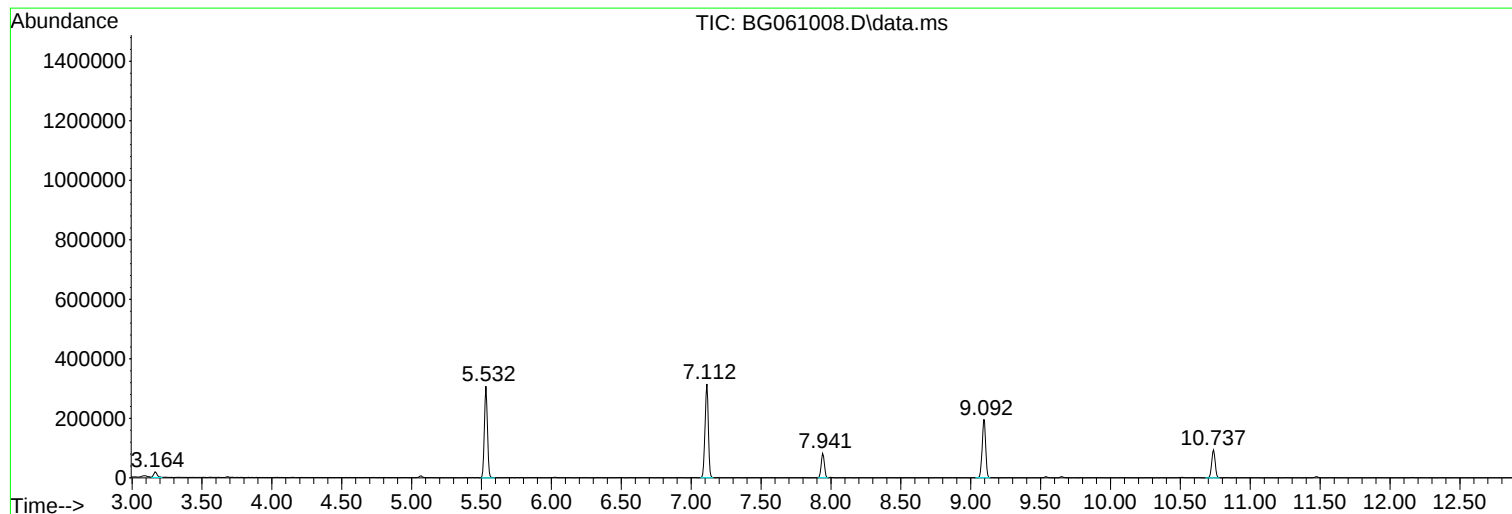

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061008.D
Acq On : 23 Apr 2024 15:09
Operator : MA/JU
Sample : P2177-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LKWD-BACKFILL-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061008.D
Acq On : 23 Apr 2024 15:09
Operator : MA/JU
Sample : P2177-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
LKWD-BACKFILL-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------