
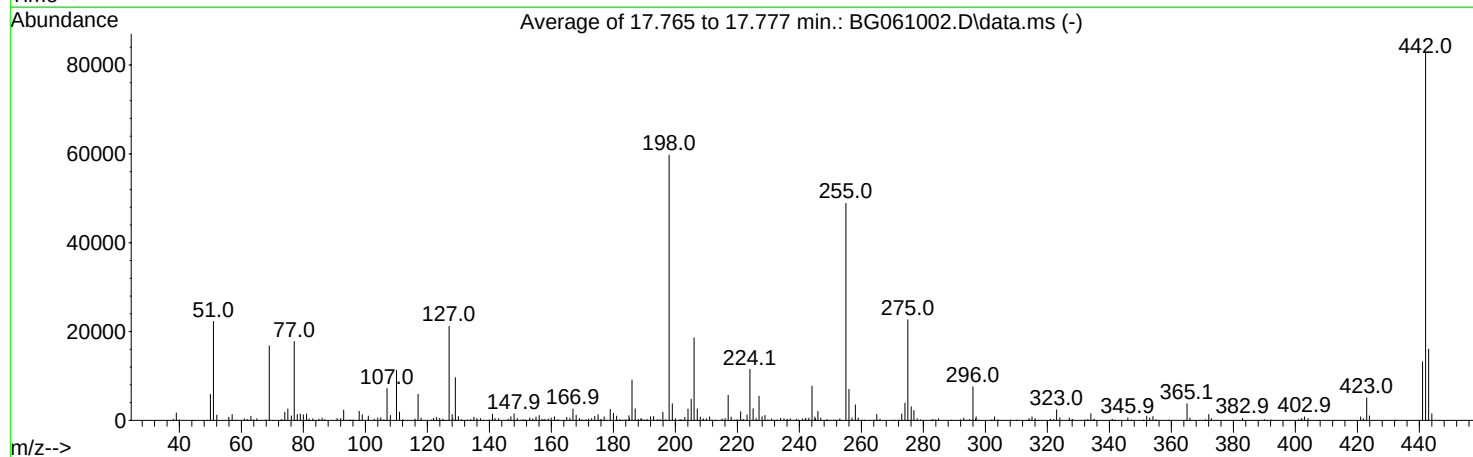


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061002.D
Acq On : 23 Apr 2024 10:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 22 04:22:00 2024

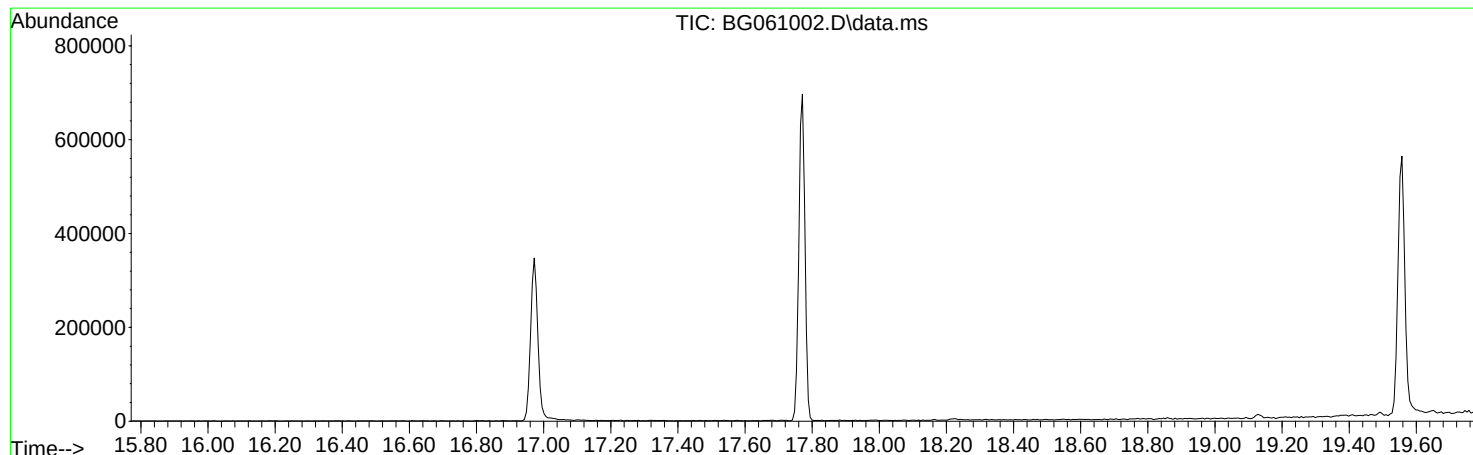




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	22254	PASS
68	69	0.00	2	0.8	128	PASS
69	198	0.00	100	28.1	16795	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	35.5	21192	PASS
197	198	0.00	2	0.2	133	PASS
198	198	100	100	100.0	59749	PASS
199	198	5	9	6.3	3756	PASS
275	198	10	60	37.9	22648	PASS
365	198	1	100	6.3	3754	PASS
441	198	0.01	100	22.1	13205	PASS
442	442	50	100	100.0	82829	PASS
443	442	15	24	19.3	16021	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061002.D
Acq On : 23 Apr 2024 10:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 23 12:58:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

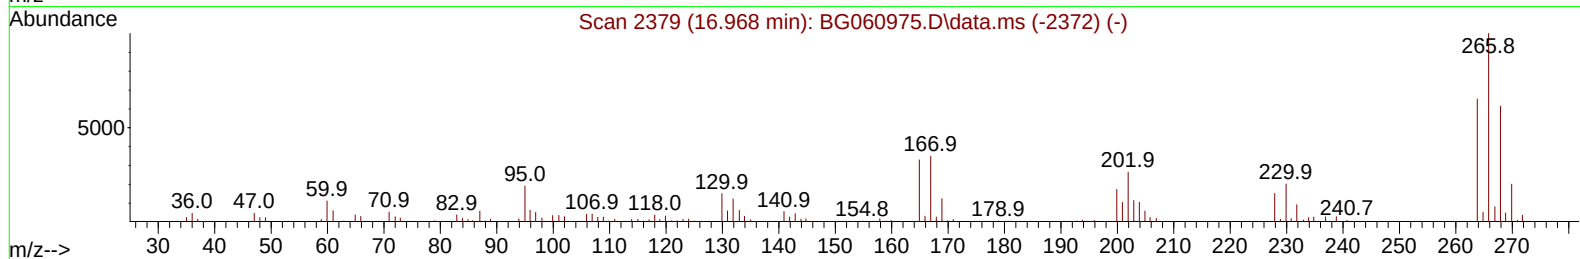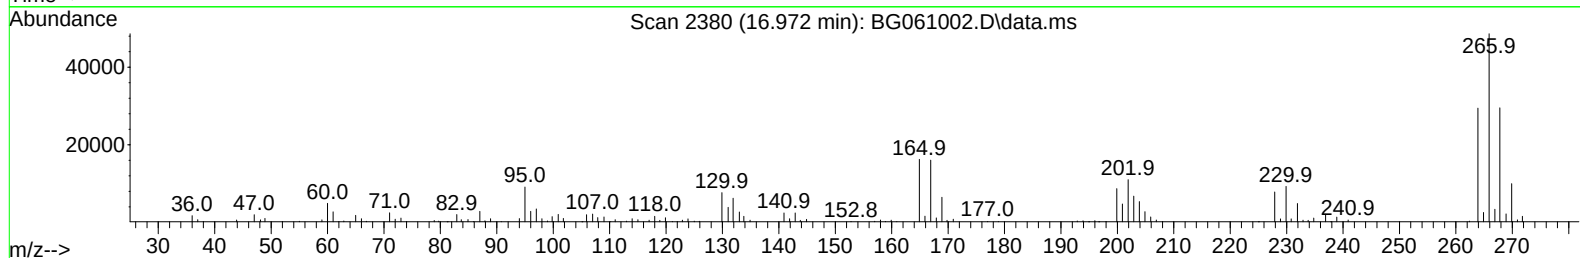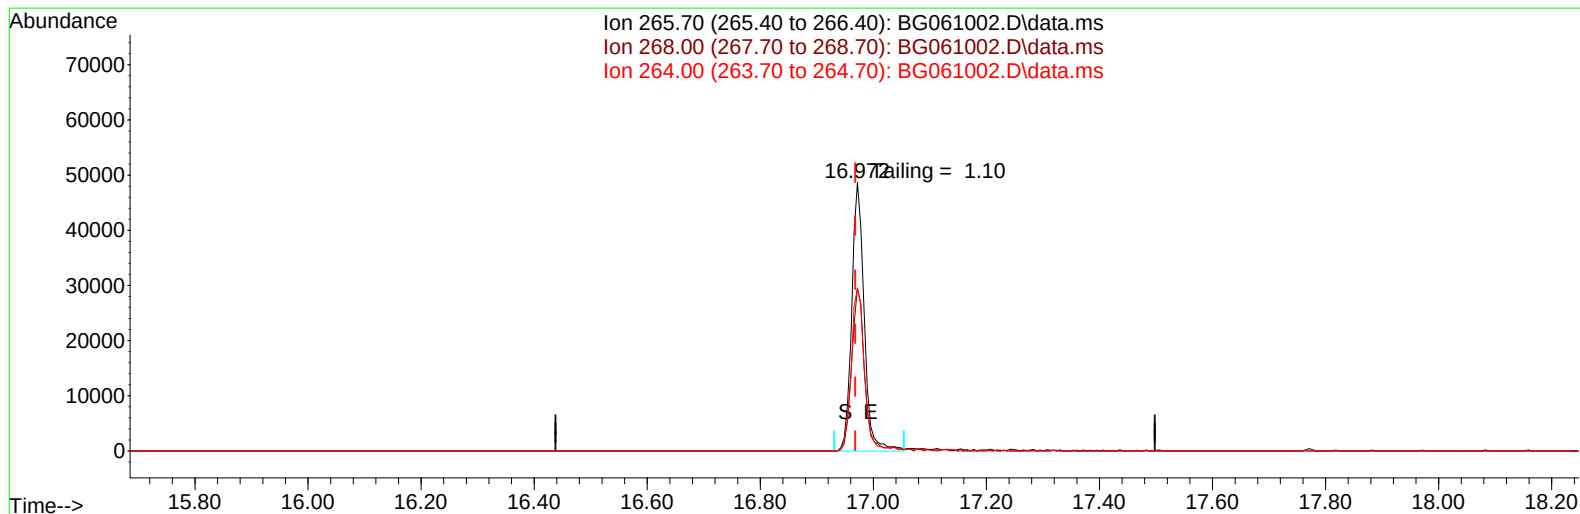

TIC: BG061002.D\data.ms

(70) Pentachlorophenol (C)

16.972min (+ 0.004) 28935.08 ng




response 74679

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	60.73
264.00	65.20	60.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042324\
Data File : BG061002.D
Acq On : 23 Apr 2024 10:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 23 12:58:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

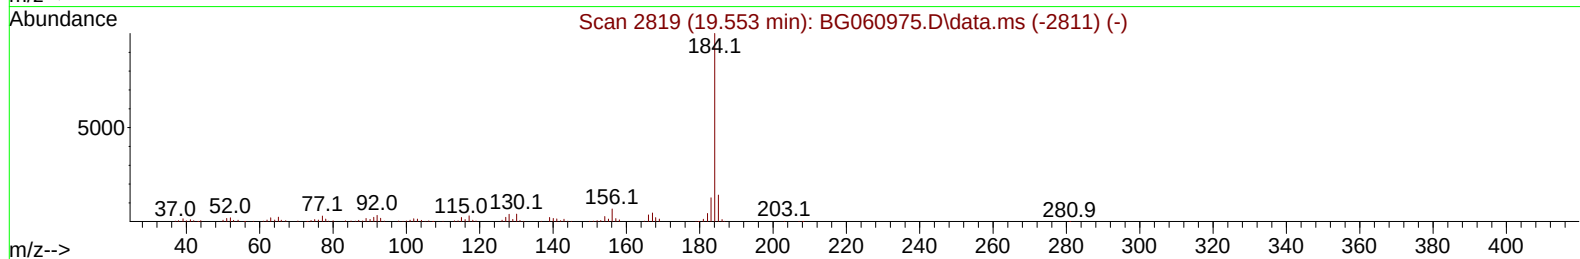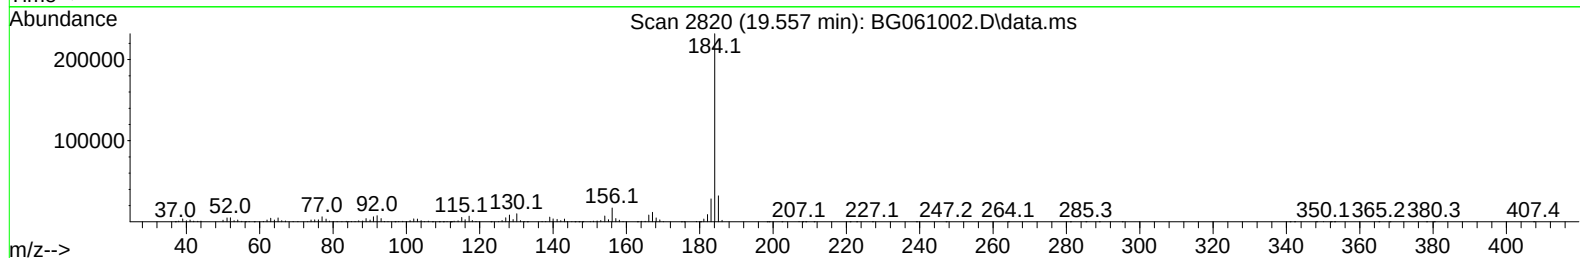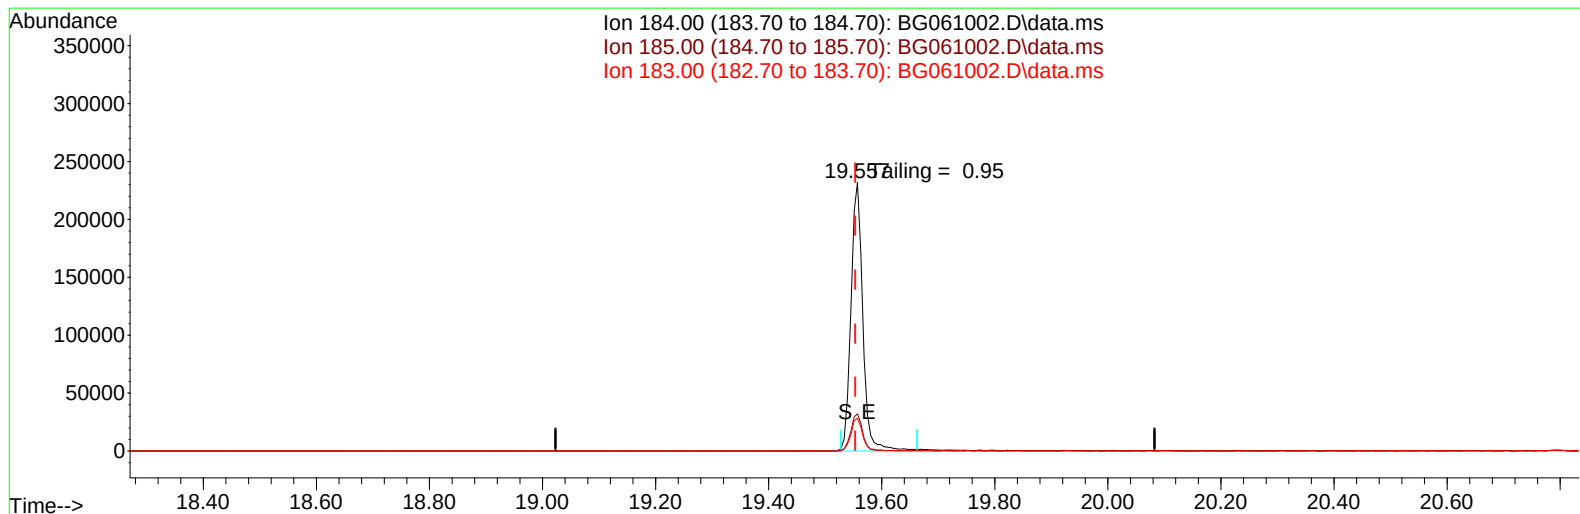

TIC: BG061002.D\data.ms

(77) Benzidine

19.557min (+ 0.004) 72117.87 ng

response 328721

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.87
183.00	12.70	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/23/2024	BNA_G	<u>BG061002.D</u>
Compound Name	Response	Retention Time
DDT	204256	20.797
DDD	11401	20.356
DDE	902	19.851
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12303	216559	5.68

Instrument :
BNA_G
ClientSampleId :
DFTPP