

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042415\
 Data File : BG016701.D
 Acq On : 25 Apr 2015 2:57
 Operator : TP/IZ
 Sample : G1992-14
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TEC02

Quant Time: Apr 25 04:35:51 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 24 22:57:52 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	51312	20.00	ng	0.00
21) Naphthalene-d8	10.38	136	207436	20.00	ng	0.00
38) Acenaphthene-d10	14.25	164	112882	20.00	ng	0.00
63) Phenanthrene-d10	16.99	188	243210	20.00	ng	0.00
75) Chrysene-d12	21.18	240	232646	20.00	ng	0.00
86) Perylene-d12	23.38	264	192711	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	438846	138.78	ng	0.00
7) Phenol-d6	6.80	99	557254	125.62	ng	0.00
23) Nitrobenzene-d5	8.75	82	318004	96.87	ng	0.00
41) 2,4,6-Tribromophenol	15.74	330	136975	163.57	ng	0.00
44) 2-Fluorobiphenyl	12.87	172	716797	102.02	ng	0.00
78) Terphenyl-d14	19.63	244	924142	91.50	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042415\
Data File : BG016701.D
Acq On : 25 Apr 2015 2:57
Operator : TP/IZ
Sample : G1992-14
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TEC02

Quant Time: Apr 25 04:35:51 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 24 22:57:52 2015
Response via : Initial Calibration

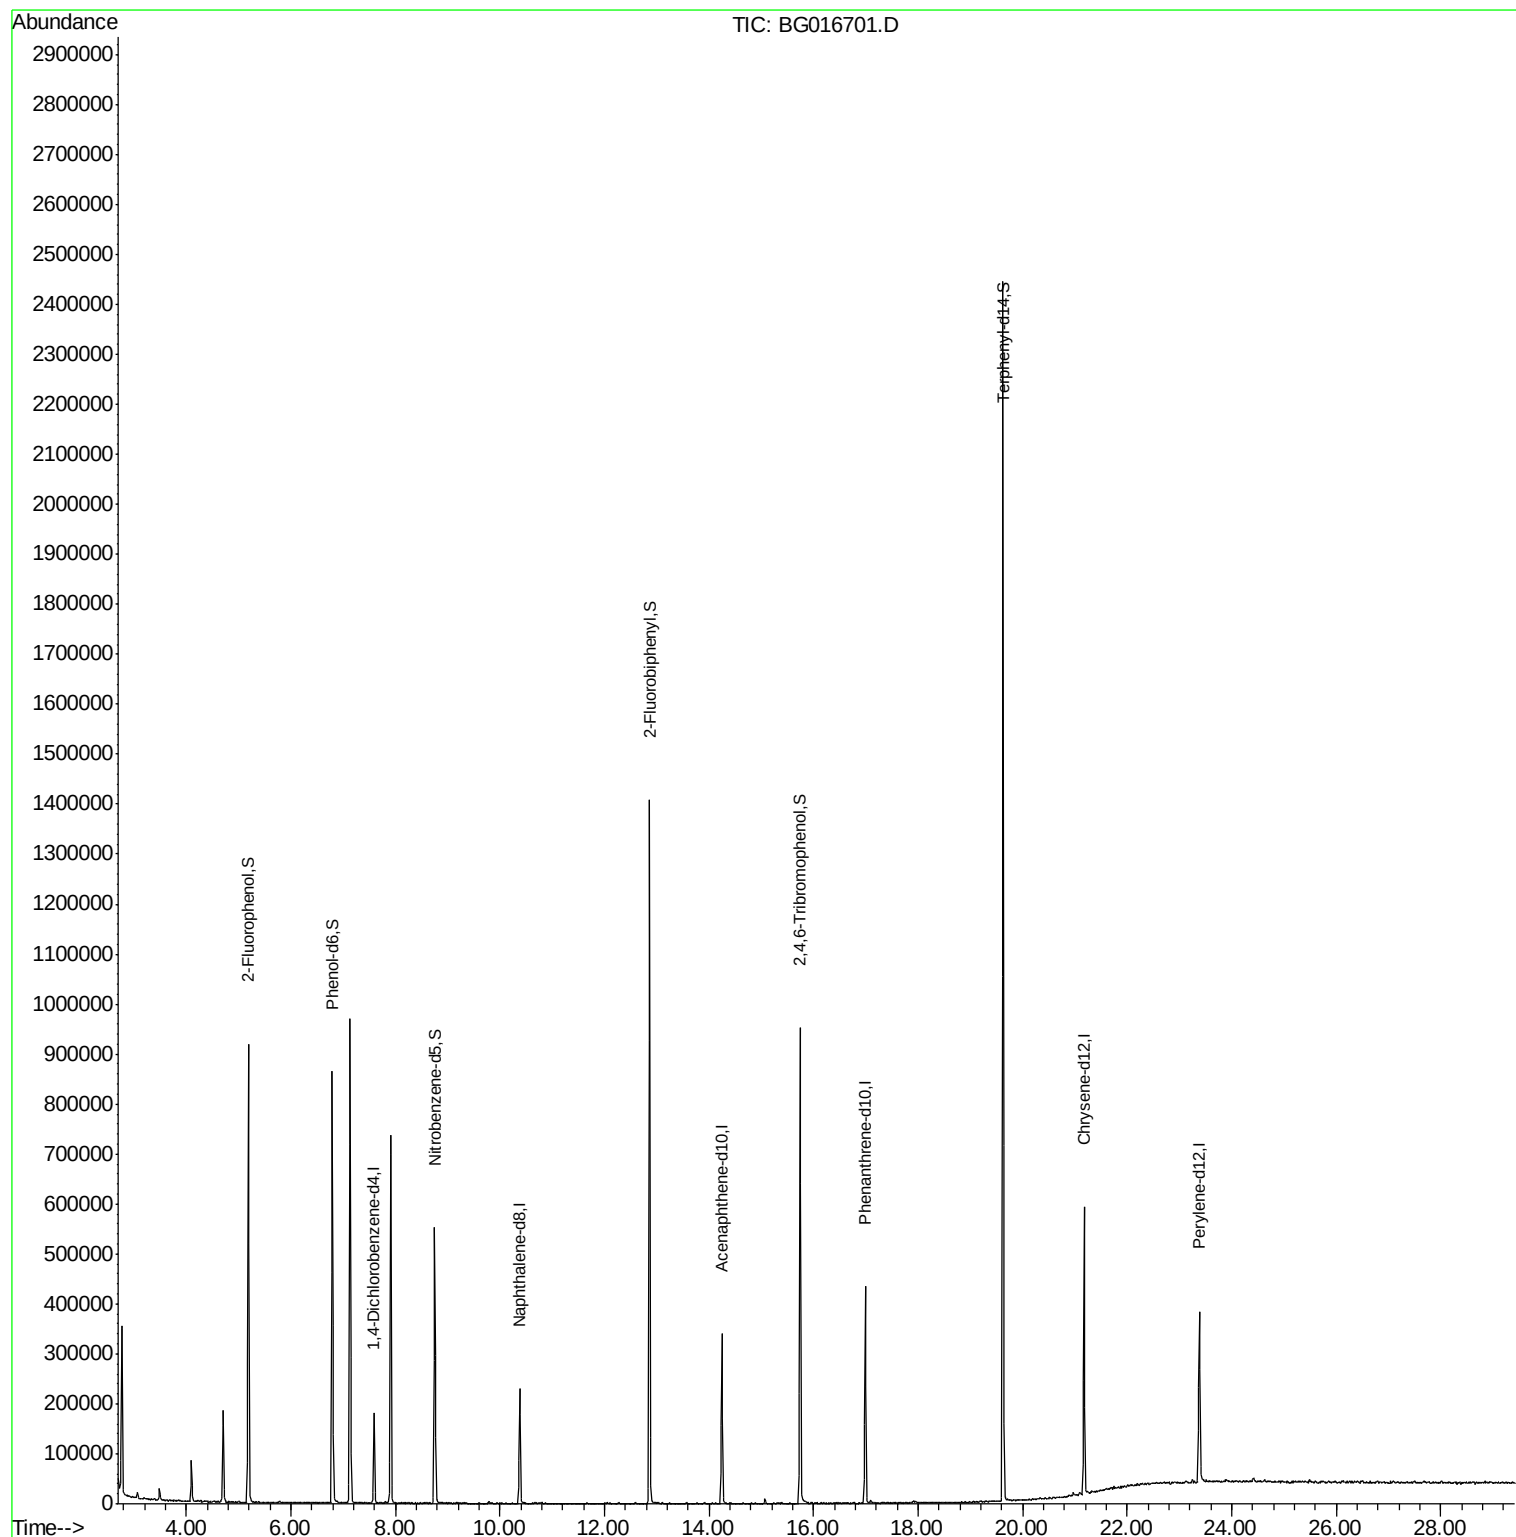

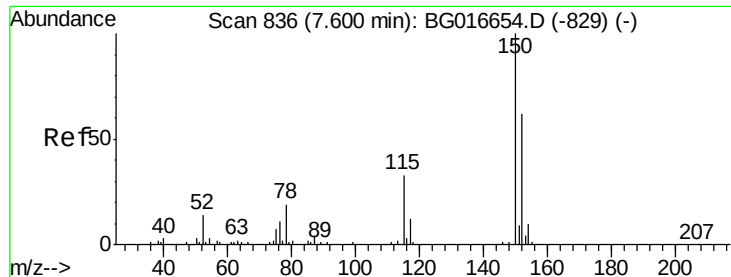

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.59 min Scan# 834

Delta R.T. -0.00 min

Lab File: BG016701.D

Acq: 25 Apr 2015 2:57

Instrument :

BNA_G

ClientSampleId :

TEC02


Tgt Ion:152 Resp: 51312

Ion Ratio Lower Upper

152 100

150 151.4 129.6 194.4




115 54.7 43.0 64.6

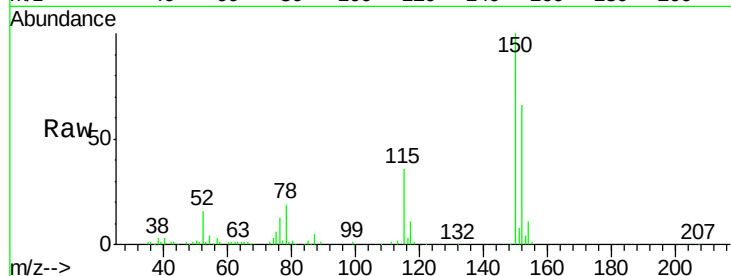

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

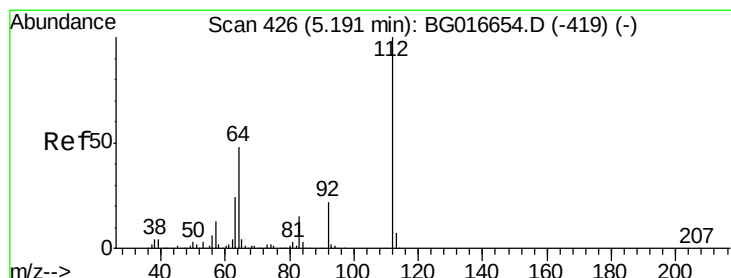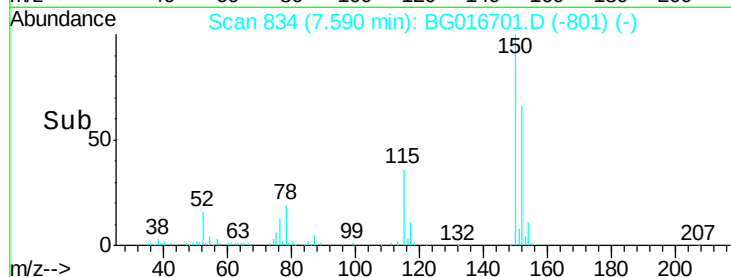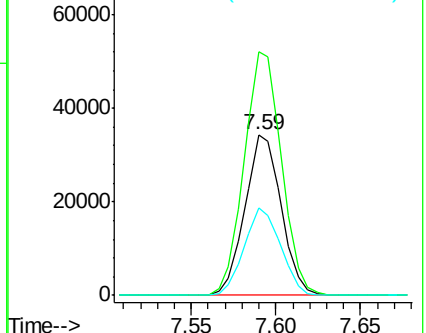

#5

2-Fluorophenol

Concen: 138.78 ng

RT: 5.19 min Scan# 425

Delta R.T. 0.00 min

Lab File: BG016701.D

Acq: 25 Apr 2015 2:57


Tgt Ion:112 Resp: 438846

Ion Ratio Lower Upper

112 100

64 48.8 38.3 57.5



63 23.5 18.9 28.3

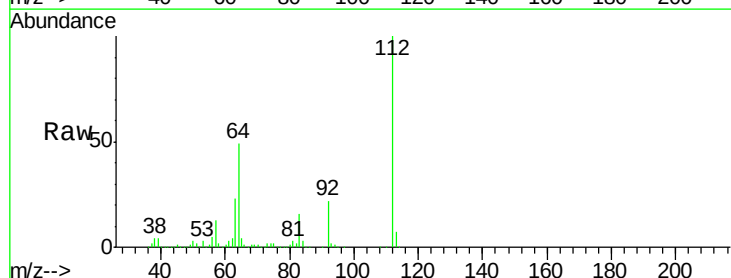


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

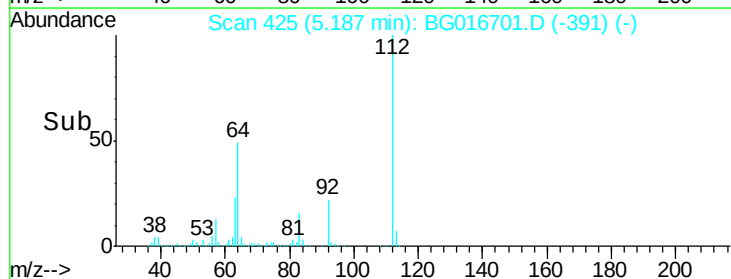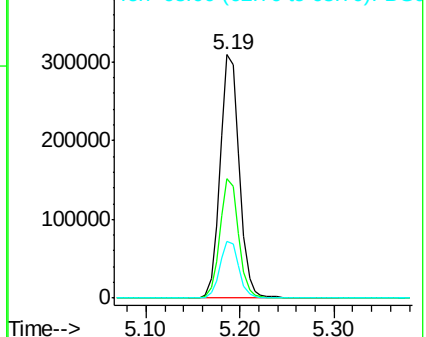

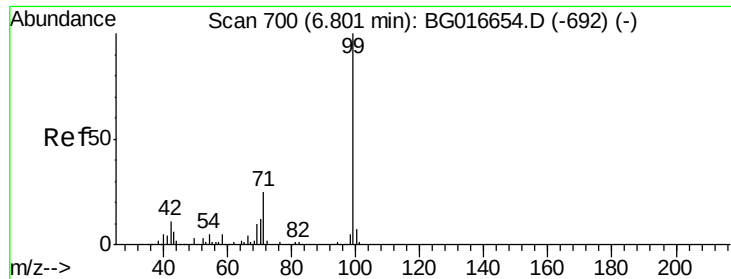

#7

Phenol-d6

Concen: 125.62 ng

RT: 6.80 min Scan# 699

Delta R.T. 0.01 min

Lab File: BG016701.D

Acq: 25 Apr 2015 2:57

Instrument :

BNA_G

ClientSampleId :

TEC02


Tgt Ion: 99 Resp: 557254

Ion Ratio Lower Upper




99 100

42 11.4 8.8 13.2

71 25.0 19.9 29.9

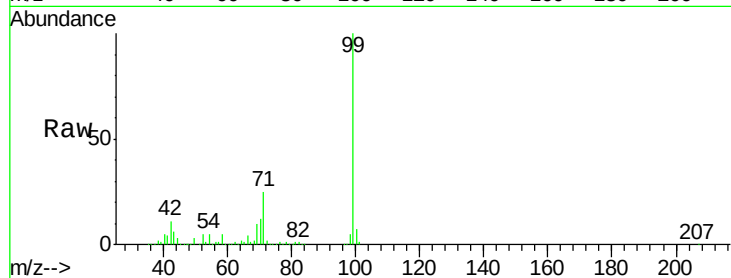

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

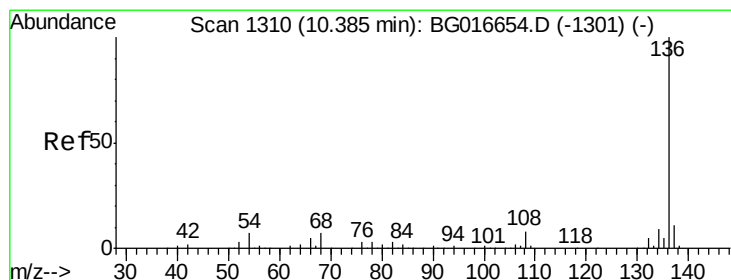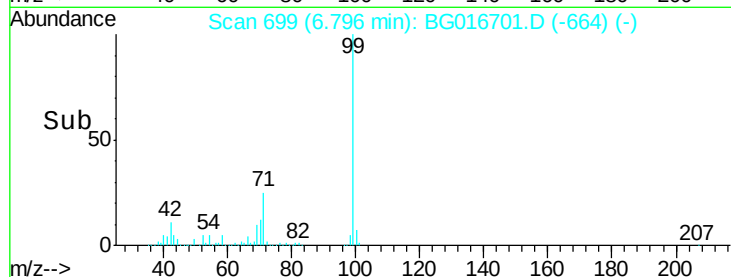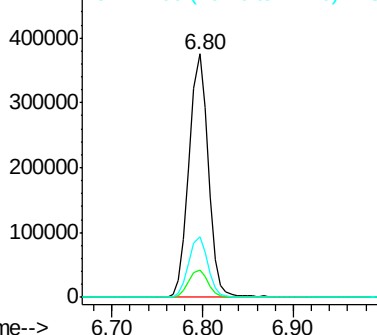

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.38 min Scan# 1309

Delta R.T. 0.00 min

Lab File: BG016701.D

Acq: 25 Apr 2015 2:57

Tgt Ion: 136 Resp: 207436


Ion Ratio Lower Upper

136 100



137 10.5 8.5 12.7


54 5.9 5.4 8.2

68 6.1 5.2 7.8

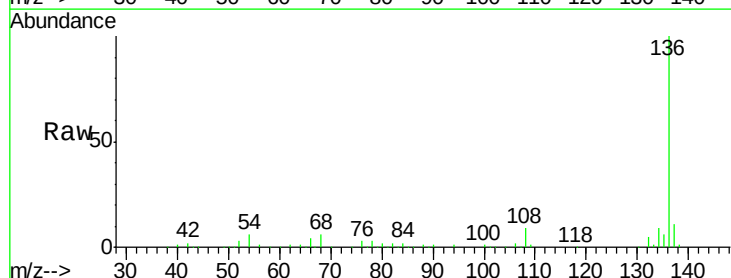

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

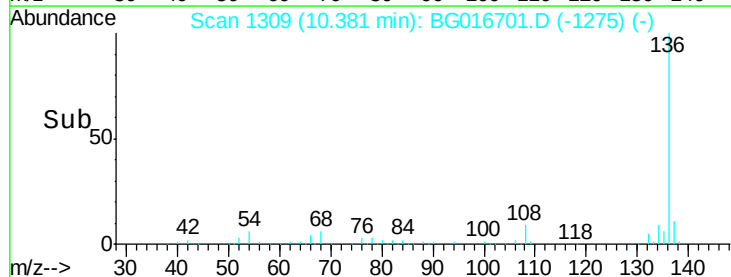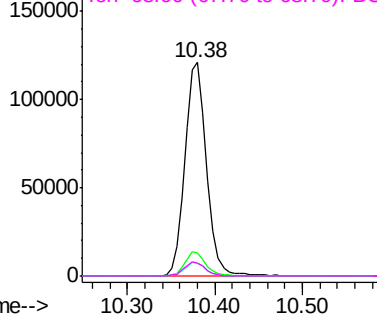


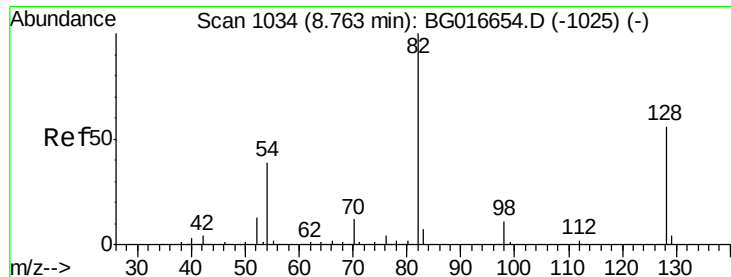




#23
 Nitrobenzene-d5
 Concen: 96.87 ng
 RT: 8.75 min Scan# 1032
 Delta R.T. 0.00 min
 Lab File: BG016701.D
 Acq: 25 Apr 2015 2:57

Instrument :
 BNA_G
 ClientSampleId :
 TEC02

Tgt Ion: 82 Resp: 318004
 Ion Ratio Lower Upper
 82 100
 128 53.6 44.7 67.1
 54 38.1 30.9 46.3

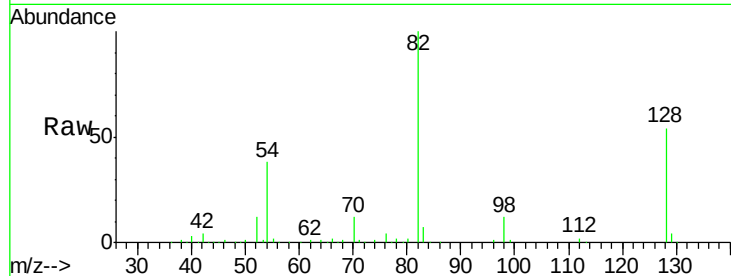


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

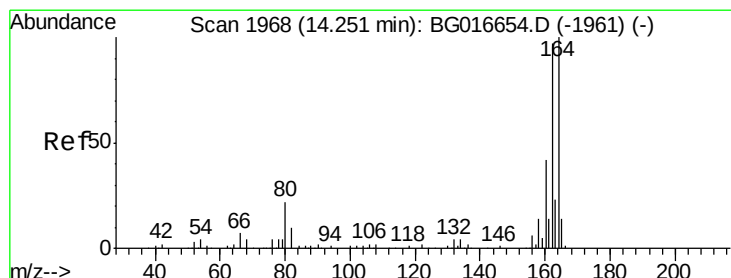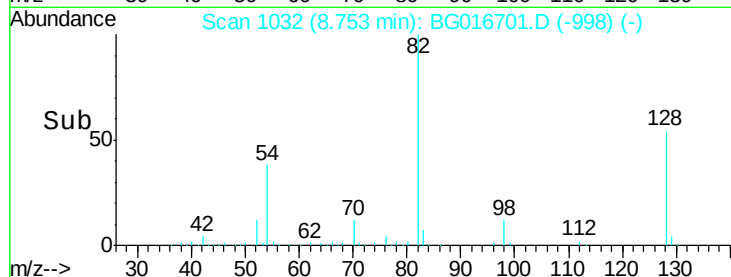
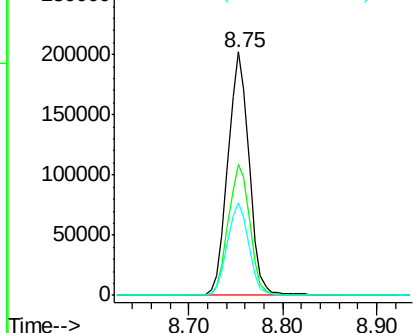



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.25 min Scan# 1967
 Delta R.T. -0.00 min
 Lab File: BG016701.D
 Acq: 25 Apr 2015 2:57

Tgt Ion: 164 Resp: 112882
 Ion Ratio Lower Upper
 164 100
 162 95.6 77.3 115.9
 160 43.9 33.7 50.5

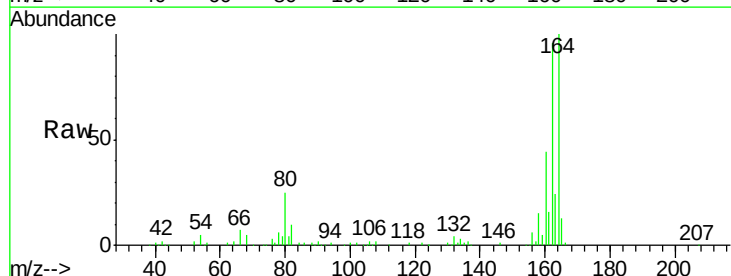

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

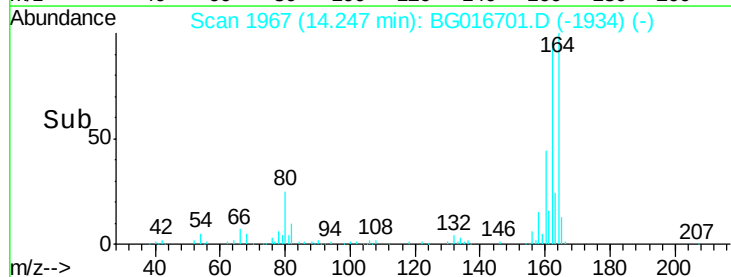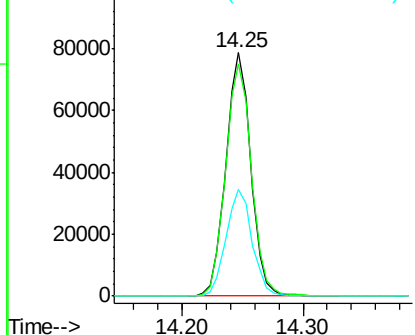


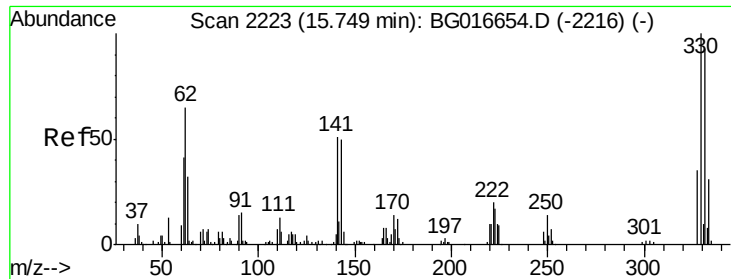




#41
 2,4,6-Tribromophenol
 Concen: 163.57 ng
 RT: 15.74 min Scan# 2222
 Delta R.T. 0.00 min
 Lab File: BG016701.D
 Acq: 25 Apr 2015 2:57

Instrument :
 BNA_G
 ClientSampleId :
 TEC02

Tgt Ion: 330 Resp: 136975
 Ion Ratio Lower Upper
 330 100
 332 93.6 76.2 114.4
 141 53.4 43.0 64.6

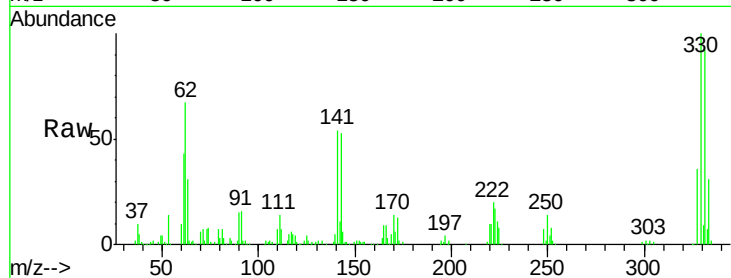


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

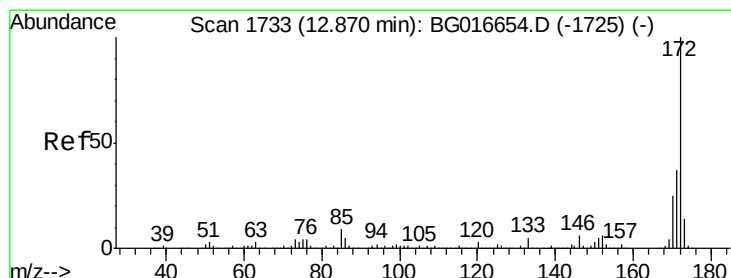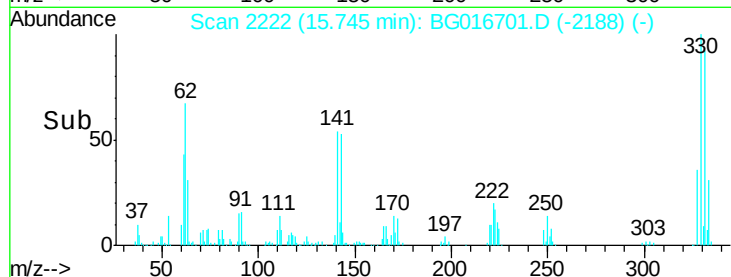
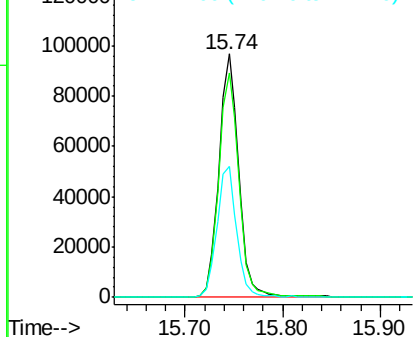



#44
 2-Fluorobiphenyl
 Concen: 102.02 ng
 RT: 12.87 min Scan# 1732
 Delta R.T. 0.00 min
 Lab File: BG016701.D
 Acq: 25 Apr 2015 2:57

Tgt Ion: 172 Resp: 716797
 Ion Ratio Lower Upper
 172 100
 171 37.1 29.9 44.9
 170 24.3 19.8 29.8

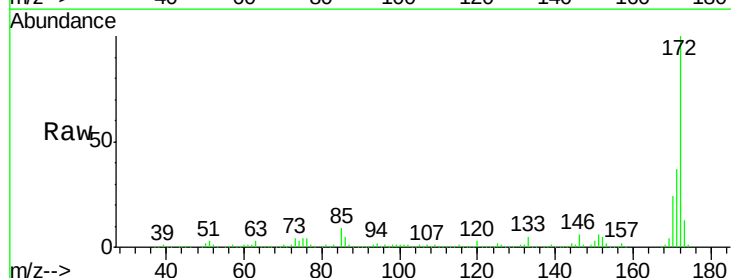

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

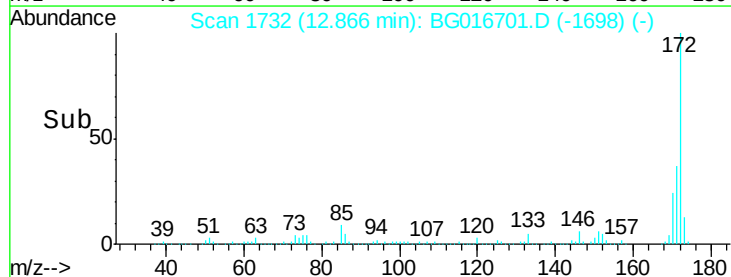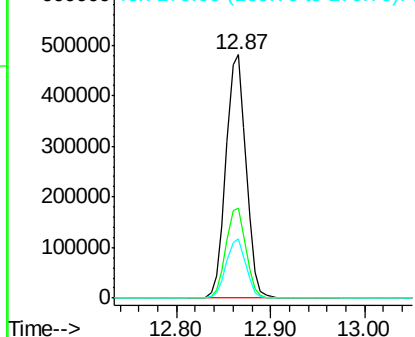


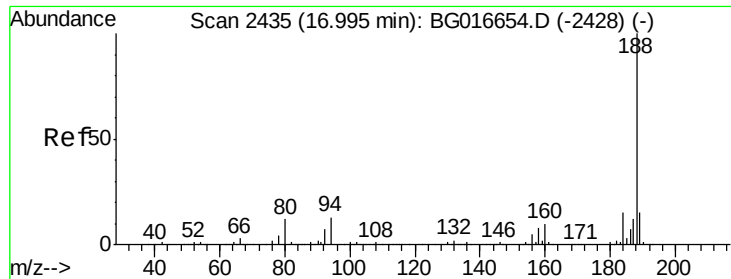




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 16.99 min Scan# 2434
Delta R.T. -0.00 min
Lab File: BG016701.D
Acq: 25 Apr 2015 2:57

Instrument :
BNA_G
ClientSampleId :
TEC02

Tgt Ion:188 Resp: 243210
Ion Ratio Lower Upper
188 100
94 12.1 10.7 16.1
80 13.1 9.9 14.9

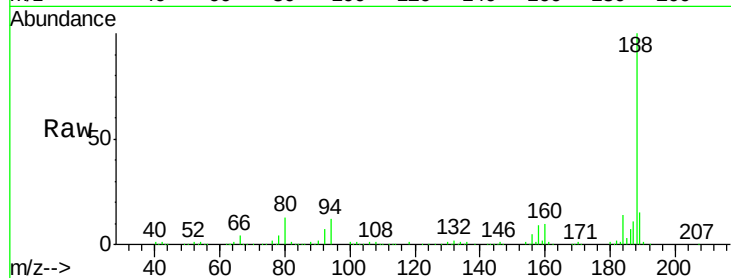


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): B
Ion 80.00 (79.70 to 80.70): B

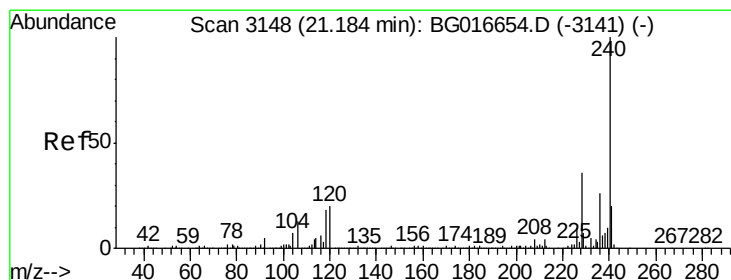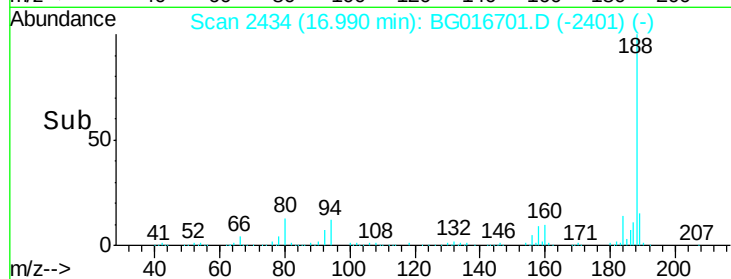
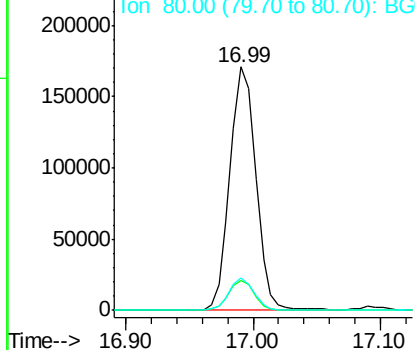



#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.18 min Scan# 3147
Delta R.T. -0.00 min
Lab File: BG016701.D
Acq: 25 Apr 2015 2:57

Tgt Ion:240 Resp: 232646
Ion Ratio Lower Upper
240 100
120 19.1 16.3 24.5
236 26.3 21.1 31.7

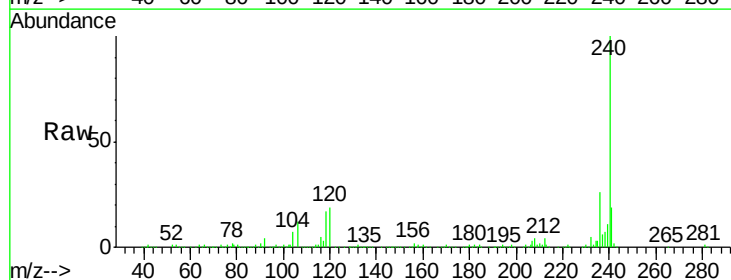

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

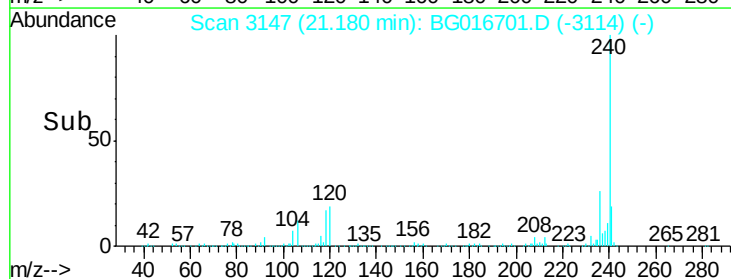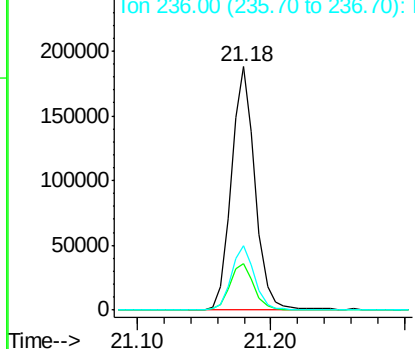

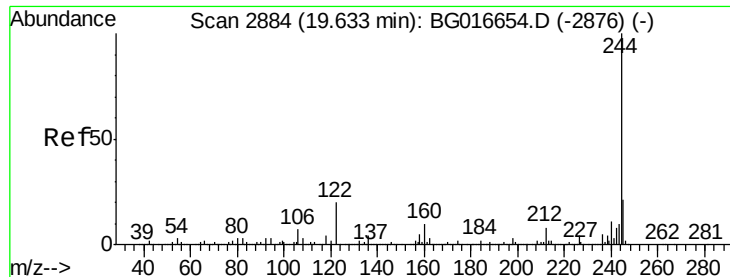

#78

Terphenyl-d14

Concen: 91.50 ng

RT: 19.63 min Scan# 2883

Delta R.T. 0.00 min

Lab File: BG016701.D

Acq: 25 Apr 2015 2:57

Instrument :

BNA_G

ClientSampleId :

TEC02


Tgt Ion:244 Resp: 924142

Ion Ratio Lower Upper

244 100

212 8.3 6.4 9.6




122 21.0 15.9 23.9

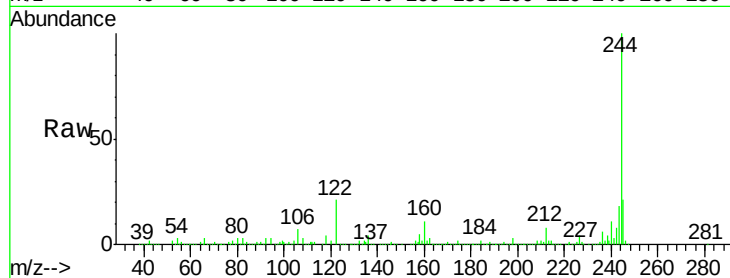

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

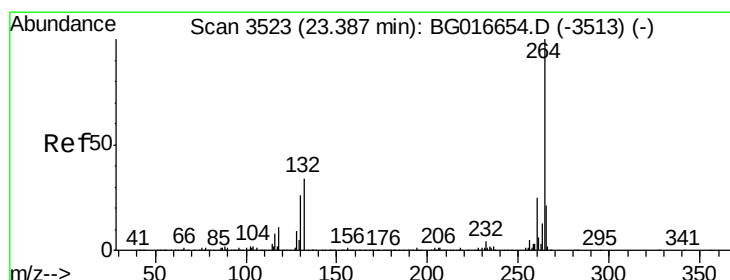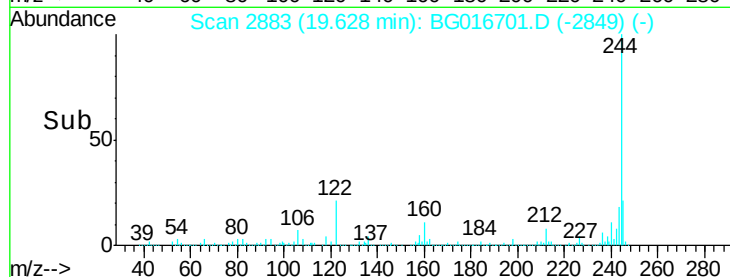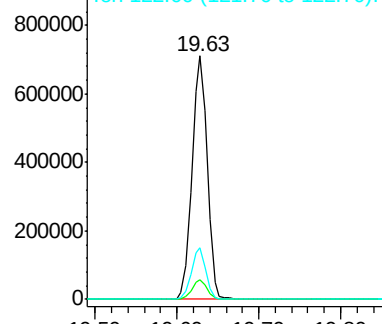

#86

Perylene-d12

Concen: 20.00 ng

RT: 23.38 min Scan# 3522

Delta R.T. -0.00 min

Lab File: BG016701.D

Acq: 25 Apr 2015 2:57


Tgt Ion:264 Resp: 192711

Ion Ratio Lower Upper

264 100

260 25.3 20.0 30.0

265 21.6 16.8 25.2

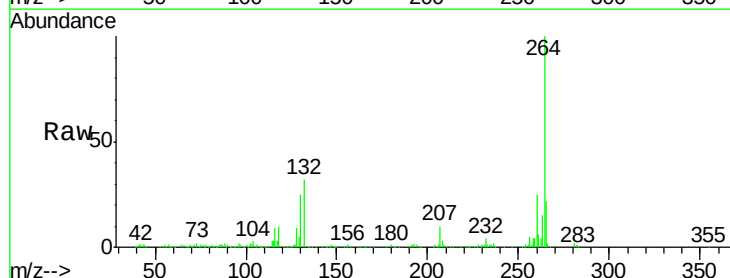

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

