


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042415\
 Data File : BG016703.D
 Acq On : 25 Apr 2015 6:07
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 24 22:57:52 2015

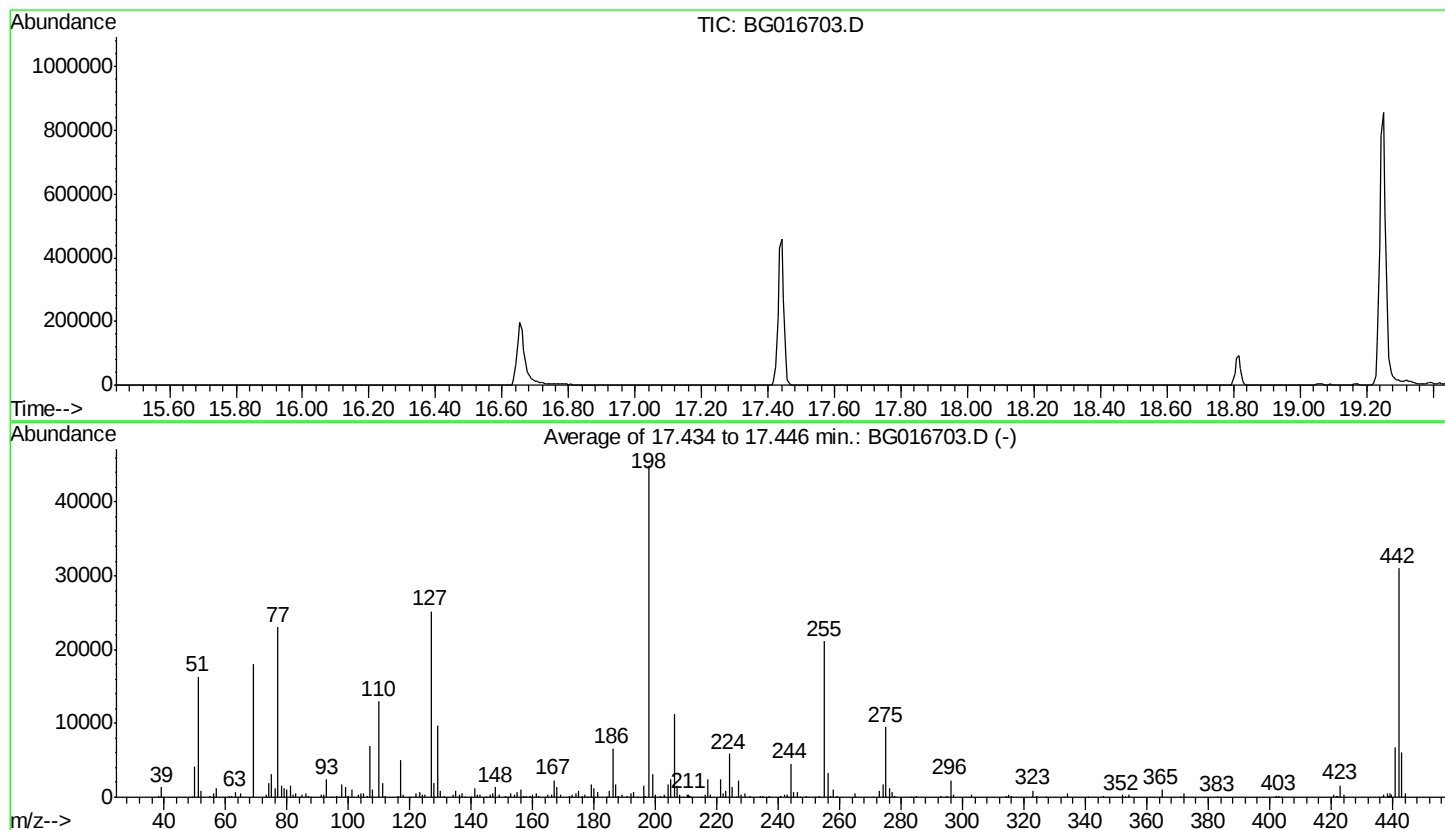

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	16346	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.0	17969	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.1	25213	PASS
197	198	0.00	2	0.3	135	PASS
198	198	100	100	100.0	44925	PASS
199	198	5	9	6.8	3049	PASS
275	198	10	60	21.2	9525	PASS
365	198	1	100	2.2	978	PASS
441	442	0.01	24	21.9	6790	PASS
442	198	50	100	69.1	31034	PASS
443	442	15	24	19.8	6159	PASS