


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG042415\
 Data File : BG016721.D
 Acq On : 25 Apr 2015 19:09
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 27 00:50:46 2015

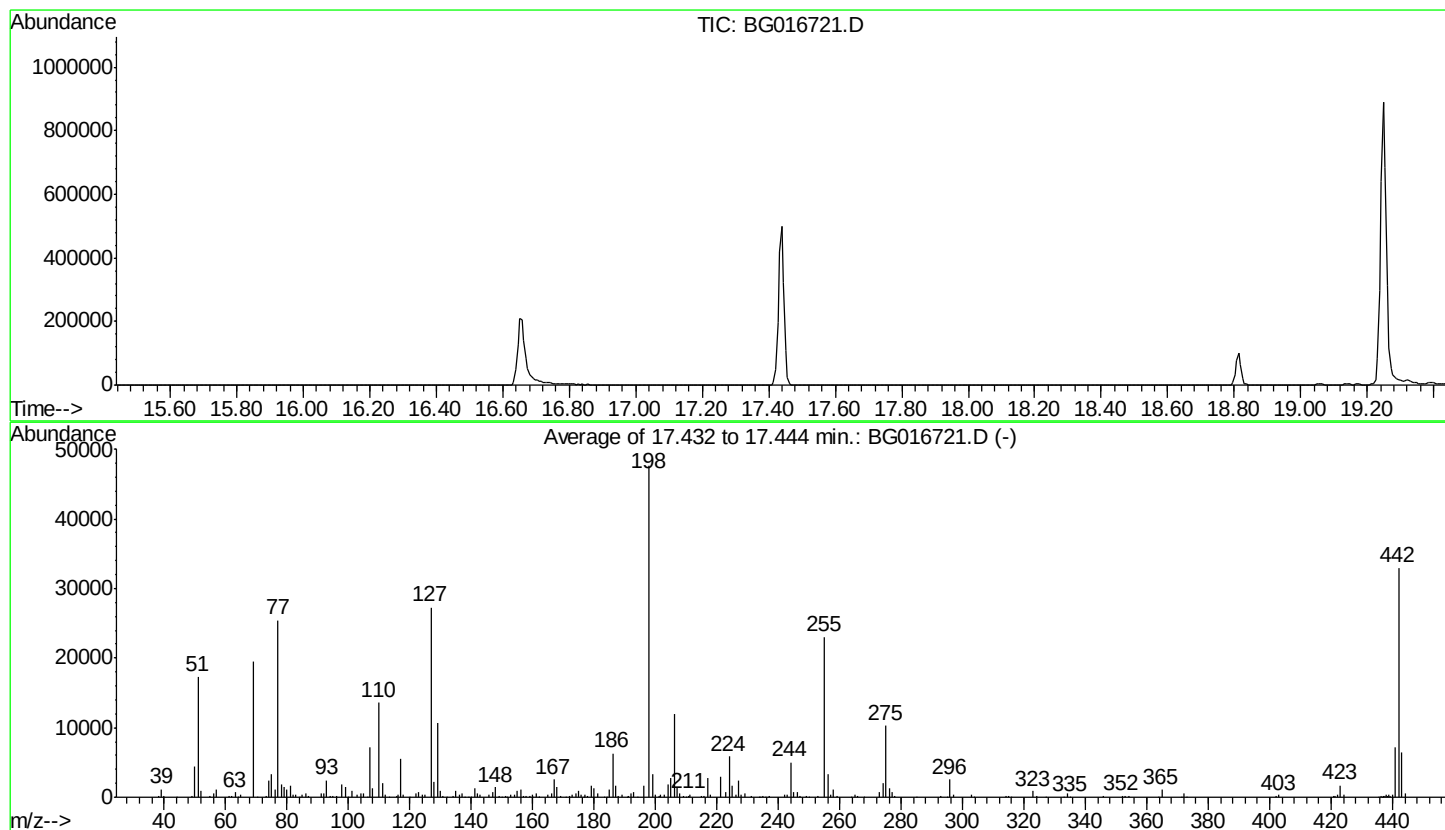

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	17358	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.1	19586	PASS
70	69	0.00	2	0.3	52	PASS
127	198	10	80	57.3	27298	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47645	PASS
199	198	5	9	7.2	3407	PASS
275	198	10	60	21.5	10247	PASS
365	198	1	100	2.2	1059	PASS
441	442	0.01	24	21.8	7202	PASS
442	198	50	100	69.2	32994	PASS
443	442	15	24	19.4	6388	PASS