
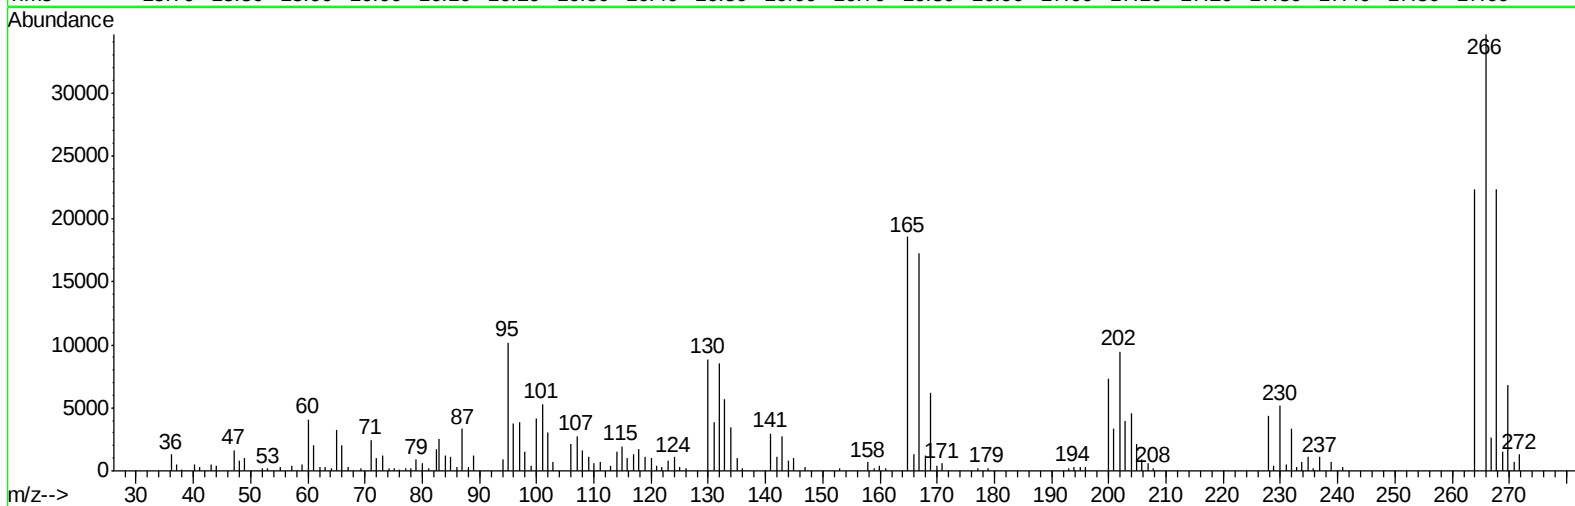


Data Path : Z:\HPCHEM1\BNA_G\Data\BG042415\
Data File : BG016684.D
Acq On : 24 Apr 2015 15:36
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:25:06 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

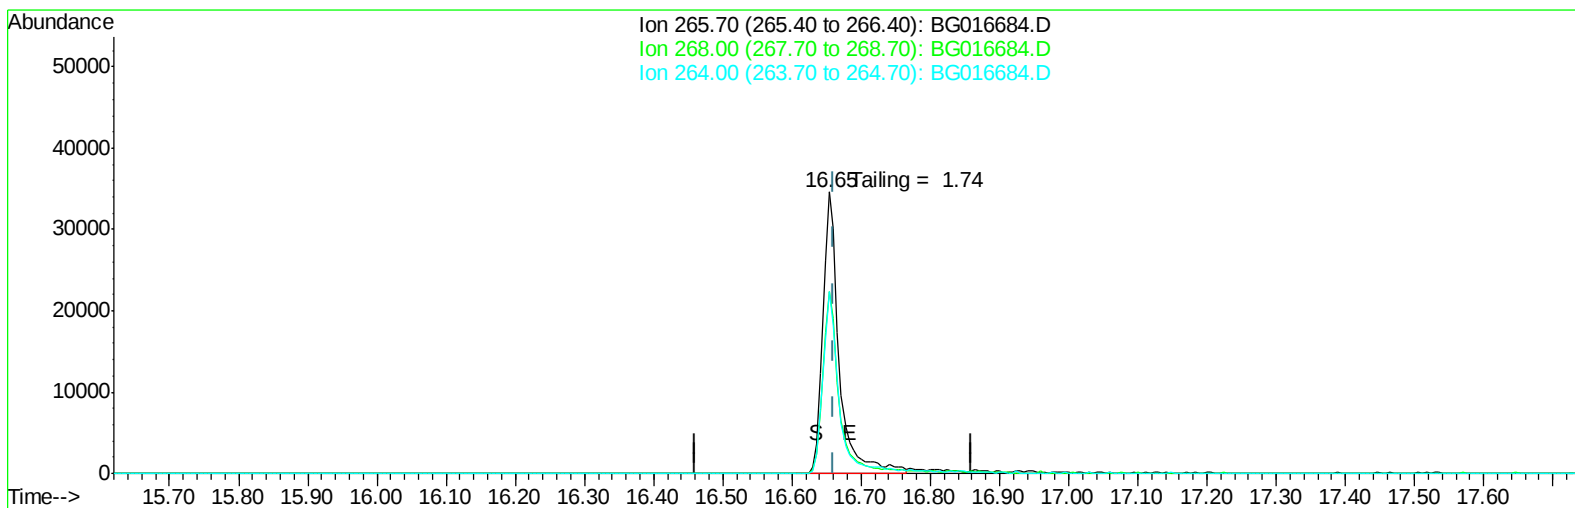

TIC: BG016684.D

(69) Pentachlorophenol (C)



16.654min (-0.006) 26805.94ng

response 55595

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	64.40
264.00	64.70	64.43
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG042415\
Data File : BG016684.D
Acq On : 24 Apr 2015 15:36
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:25:06 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

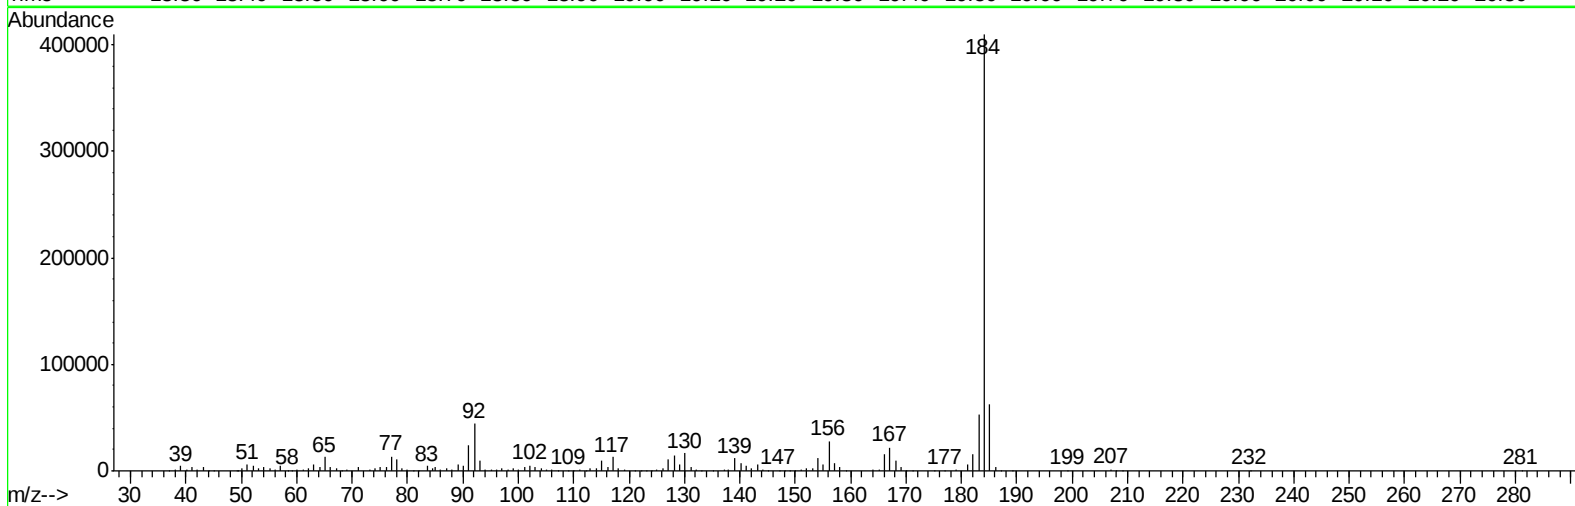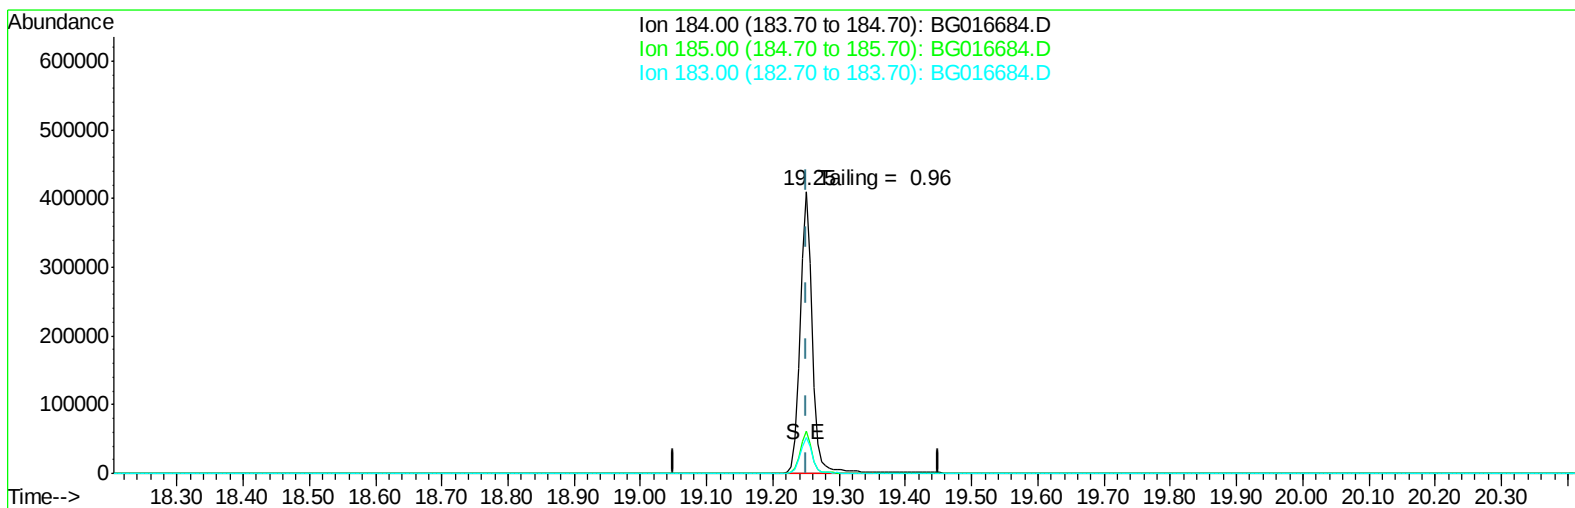

TIC: BG016684.D

(76) Benzidine

19.251min (-0.000) 15124.64ng

response 529037

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.15
183.00	12.60	12.81
0.00	0.00	0.00