
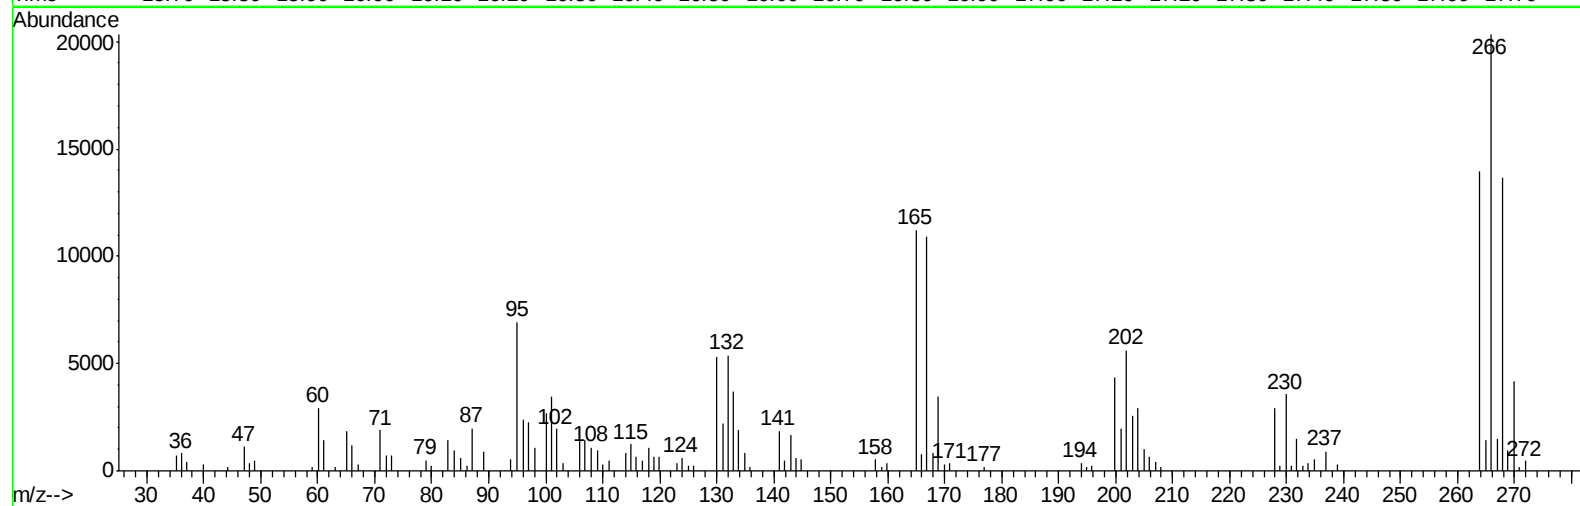


Data Path : Z:\HPCHEM1\BNA_G\Data\BG042415\
Data File : BG016703.D
Acq On : 25 Apr 2015 6:07
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:26:14 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

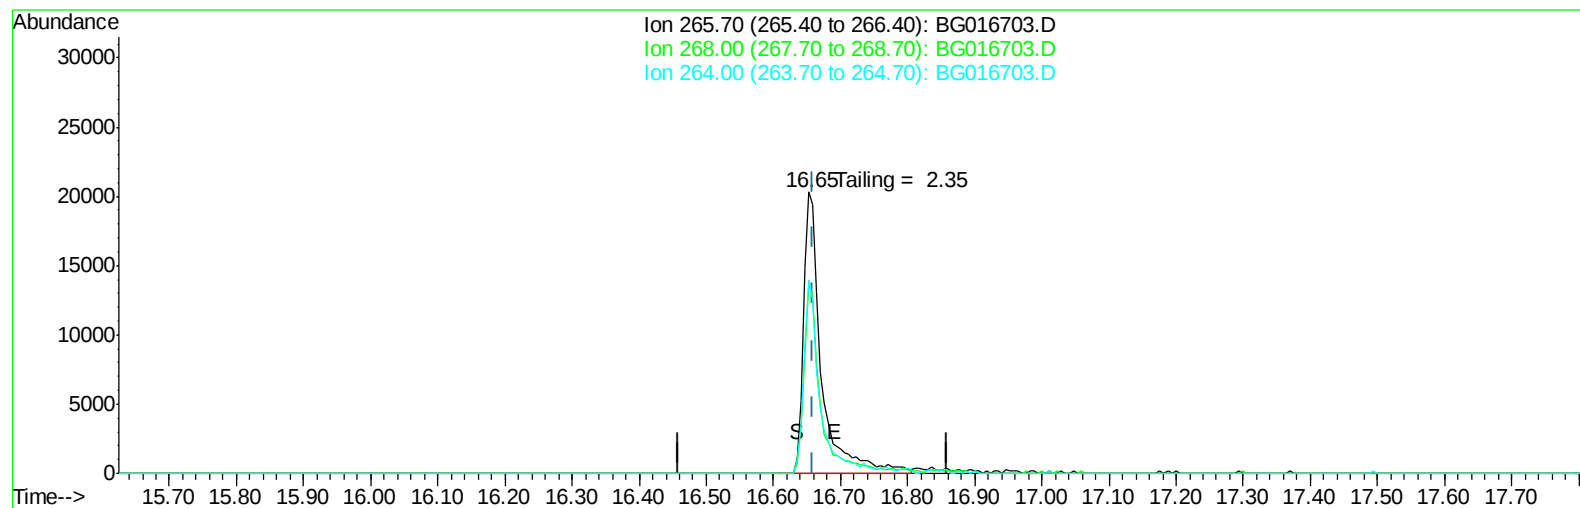

TIC: BG016703.D

(69) Pentachlorophenol (C)



16.653min (-0.007) 23653.72ng

response 38397

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	67.24
264.00	64.70	68.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG042415\
Data File : BG016703.D
Acq On : 25 Apr 2015 6:07
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:26:14 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

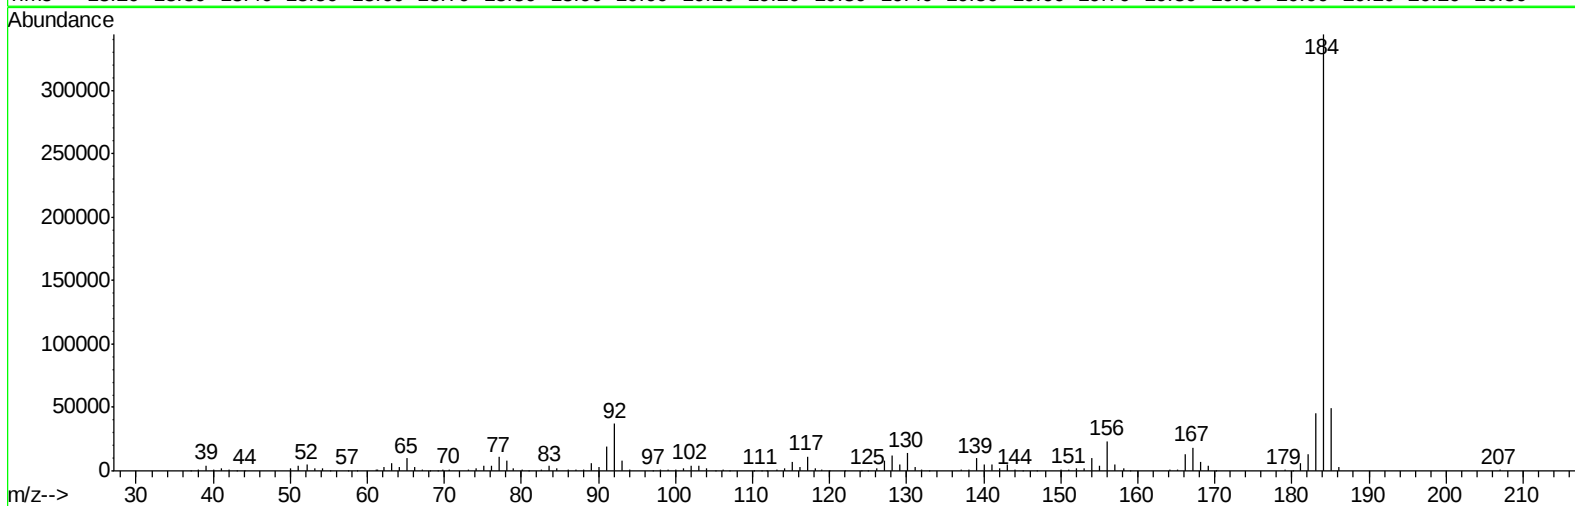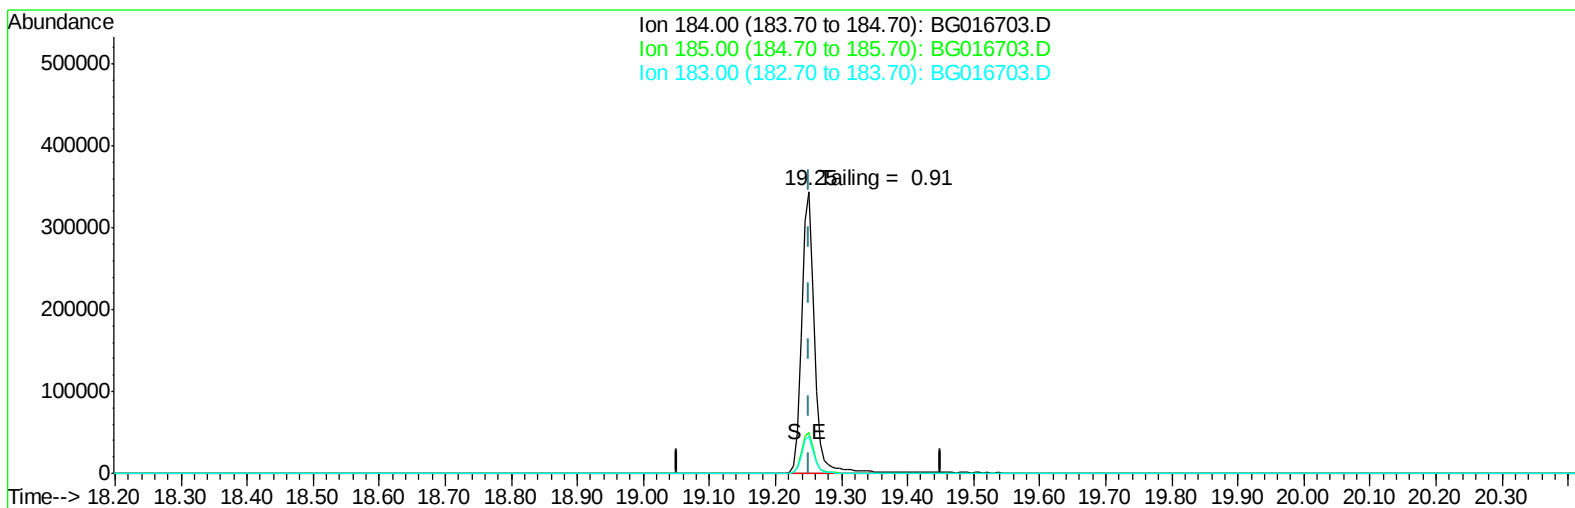

TIC: BG016703.D

(76) Benzidine

19.250min (-0.001) 23031.53ng

response 472226

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.44
183.00	12.60	13.27
0.00	0.00	0.00