
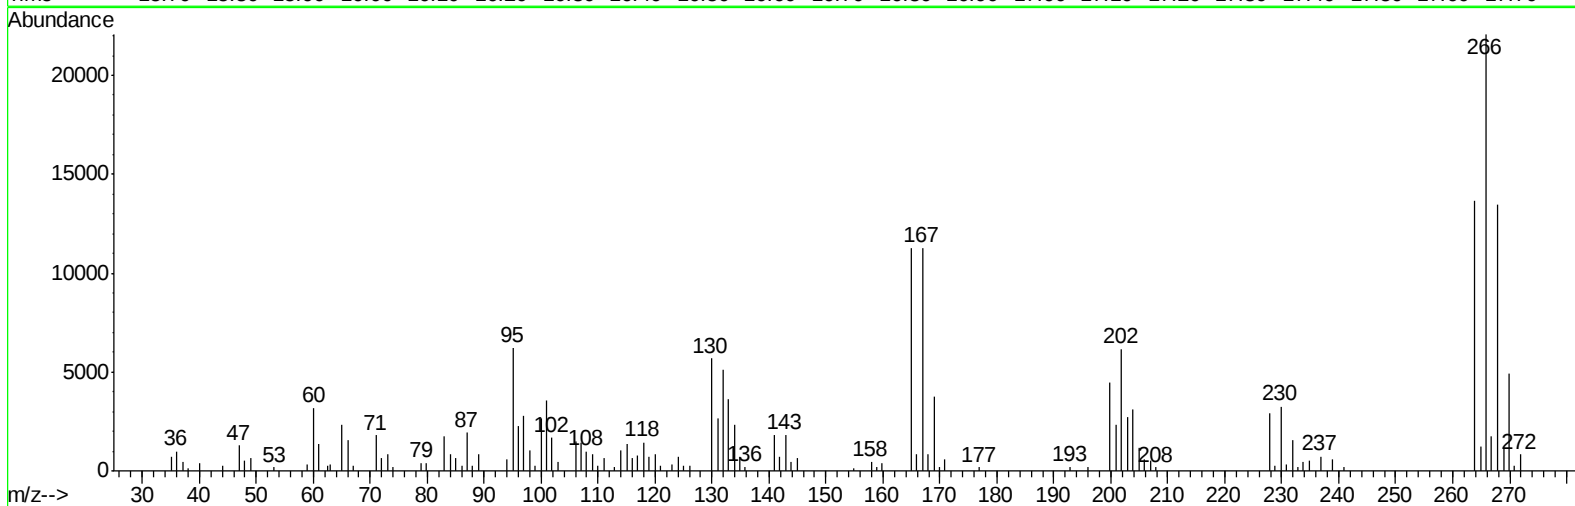


Data Path : Z:\HPCHEM1\BNA_G\Data\BG042415\
Data File : BG016721.D
Acq On : 25 Apr 2015 19:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:27:56 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

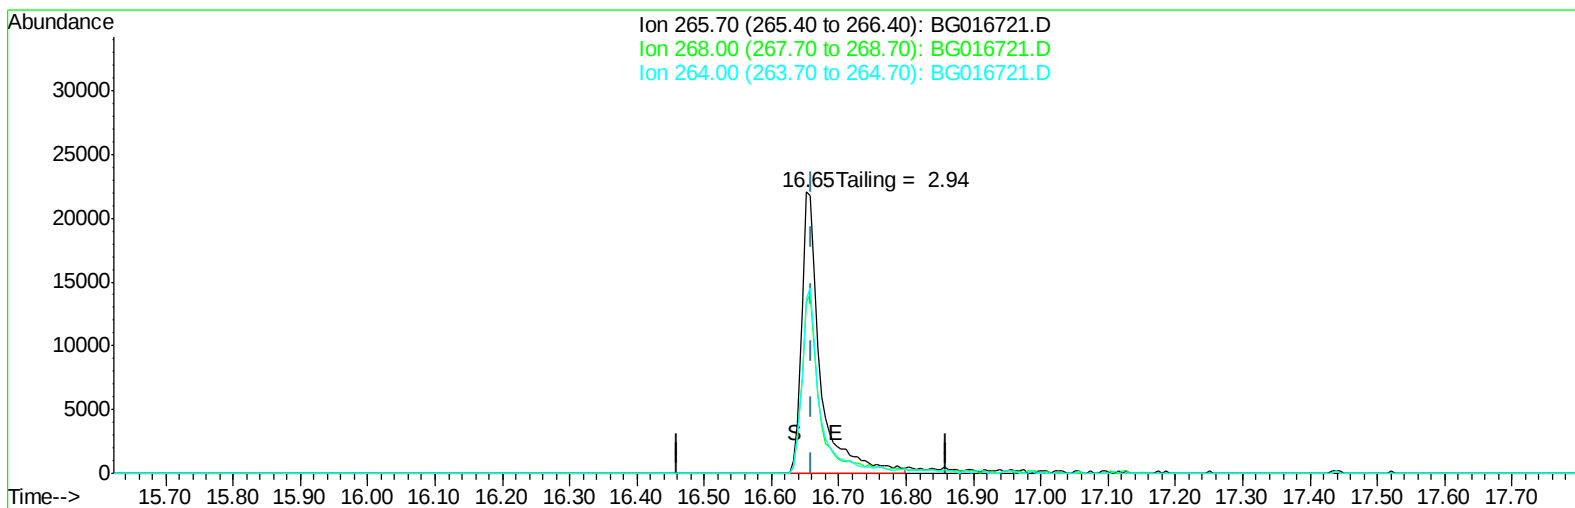

TIC: BG016721.D

(69) Pentachlorophenol (C)



16.651min (-0.009) 33433.11ng

response 42692

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	61.01
264.00	64.70	62.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG042415\
Data File : BG016721.D
Acq On : 25 Apr 2015 19:09
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 27 05:27:56 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 23 19:19:11 2015
Response via : Initial Calibration

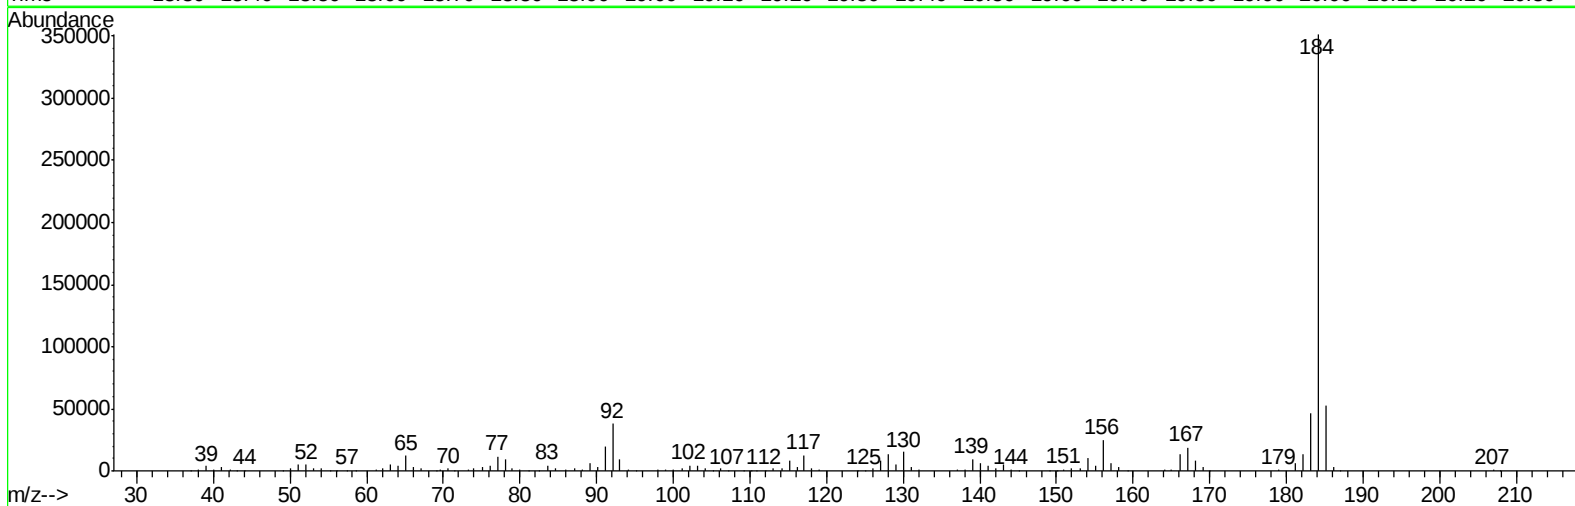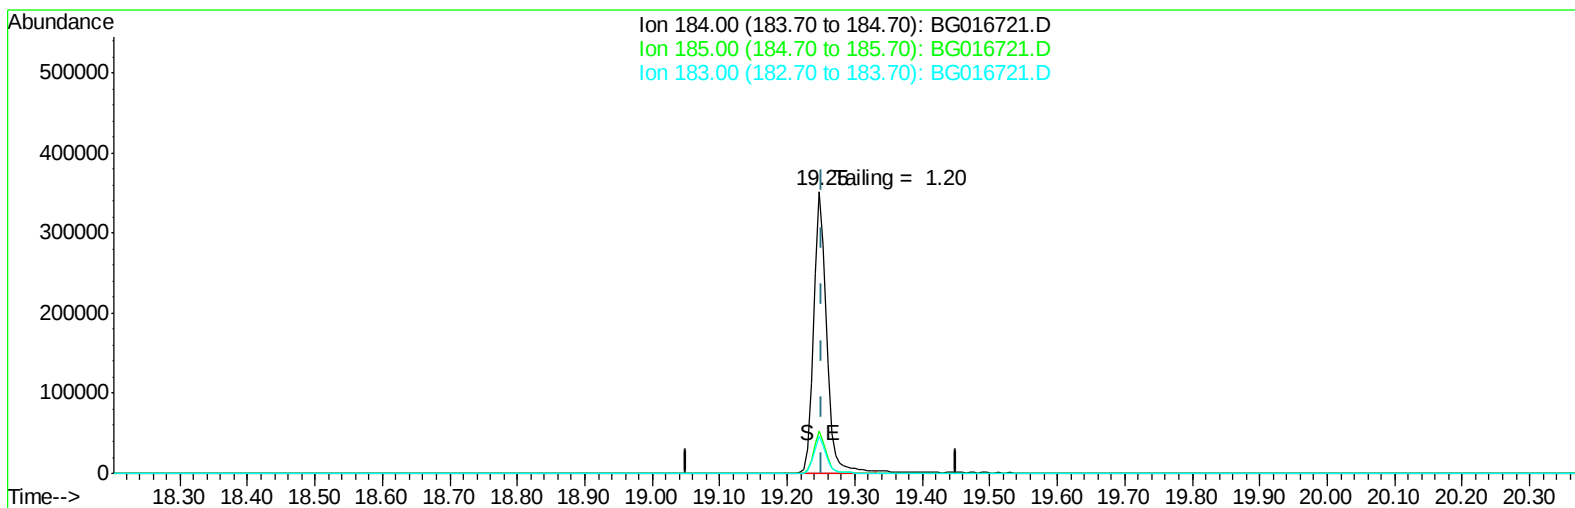

TIC: BG016721.D

(76) Benzidine

19.248min (-0.003) 23925.40ng

response 466922

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.94
183.00	12.60	13.23
0.00	0.00	0.00