

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042415\
 Data File : BG016725.D
 Acq On : 25 Apr 2015 22:03
 Operator : TP/IZ
 Sample : G1991-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SB-75D

Quant Time: Apr 27 02:00:59 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 27 01:43:02 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	53560	20.00	ng	0.00
21) Naphthalene-d8	10.38	136	227682	20.00	ng	0.00
38) Acenaphthene-d10	14.24	164	130627	20.00	ng	0.00
63) Phenanthrene-d10	16.99	188	280072	20.00	ng	0.00
75) Chrysene-d12	21.18	240	269869	20.00	ng	0.00
86) Perylene-d12	23.38	264	254519	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	424254	128.54	ng	0.00
7) Phenol-d6	6.79	99	579277	125.10	ng	0.00
23) Nitrobenzene-d5	8.75	82	282446	78.39	ng	0.00
41) 2,4,6-Tribromophenol	15.74	330	119548	123.36	ng	0.00
44) 2-Fluorobiphenyl	12.86	172	556624	68.46	ng	0.00
78) Terphenyl-d14	19.62	244	616856	52.65	ng	0.00
Target Compounds						
49) Dimethylphthalate	13.71	163	35449	3.63	ng	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042415\
Data File : BG016725.D
Acq On : 25 Apr 2015 22:03
Operator : TP/IZ
Sample : G1991-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SB-75D

Quant Time: Apr 27 02:00:59 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG042315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 27 01:43:02 2015
Response via : Initial Calibration

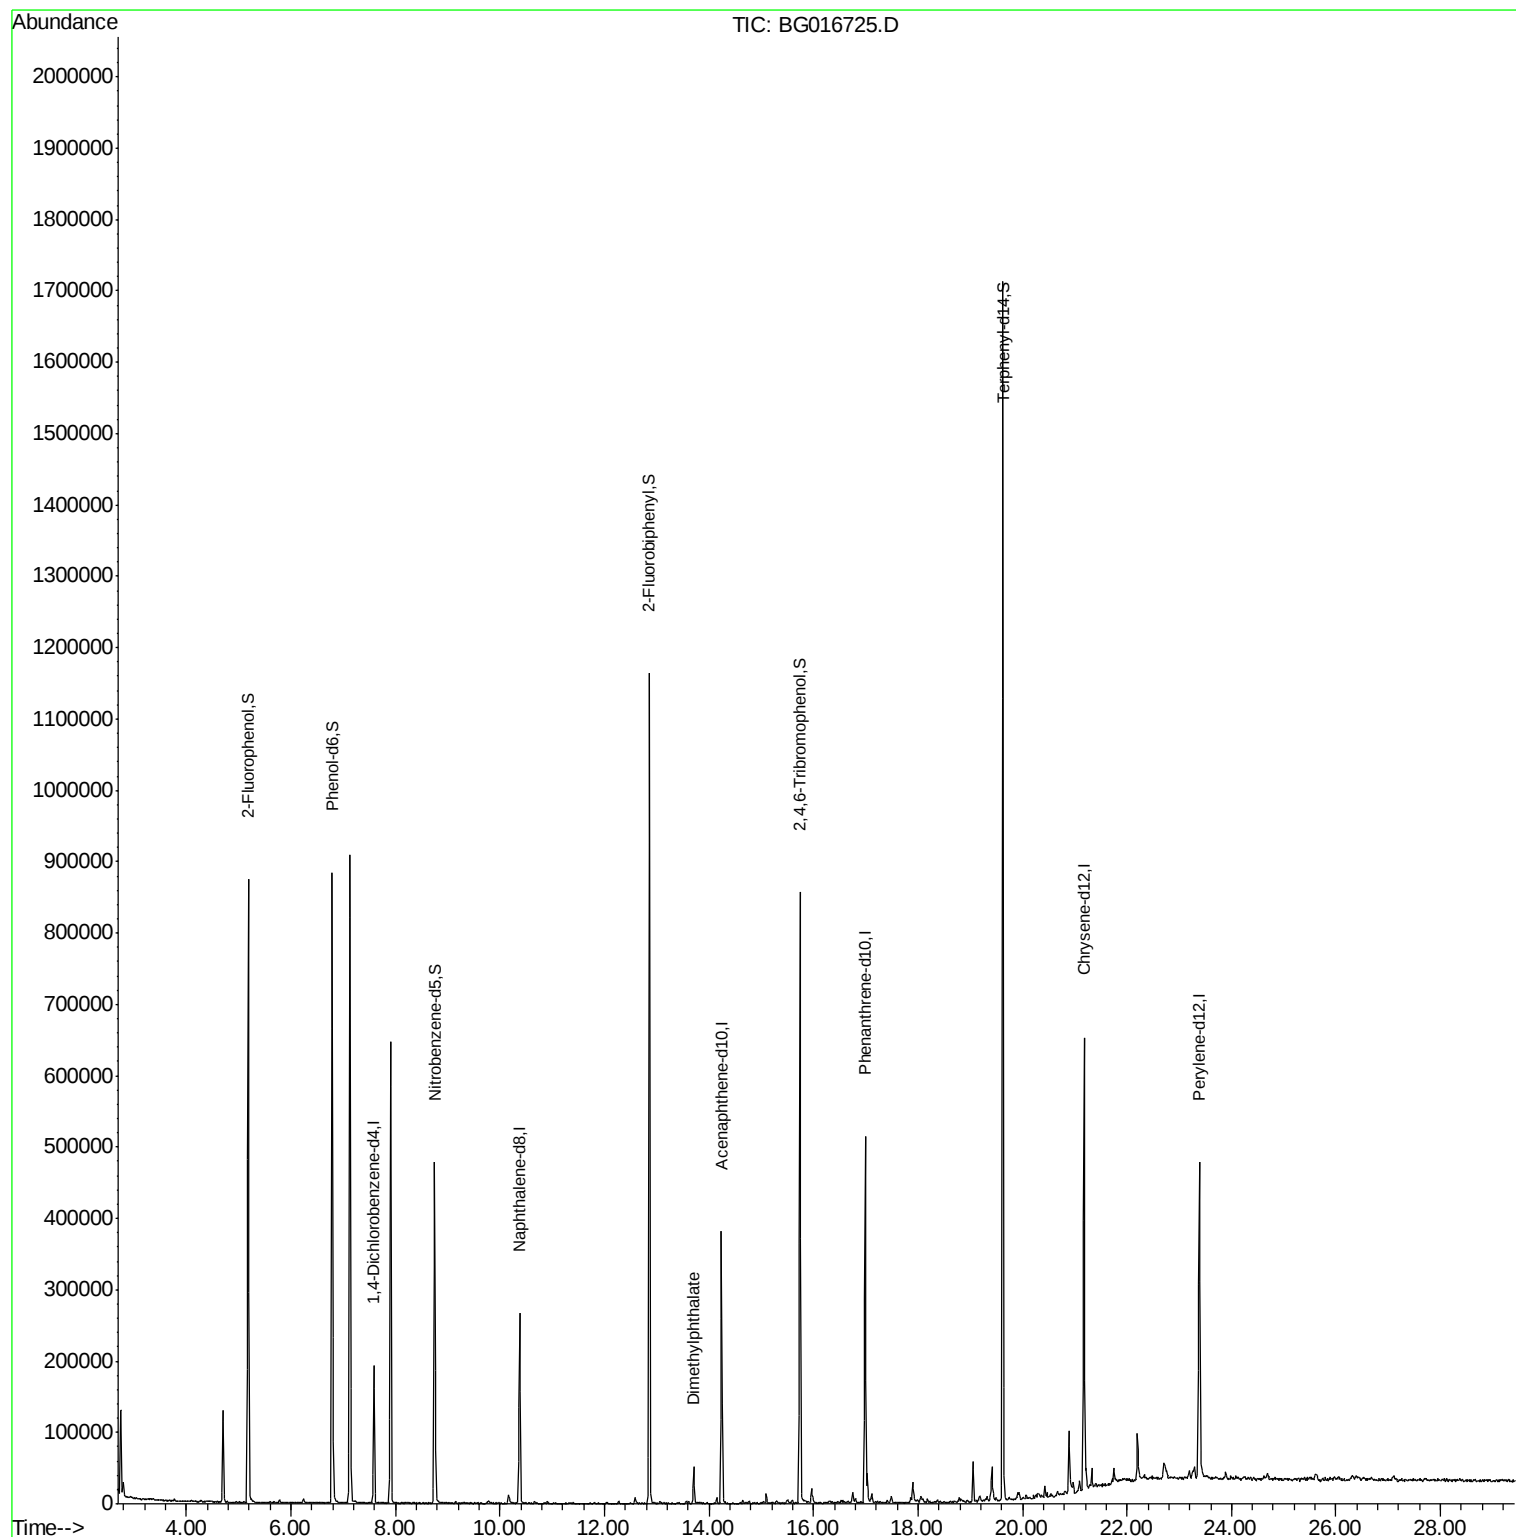



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.59 min Scan# 834

Delta R.T. -0.00 min

Lab File: BG016725.D

Acq: 25 Apr 2015 22:03

Instrument :

BNA_G

ClientSampleId :

SB-75D


Tot Ion:152 Resp: 53560

Ion Ratio Lower Upper

152 100

150 159.8 129.6 194.4



115 57.1 43.0 64.6

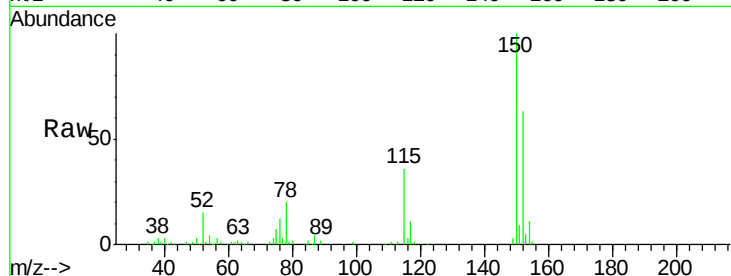

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

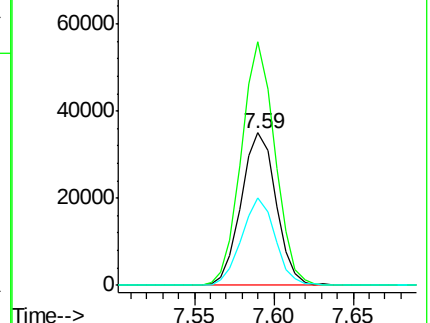

#5

2-Fluorophenol

Concen: 128.54 ng

RT: 5.19 min Scan# 425

Delta R.T. 0.00 min

Lab File: BG016725.D

Acq: 25 Apr 2015 22:03


Tgt Ion:112 Resp: 424254

Ion Ratio Lower Upper

112 100

64 45.6 38.3 57.5



63 22.6 18.9 28.3



Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BGC

Ion 63.00 (62.70 to 63.70): BGC

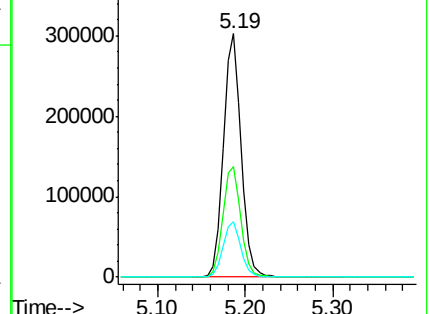



#7

Phenol-d6

Concen: 125.10 ng

RT: 6.79 min Scan# 698

Delta R.T. -0.00 min

Lab File: BG016725.D

Acq: 25 Apr 2015 22:03

Instrument :

BNA_G

ClientSampled :

SB-75D


Tot Ion: 99 Resp: 579277

Ion Ratio Lower Upper




99 100

42 11.8 8.8 13.2

71 25.9 19.9 29.9



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

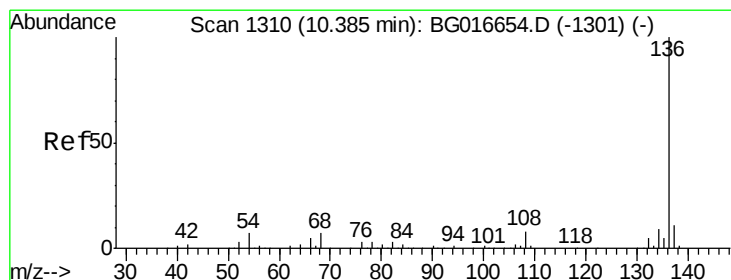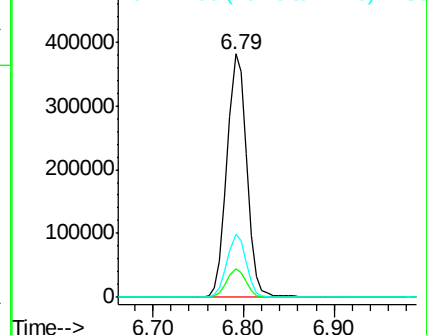

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.38 min Scan# 1308

Delta R.T. -0.00 min

Lab File: BG016725.D

Acq: 25 Apr 2015 22:03

Tgt Ion: 136 Resp: 227682


Ion Ratio Lower Upper

136 100



137 10.8 8.5 12.7

54 6.2 5.4 8.2

68 6.3 5.2 7.8



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



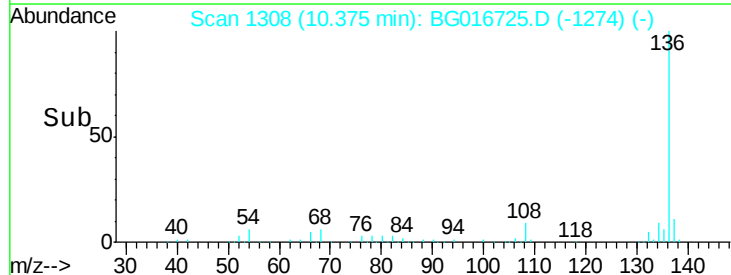
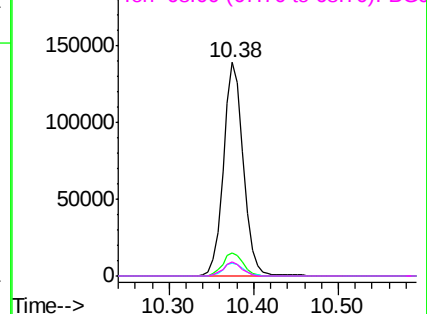




#23
 Nitrobenzene-d5
 Concen: 78.39 ng
 RT: 8.75 min Scan# 1032
 Delta R.T. 0.00 min
 Lab File: BG016725.D
 Acq: 25 Apr 2015 22:03




Instrument :
 BNA_G
 ClientSampled :
 SB-75D

Tot Ion	82	Resp	282446
Ion Ratio	100	Lower	Upper
128	54.9	44.7	67.1
54	38.4	30.9	46.3

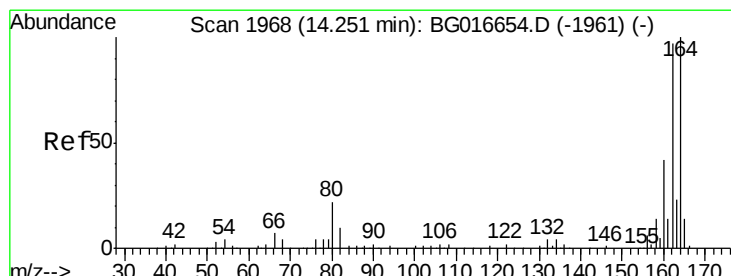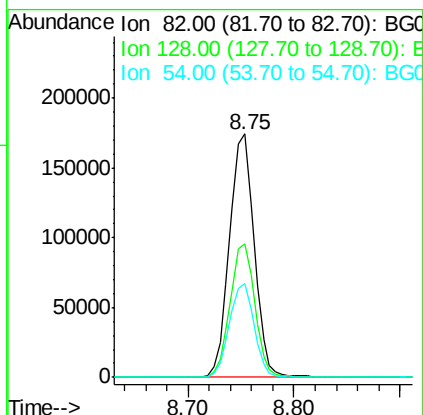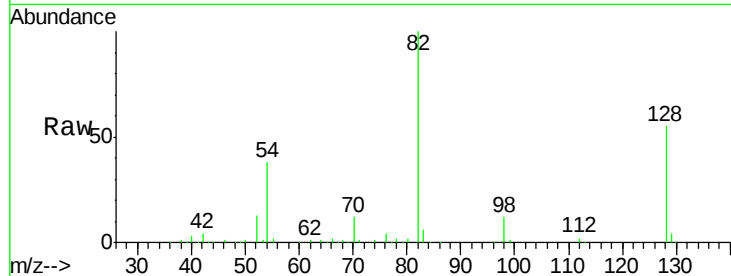

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.24 min Scan# 1966
 Delta R.T. -0.00 min
 Lab File: BG016725.D
 Acq: 25 Apr 2015 22:03

Tgt Ion	164	Resp	130627
Ion Ratio	100	Lower	Upper
162	96.8	77.3	115.9
160	42.9	33.7	50.5

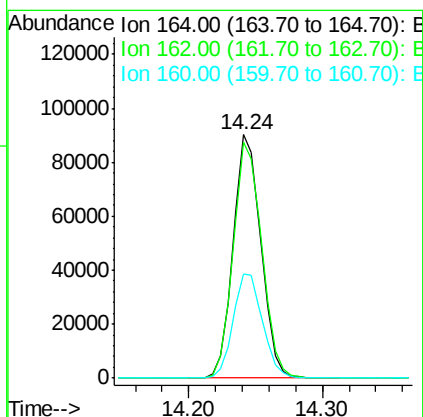







#41
 2,4,6-Tribromophenol
 Concen: 123.36 ng
 RT: 15.74 min Scan# 2221
 Delta R.T. -0.00 min
 Lab File: BG016725.D
 Acq: 25 Apr 2015 22:03

Instrument :
 BNA_G
 ClientSampled :
 SB-75D

Tot Ion:330 Resp: 119548
 Ion Ratio Lower Upper
 330 100
 332 95.5 76.2 114.4
 141 54.3 43.0 64.6




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


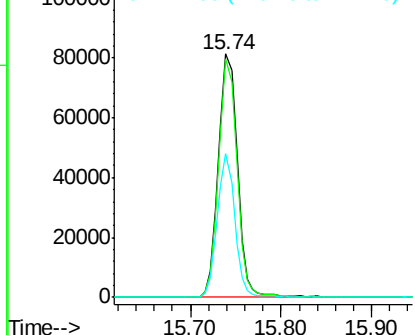



#44
 2-Fluorobiphenyl
 Concen: 68.46 ng
 RT: 12.86 min Scan# 1731
 Delta R.T. -0.00 min
 Lab File: BG016725.D
 Acq: 25 Apr 2015 22:03

Tgt Ion:172 Resp: 556624
 Ion Ratio Lower Upper
 172 100
 171 37.0 29.9 44.9
 170 24.5 19.8 29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

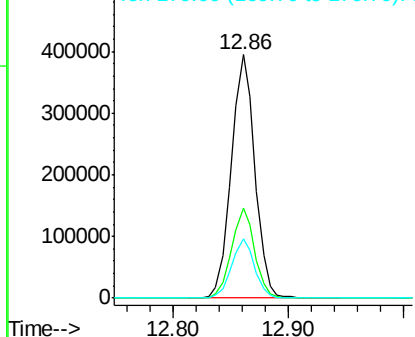

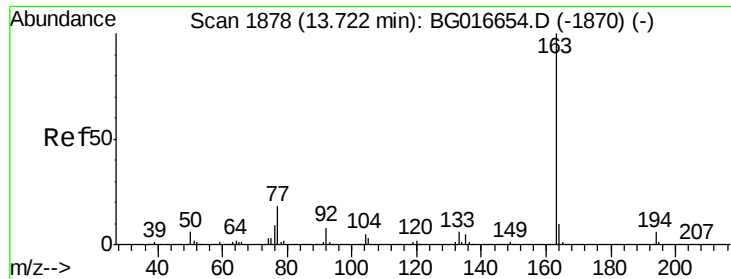

#49

Dimethylphthalate

Concen: 3.63 ng

RT: 13.71 min Scan# 1875

Delta R.T. -0.01 min

Lab File: BG016725.D

Acq: 25 Apr 2015 22:03

Instrument :

BNA_G

ClientSampleId :

SB-75D


Tot Ion:163 Resp: 35449

Ion Ratio Lower Upper

163 100

194 5.8 5.0 7.4




164 11.2 7.8 11.8



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

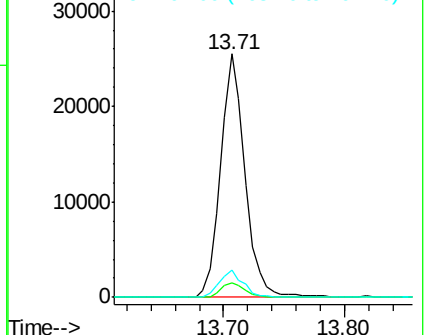

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 16.99 min Scan# 2434

Delta R.T. -0.00 min

Lab File: BG016725.D

Acq: 25 Apr 2015 22:03


Tgt Ion:188 Resp: 280072

Ion Ratio Lower Upper

188 100

94 12.1 10.7 16.1



80 11.8 9.9 14.9




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

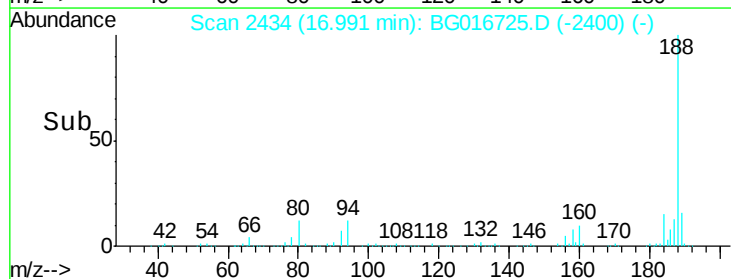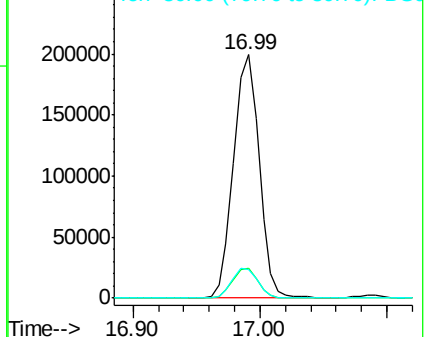



#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.18 min Scan# 3147

Delta R.T. -0.00 min

Lab File: BG016725.D

Acq: 25 Apr 2015 22:03

Instrument :

BNA_G

ClientSampleId :

SB-75D


Tot Ion:240 Resp: 269869

Ion Ratio Lower Upper

240 100

120 19.2 16.3 24.5




236 26.0 21.1 31.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

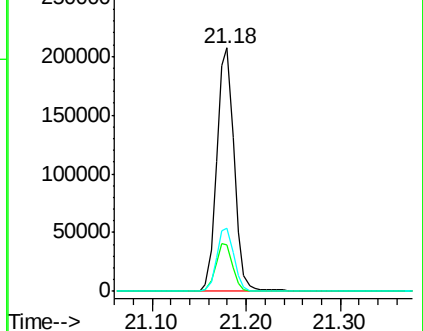

#78

Terphenyl-d14

Concen: 52.65 ng

RT: 19.62 min Scan# 2882

Delta R.T. -0.00 min

Lab File: BG016725.D

Acq: 25 Apr 2015 22:03


Tgt Ion:244 Resp: 616856

Ion Ratio Lower Upper

244 100

212 7.9 6.4 9.6



122 20.3 15.9 23.9




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

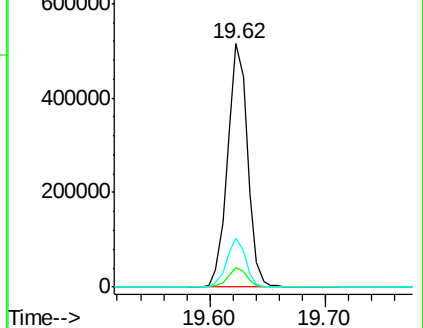


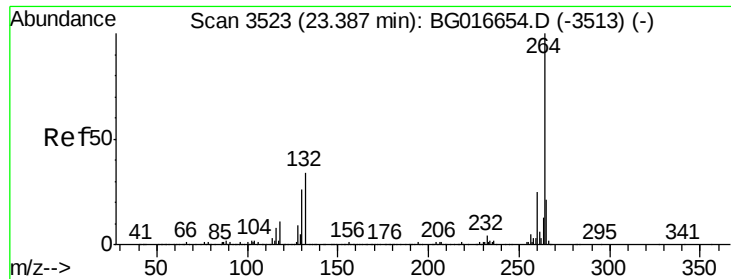

#86
Pervlene-d12
Concen: 20.00 ng
RT: 23.38 min Scan# 3522
Delta R.T. -0.00 min
Lab File: BG016725.D
Acq: 25 Apr 2015 22:03

Instrument :
BNA_G
ClientSampleId :
SB-75D

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.1	20.0	30.0
265	21.6	16.8	25.2



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

