


Data Path : Z:\HPCHEM1\BNA G\Data\BG042415\  
 Data File : BG016703.D  
 Acq On : 25 Apr 2015 6:07  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG042315.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Apr 23 19:19:11 2015

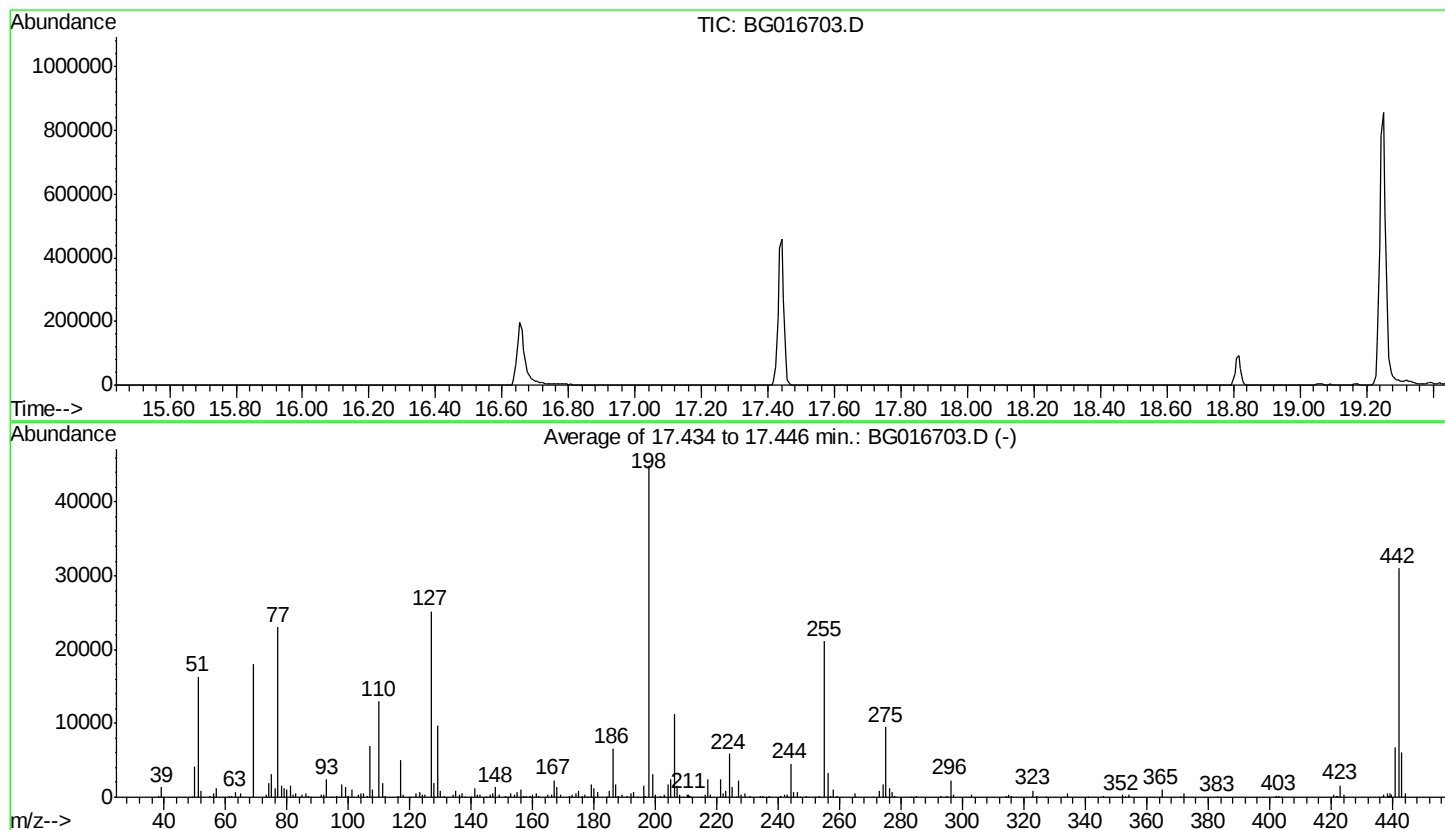

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 36.4      | 16346   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 40.0      | 17969   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 56.1      | 25213   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 135     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 44925   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 3049    | PASS             |
| 275         | 198          | 10           | 60           | 21.2      | 9525    | PASS             |
| 365         | 198          | 1            | 100          | 2.2       | 978     | PASS             |
| 441         | 442          | 0.01         | 24           | 21.9      | 6790    | PASS             |
| 442         | 198          | 50           | 100          | 69.1      | 31034   | PASS             |
| 443         | 442          | 15           | 24           | 19.8      | 6159    | PASS             |