
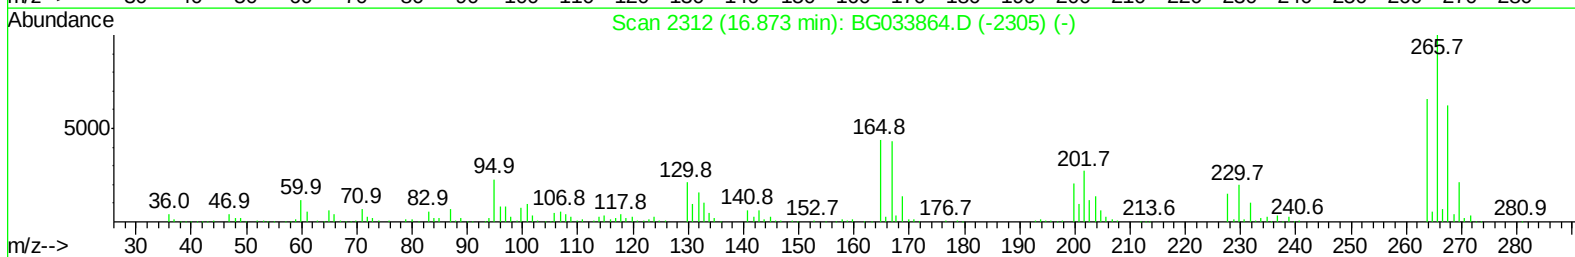
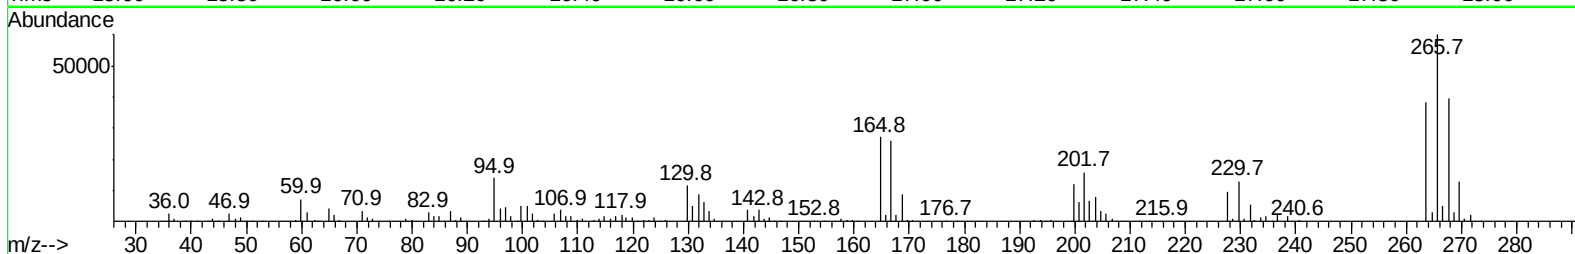


Data Path : Z:\HPCHEM1\BNA G\DATA\BG042418\
Data File : BG033968.D
Acq On : 25 Apr 2018 1:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 03:50:30 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

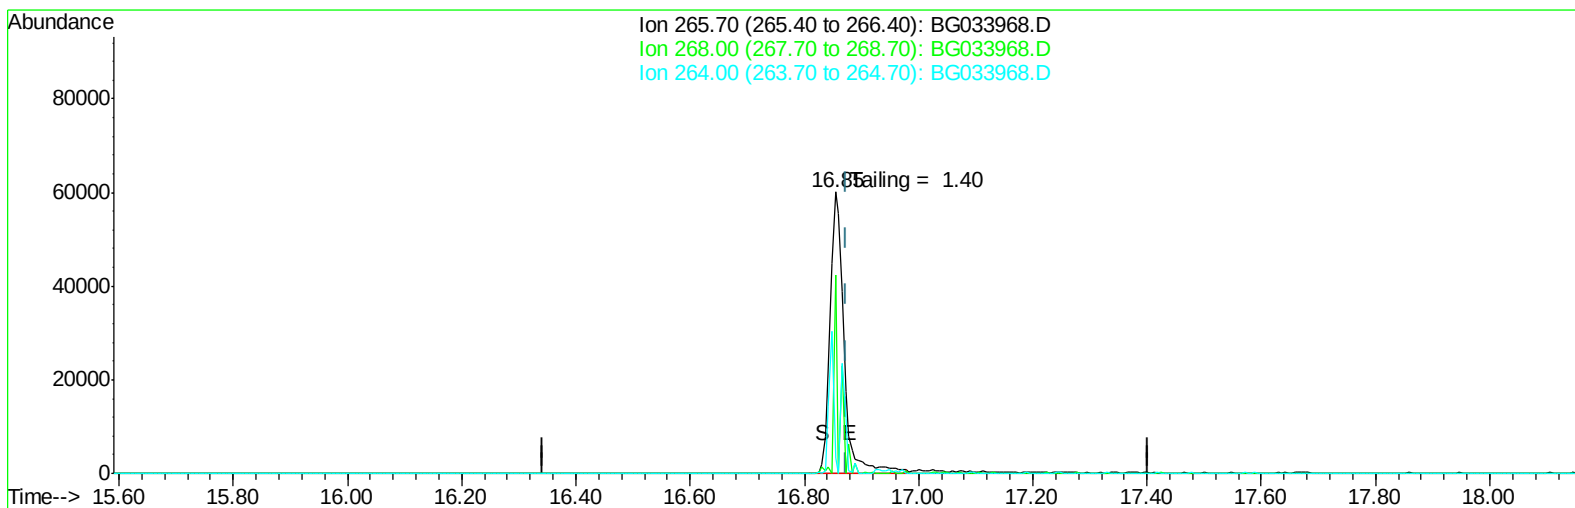

TIC: BG033968.D

(69) Pentachlorophenol (C)




16.854min (-0.019) 23388.47ng

response 101228

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	70.45
264.00	62.00	5.26#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042418\
Data File : BG033968.D
Acq On : 25 Apr 2018 1:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 03:50:30 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

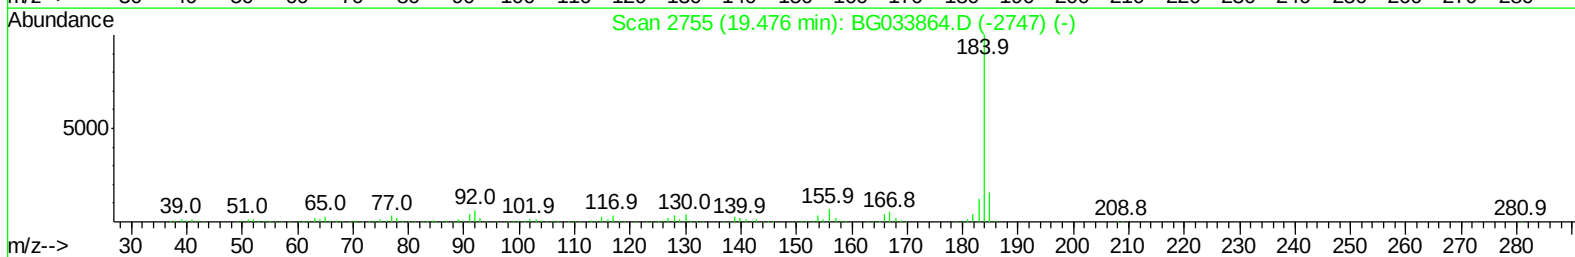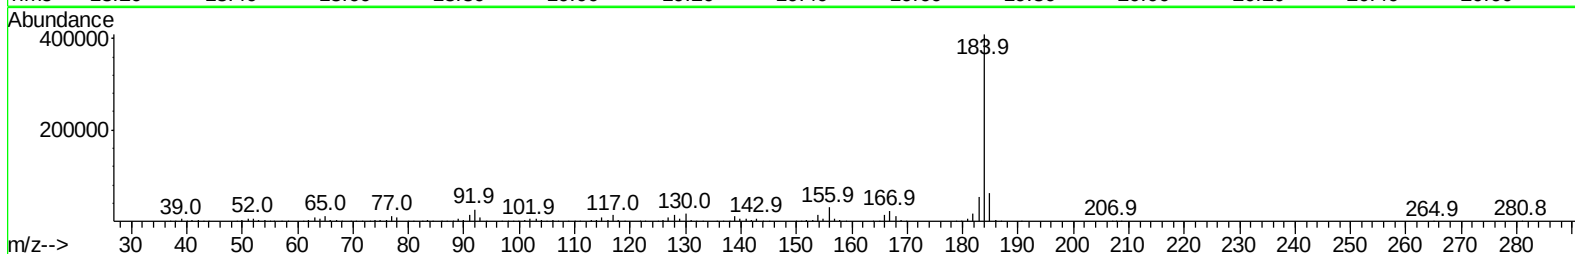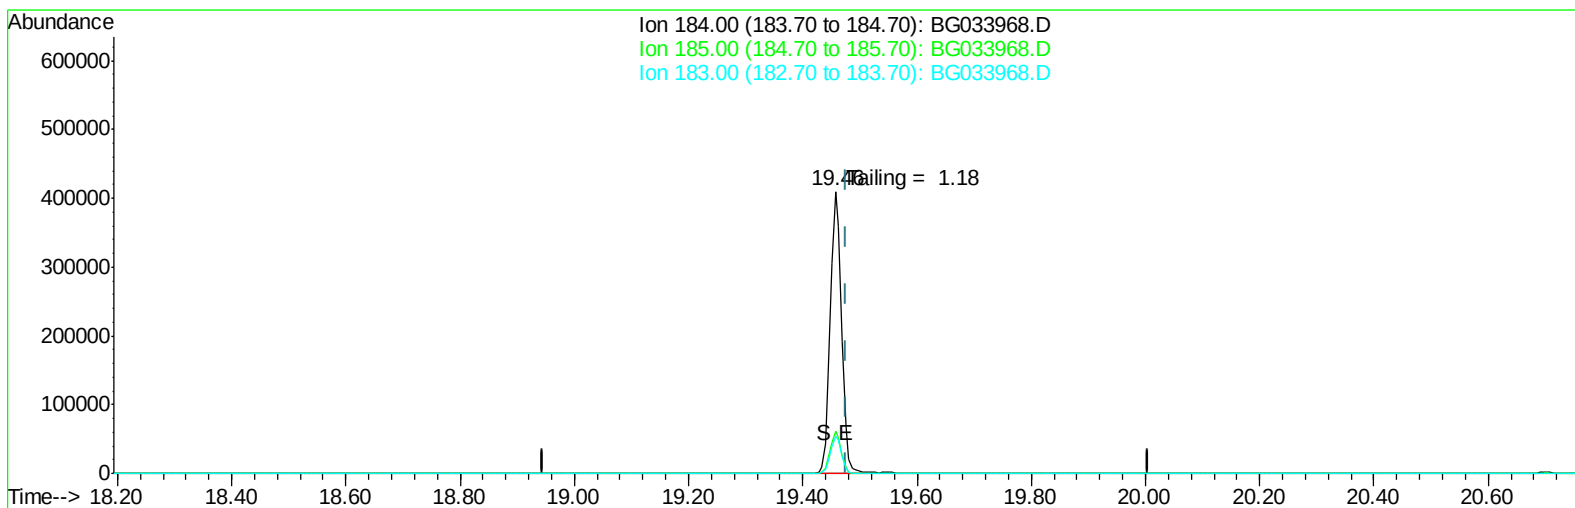

TIC: BG033968.D

(76) Benzidine

19.457min (-0.019) 0.00ng

response 557375

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.08
183.00	13.30	13.08
0.00	0.00	0.00