


Data Path : Z:\HPCHEM1\BNA G\Data\BG042418\
 Data File : BG033950.D
 Acq On : 24 Apr 2018 12:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

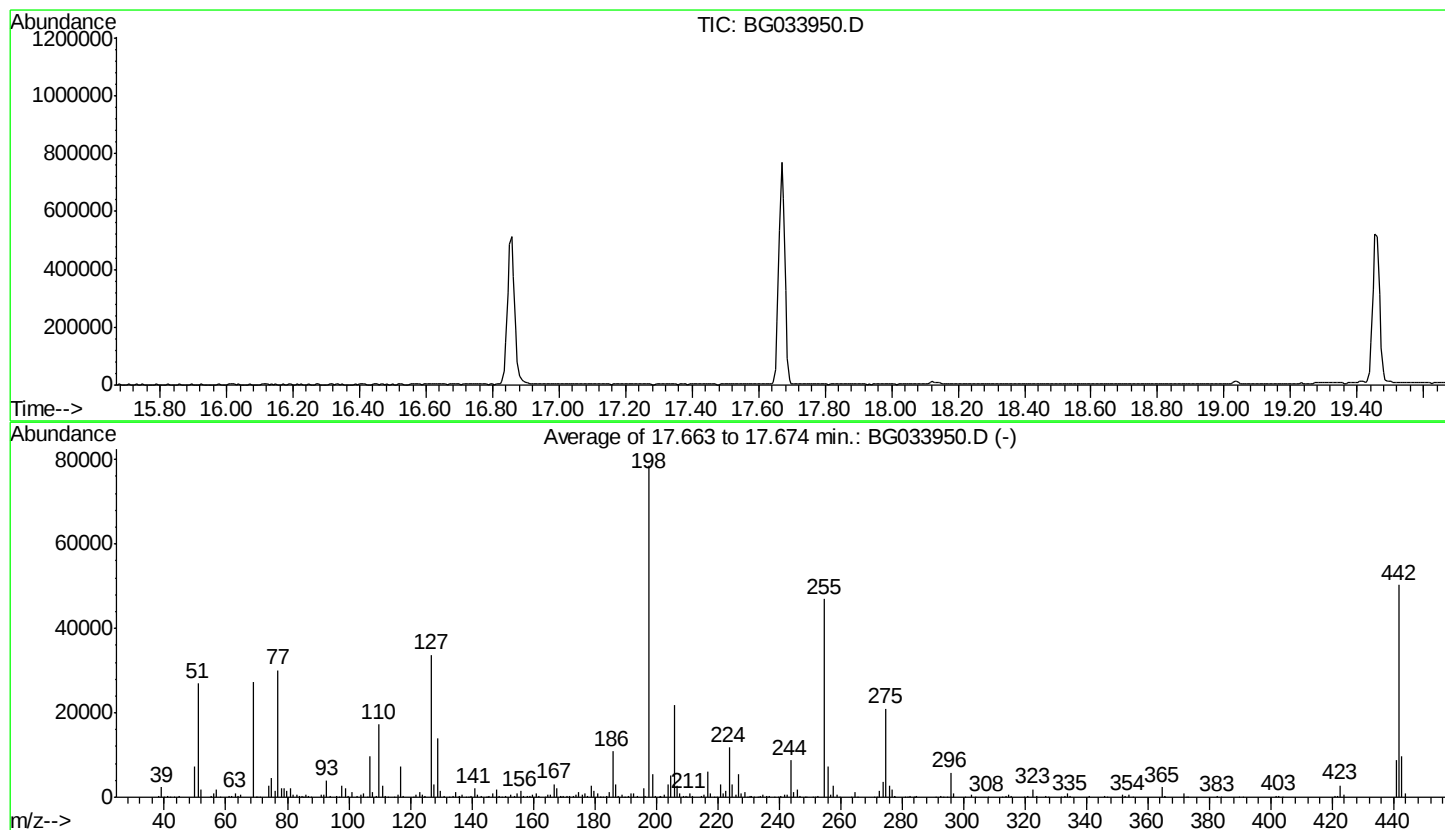

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2439

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	26906	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.7	27293	PASS
70	69	0.00	2	0.3	82	PASS
127	198	10	80	43.0	33778	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	78570	PASS
199	198	5	9	7.1	5548	PASS
275	198	10	60	26.7	20984	PASS
365	198	1	100	3.0	2386	PASS
441	443	0.01	100	89.8	8796	PASS
442	198	50	100	64.0	50296	PASS
443	442	15	24	19.5	9794	PASS