


Data Path : Z:\HPCHEM1\BNA G\Data\BG042418\
Data File : BG033968.D
Acq On : 25 Apr 2018 1:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Apr 19 13:56:22 2018

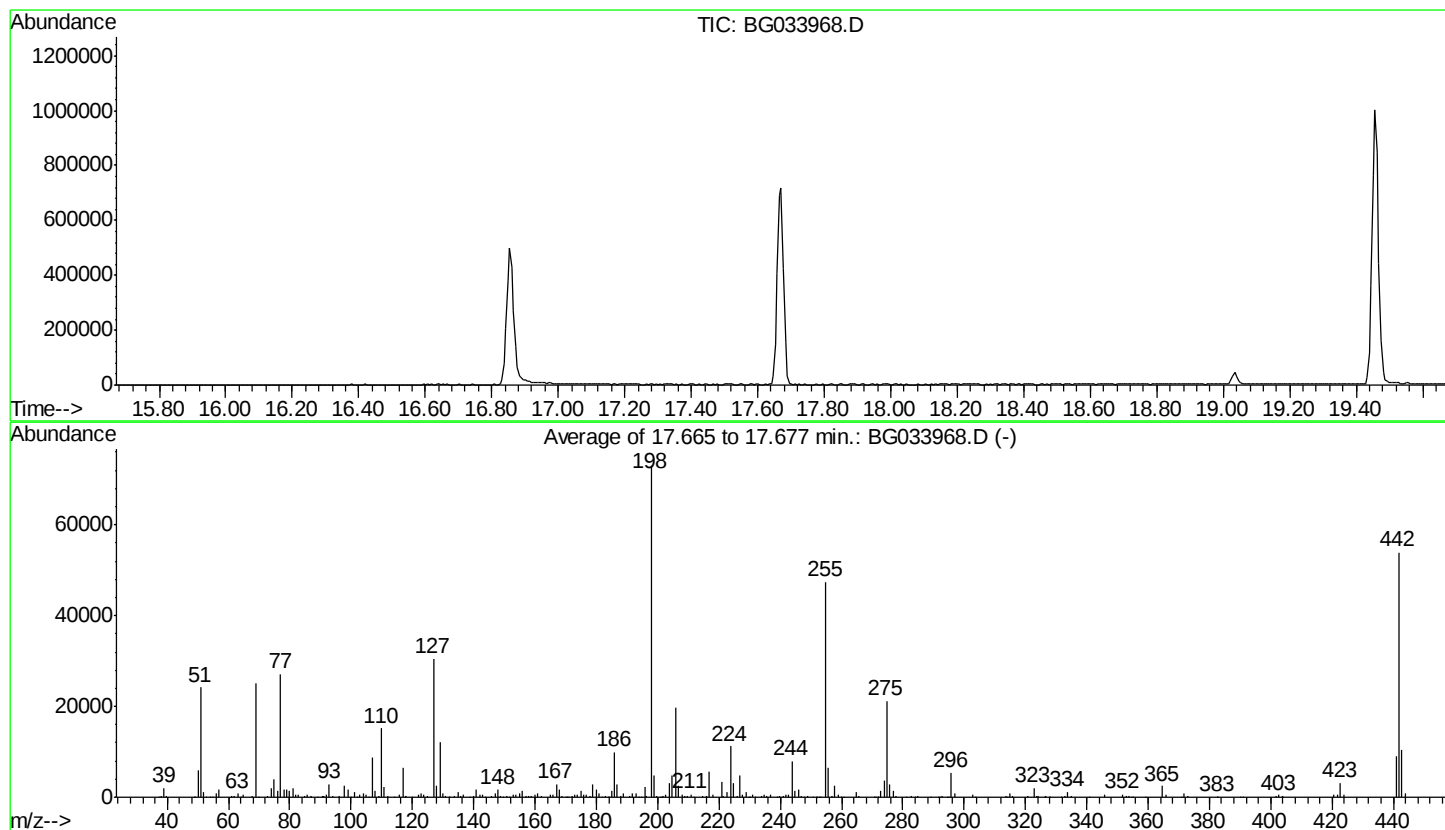

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	24172	PASS
68	69	0.00	2	0.6	156	PASS
69	198	0.00	100	34.2	25012	PASS
70	69	0.00	2	0.6	147	PASS
127	198	10	80	41.8	30493	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73032	PASS
199	198	5	9	6.5	4780	PASS
275	198	10	60	29.2	21290	PASS
365	198	1	100	3.3	2426	PASS
441	443	0.01	100	85.3	8932	PASS
442	198	50	100	73.9	53949	PASS
443	442	15	24	19.4	10476	PASS