
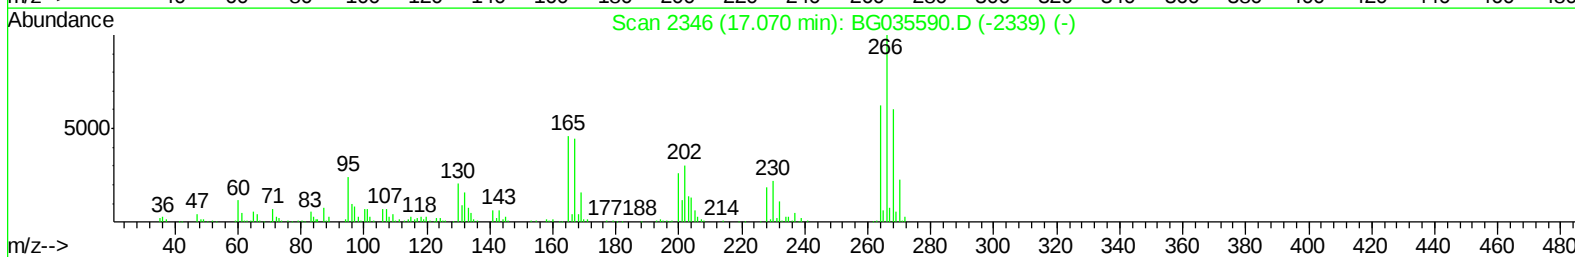
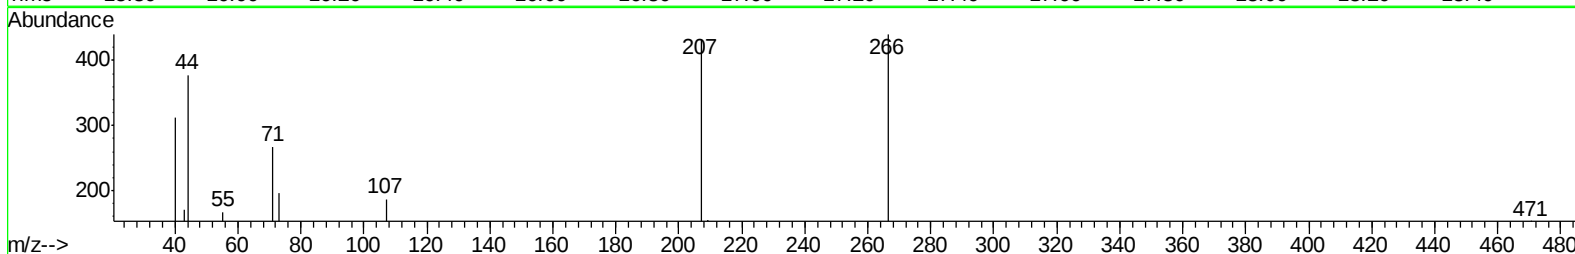


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072418\  
 Data File : BG035839.D  
 Acq On : 24 Jul 2018 9:16  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 08:23:24 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jul 31 12:30:06 2018  
 Response via : Initial Calibration

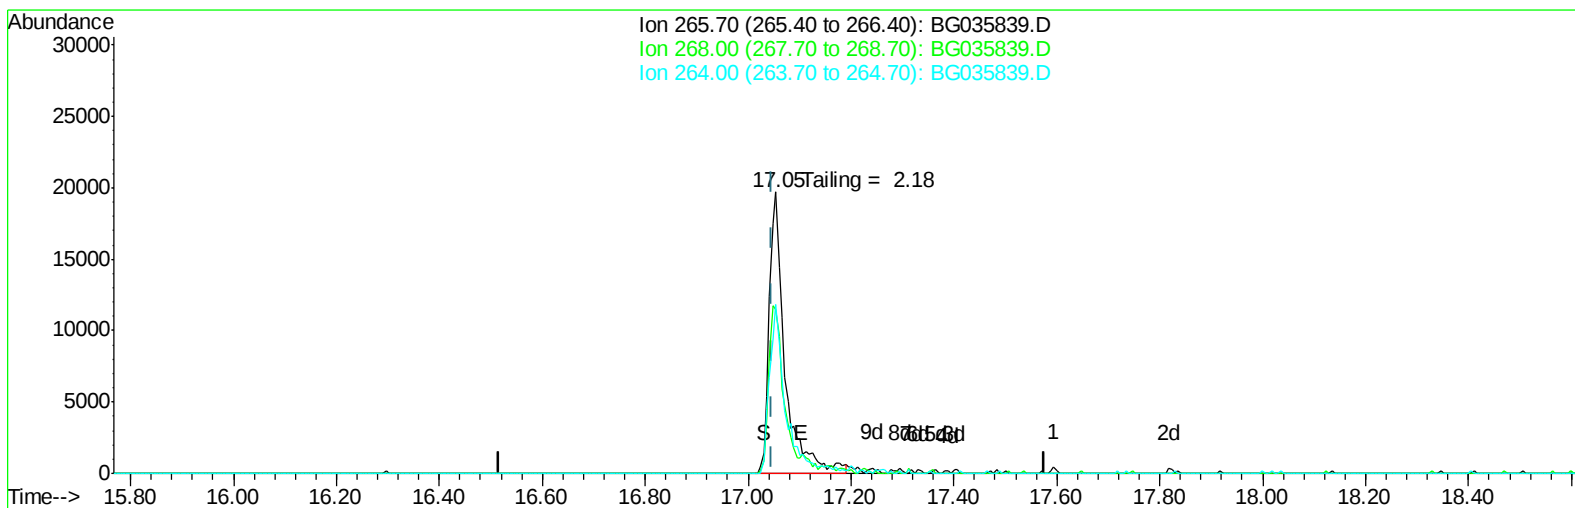

TIC: BG035839.D

(69) Pentachlorophenol (C)




17.594min (+0.547) 722.06ng

response 289

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 0.00# |
| 264.00 | 62.00 | 0.00# |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG072418\  
Data File : BG035839.D  
Acq On : 24 Jul 2018 9:16  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 25 08:23:24 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG071218.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 31 12:30:06 2018  
Response via : Initial Calibration

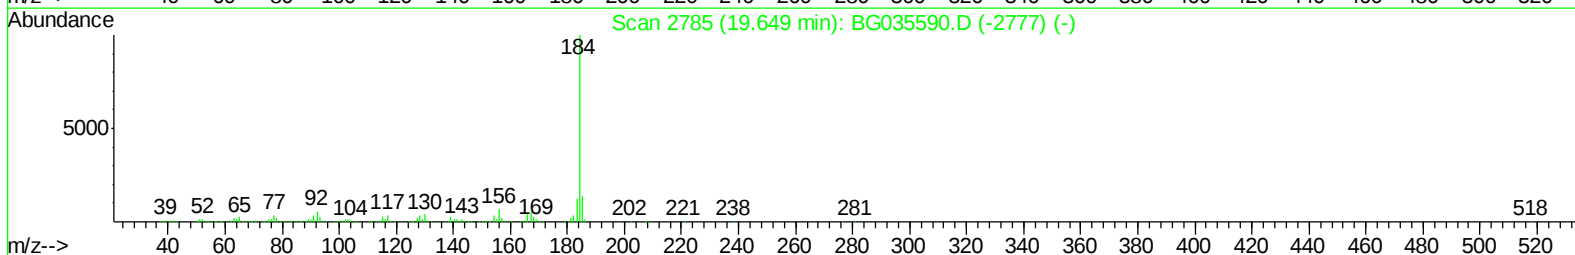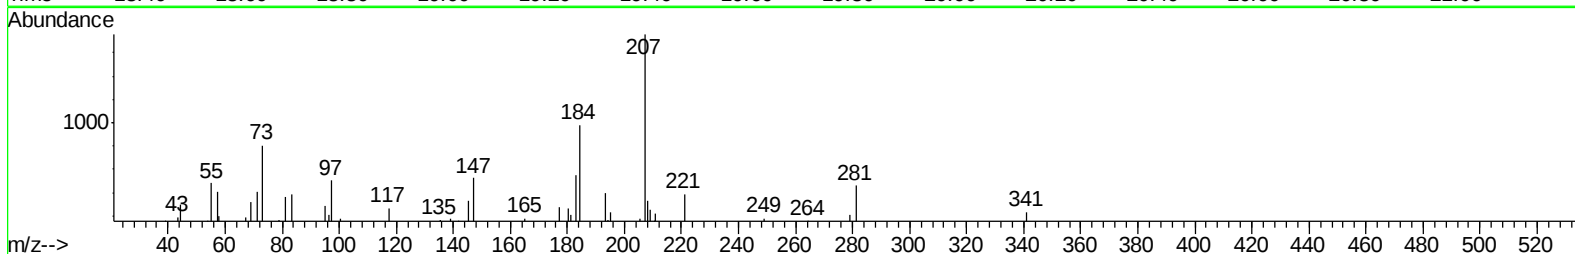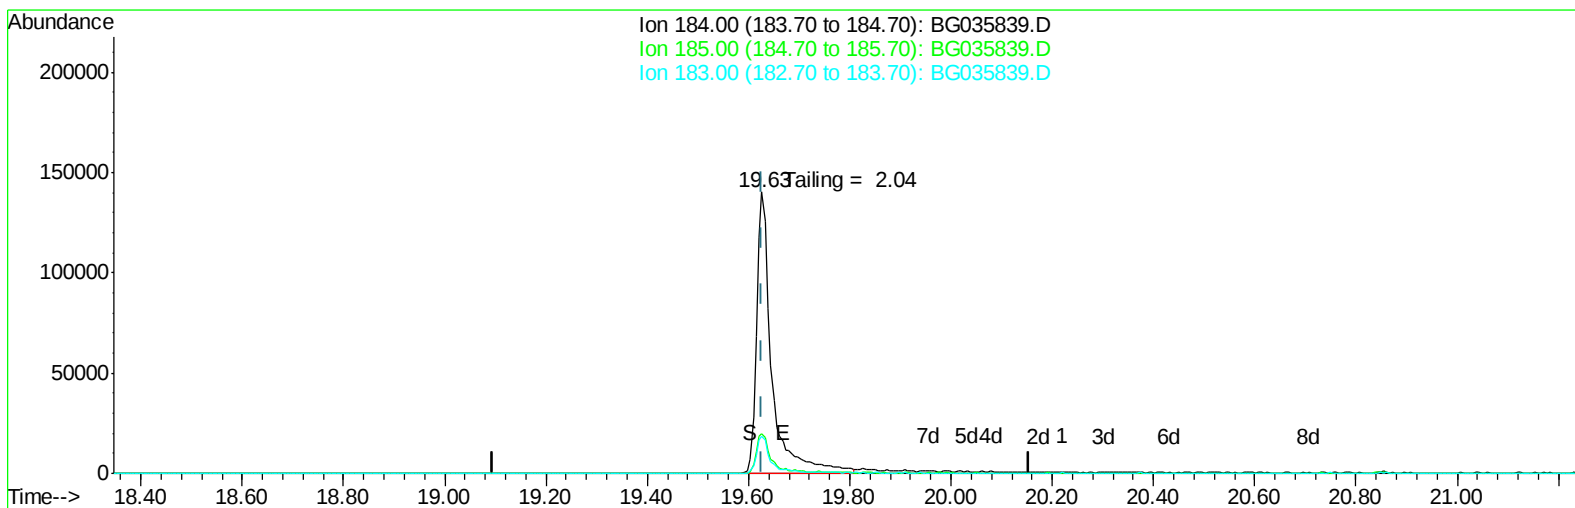

TIC: BG035839.D

(76) Benzidine

20.220min (+0.594) 388.24ng

response 592

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 13.90 | 0.00#  |
| 183.00 | 13.30 | 55.92# |
| 0.00   | 0.00  | 0.00   |