


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042419\
 Data File : BG040584.D
 Acq On : 24 Apr 2019 9:03
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

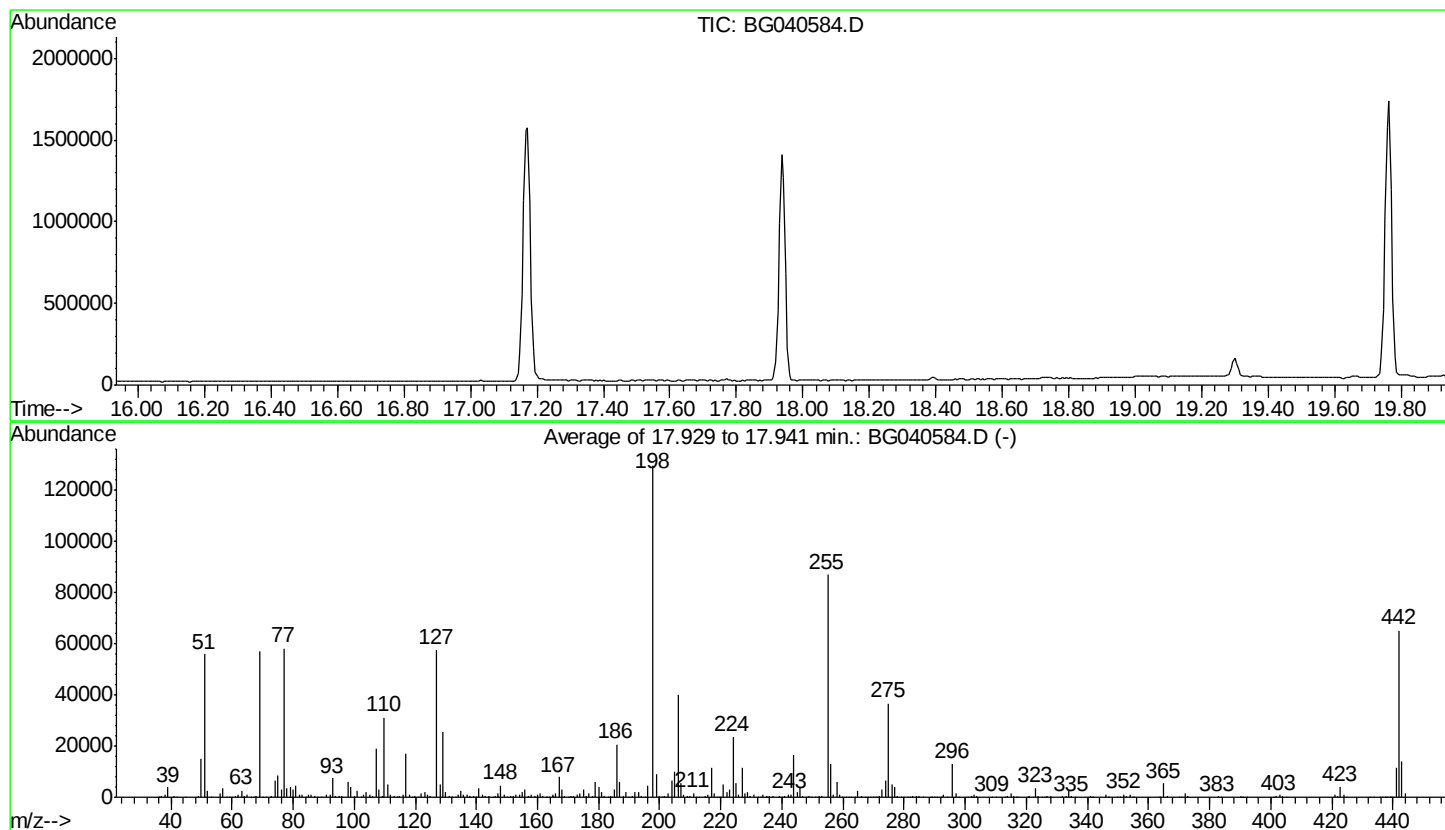

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	56077	PASS
68	69	0.00	2	0.8	469	PASS
69	198	0.00	100	43.8	56868	PASS
70	69	0.00	2	0.5	268	PASS
127	198	10	80	44.6	57824	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	129720	PASS
199	198	5	9	7.0	9143	PASS
275	198	10	60	28.4	36794	PASS
365	198	1	100	4.1	5310	PASS
441	198	0.01	100	8.8	11435	PASS
442	198	50	100	50.3	65266	PASS
443	442	15	24	21.3	13927	PASS