

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042518\
 Data File : BG034013.D
 Acq On : 26 Apr 2018 8:32
 Operator : SJ/JU
 Sample : J2541-02
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-3-4-5-WC-1

Quant Time: Apr 26 15:13:54 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 19 13:56:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	57304	20.00	ng	-0.01
21) Naphthalene-d8	10.61	136	258995	20.00	ng	-0.02
38) Acenaphthene-d10	14.46	164	177145	20.00	ng	-0.02
63) Phenanthrene-d10	17.21	188	496960	20.00	ng	-0.02
75) Chrysene-d12	21.46	240	560743	20.00	ng	-0.03
86) Perylene-d12	24.52	264	551997	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	520327	144.97	ng	0.00
7) Phenol-d6	7.00	99	646199	123.43	ng	0.00
23) Nitrobenzene-d5	8.98	82	479054	105.26	ng	-0.01
41) 2,4,6-Tribromophenol	15.95	330	397515	192.34	ng	-0.02
44) 2-Fluorobiphenyl	13.08	172	1228192	101.85	ng	-0.02
78) Terphenyl-d14	19.85	244	2439085	97.72	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG042518\
Data File : BG034013.D
Acq On : 26 Apr 2018 8:32
Operator : SJ/JU
Sample : J2541-02
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-3-4-5-WC-1

Quant Time: Apr 26 15:13:54 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG041918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 19 13:56:22 2018
Response via : Initial Calibration

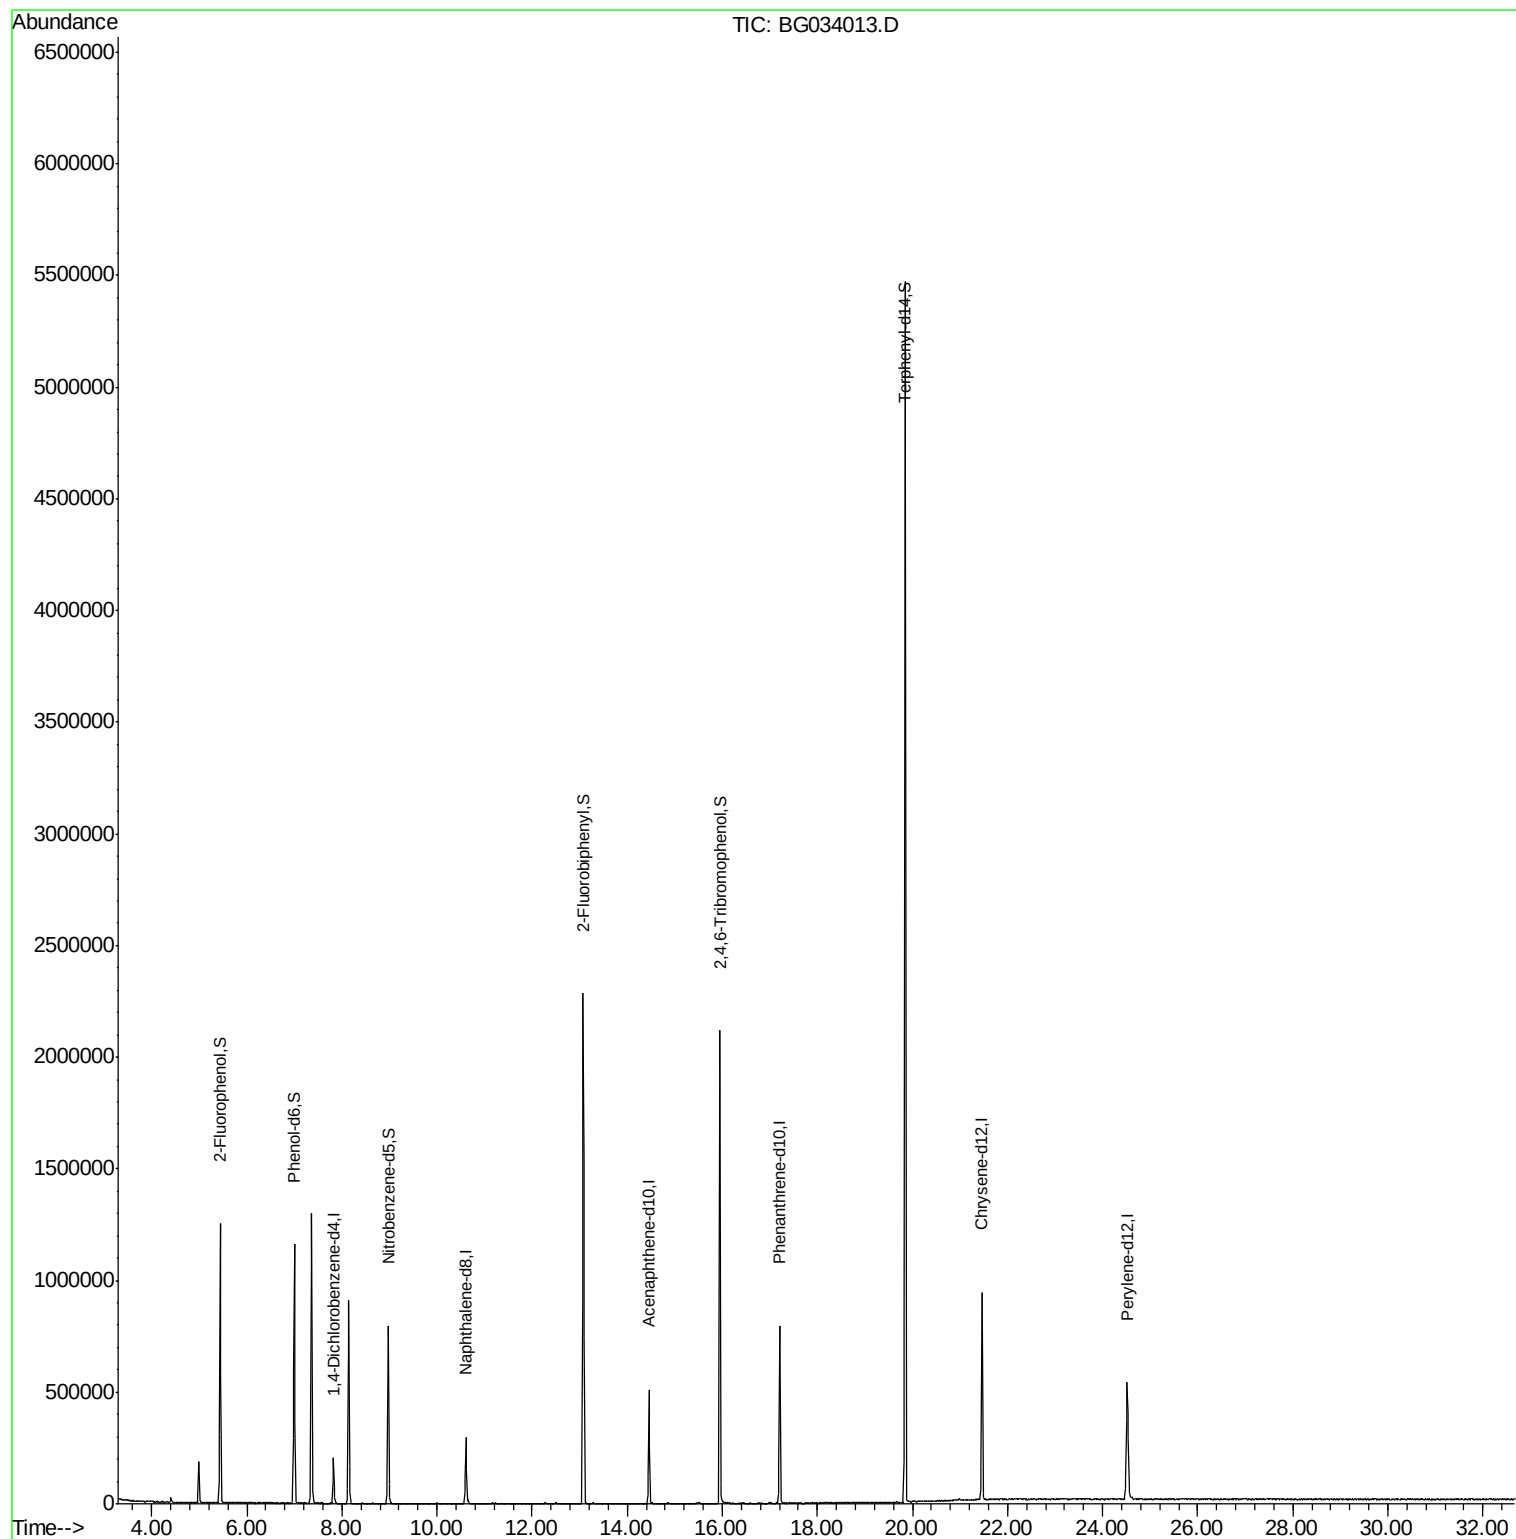

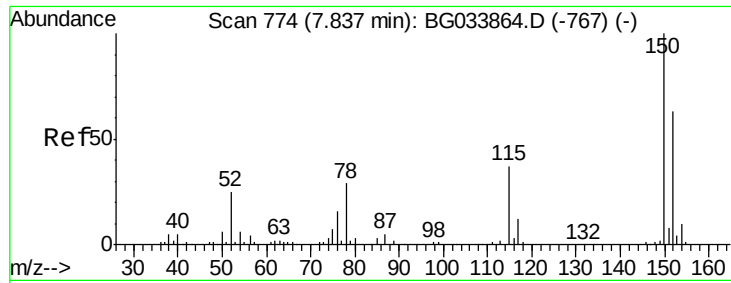


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.82 min Scan# 772
Delta R.T. -0.01 min
Lab File: BG034013.D
Acq: 26 Apr 2018 8:32

Instrument :
BNA_G
ClientSampleId :
TP-3-4-5-WC-1

Tot Ion	Ratio	Lower	Upper
152	100		
150	161.4	126.6	189.8
115	62.8	53.0	79.4

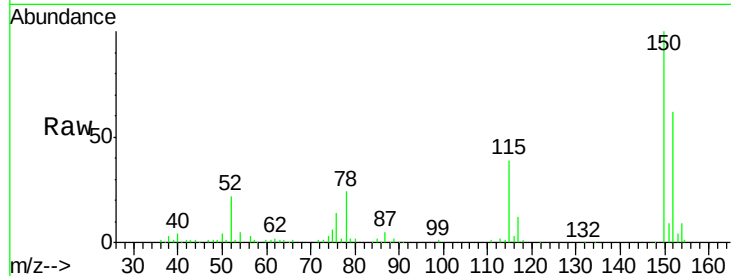


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

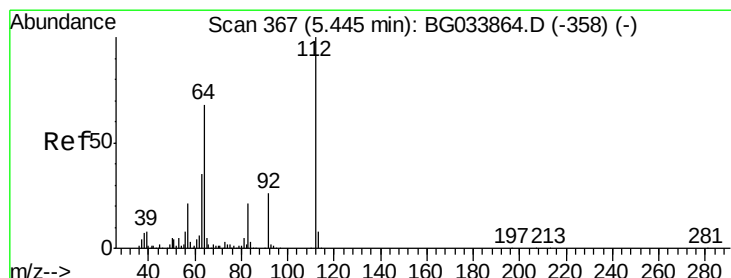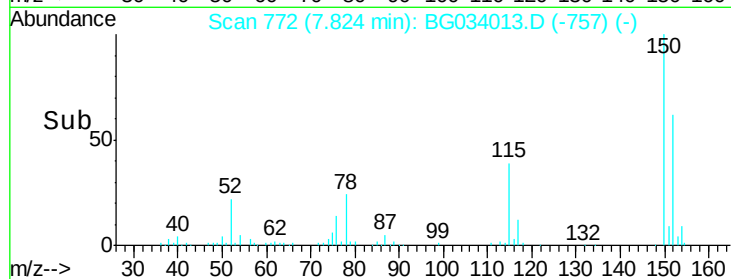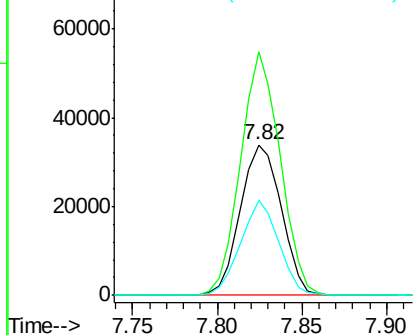



#5


2-Fluorophenol
Concen: 144.967 ng
RT: 5.44 min Scan# 366
Delta R.T. -0.01 min
Lab File: BG034013.D
Acq: 26 Apr 2018 8:32

Tgt Ion	Ratio	Lower	Upper
112	100		
64	64.6	56.3	84.5
63	33.5	30.1	45.1

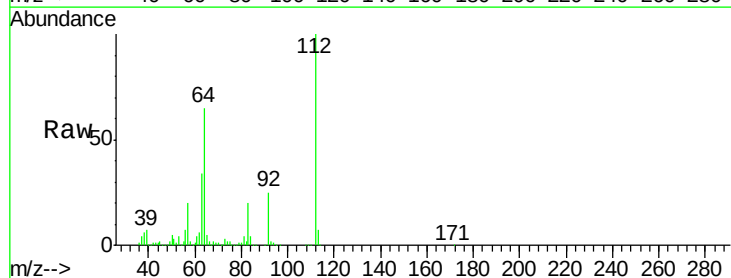

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

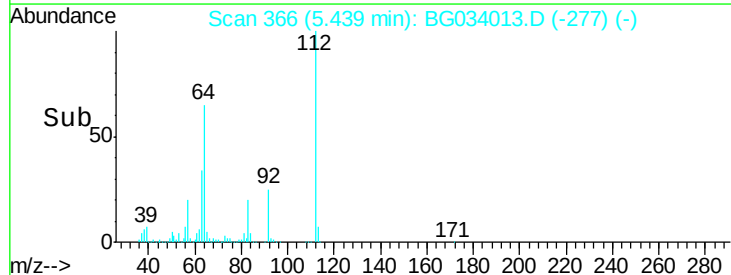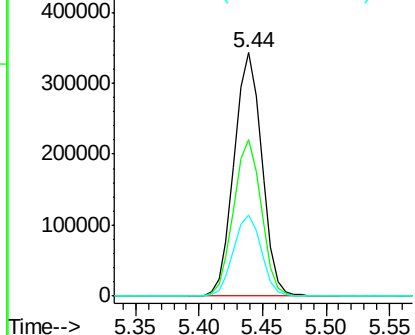

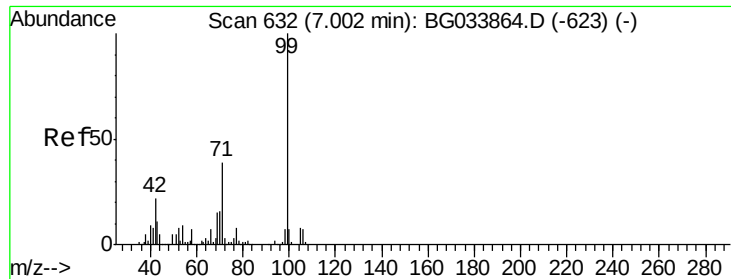

#7

Phenol-d6

Concen: 123.434 ng

RT: 7.00 min Scan# 631

Delta R.T. -0.01 min

Lab File: BG034013.D

Acq: 26 Apr 2018 8:32

Instrument :

BNA_G

ClientSampleId :

TP-3-4-5-WC-1





Tot Ion: 99 Resp: 646199

Ion Ratio Lower Upper

99 100

42 19.6 14.1 21.1

71 36.3 26.1 39.1

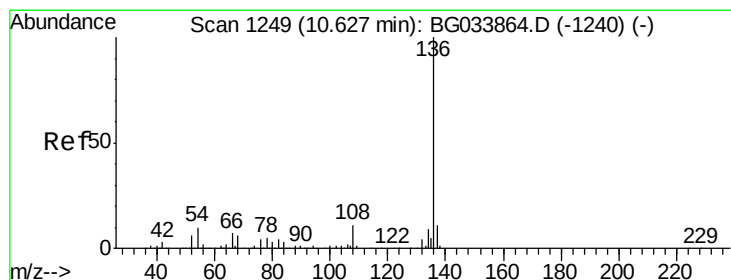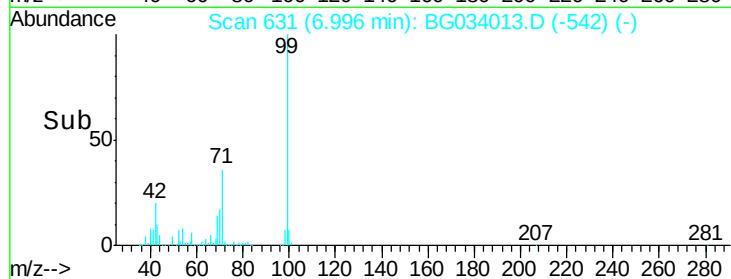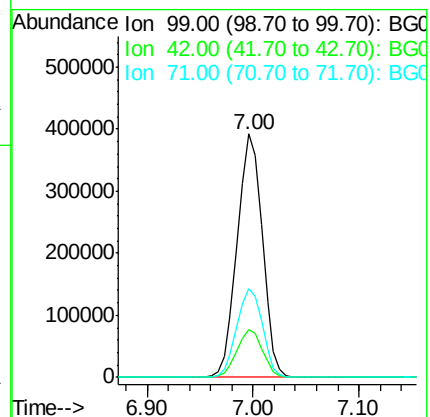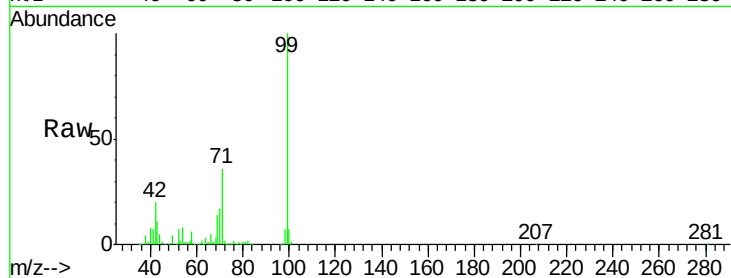

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.61 min Scan# 1246

Delta R.T. -0.02 min

Lab File: BG034013.D

Acq: 26 Apr 2018 8:32

Tgt Ion: 136 Resp: 258995




Ion Ratio Lower Upper


136 100

137 12.0 9.2 13.8

54 8.1 10.3 15.5#

68 5.9 4.5 6.7


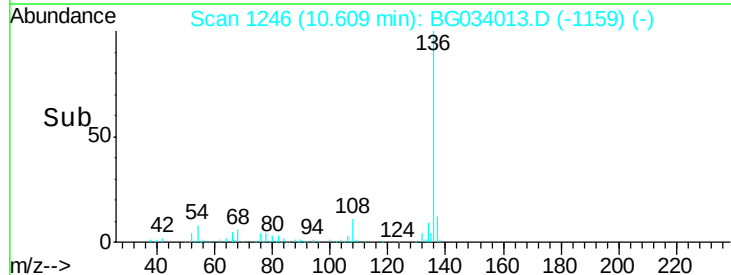
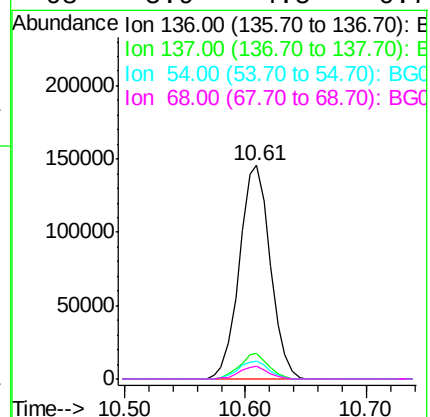
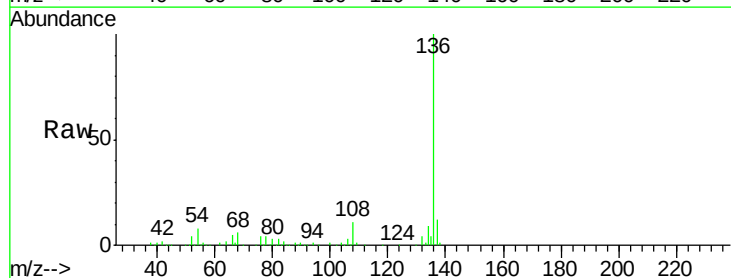


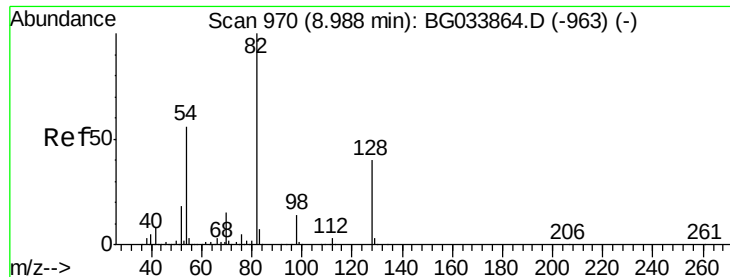

#23
 Nitrobenzene-d5
 Concen: 105.264 ng
 RT: 8.98 min Scan# 968
 Delta R.T. -0.01 min
 Lab File: BG034013.D
 Acq: 26 Apr 2018 8:32




Instrument :
 BNA_G
 ClientSampleId :
 TP-3-4-5-WC-1


Tot Ion	82	Resp	479054
Ion Ratio	Lower	Upper	
82	100		
128	41.3	29.7	44.5
54	53.2	43.1	64.7

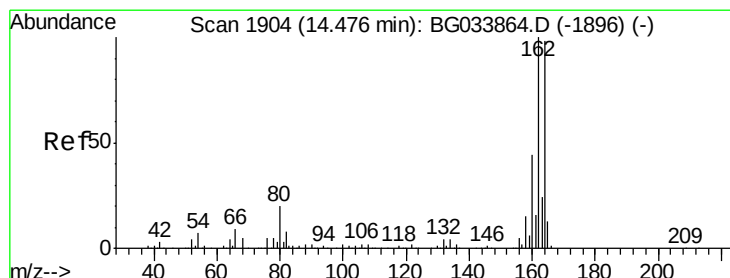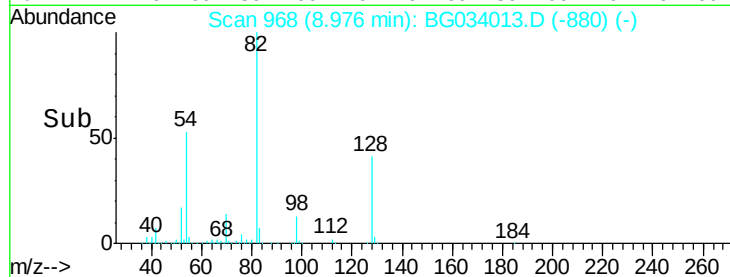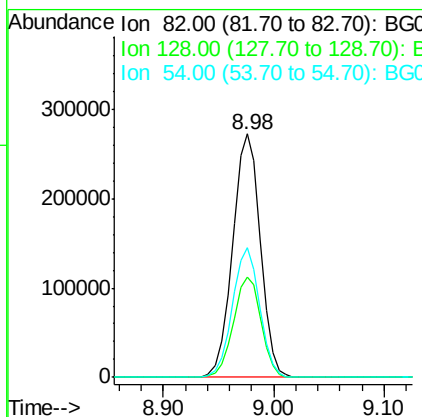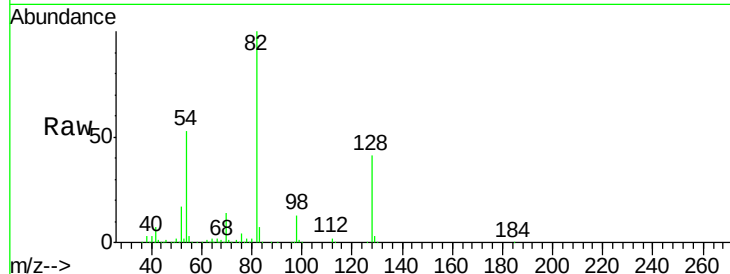

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.46 min Scan# 1901
 Delta R.T. -0.02 min
 Lab File: BG034013.D
 Acq: 26 Apr 2018 8:32

Tgt Ion	164	Resp	177145
Ion Ratio	Lower	Upper	
164	100		
162	99.7	78.8	118.2
160	45.9	35.4	53.0

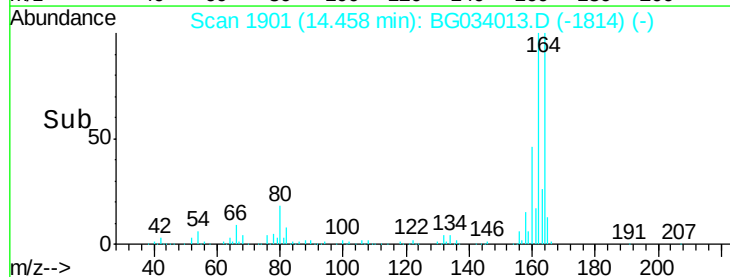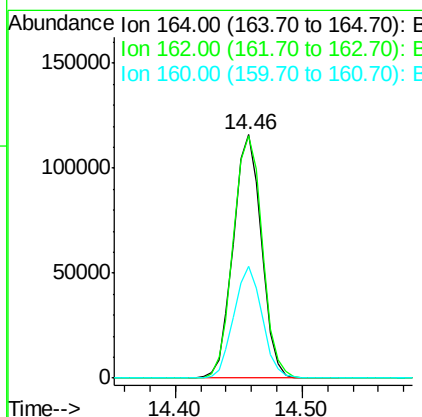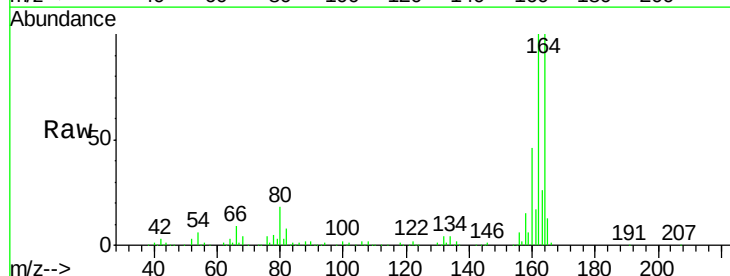


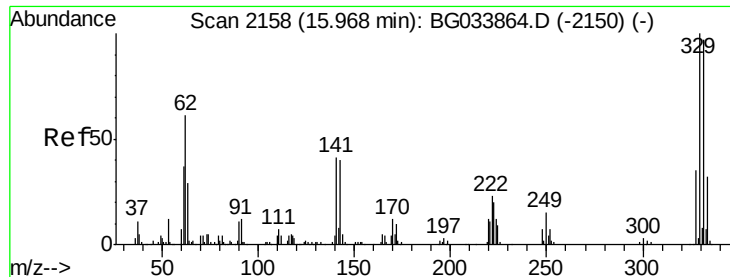




#41
 2,4,6-Tribromophenol
 Concen: 192.345 ng
 RT: 15.95 min Scan# 2155
 Delta R.T. -0.02 min
 Lab File: BG034013.D
 Acq: 26 Apr 2018 8:32

Instrument :
 BNA_G
 ClientSampleId :
 TP-3-4-5-WC-1

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.3	77.0	115.6
141	37.0	25.2	37.8

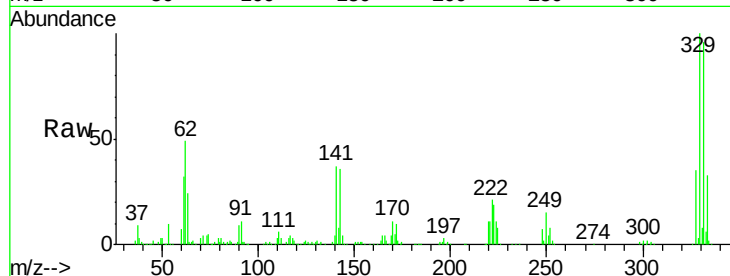


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

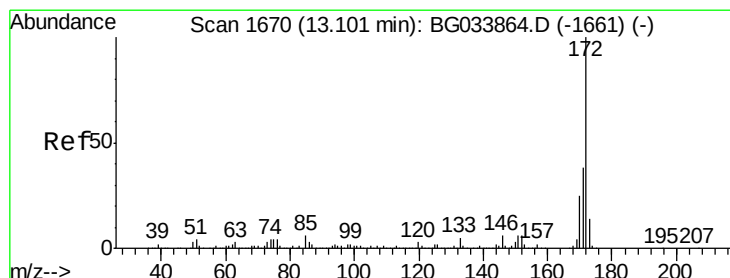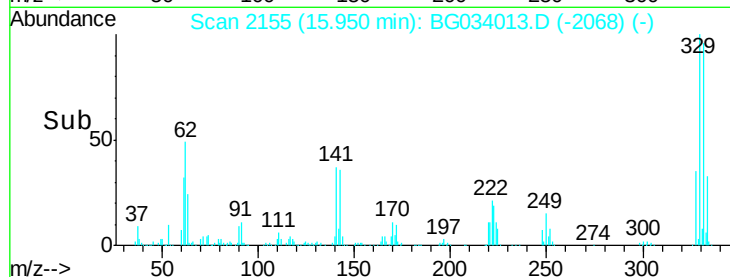
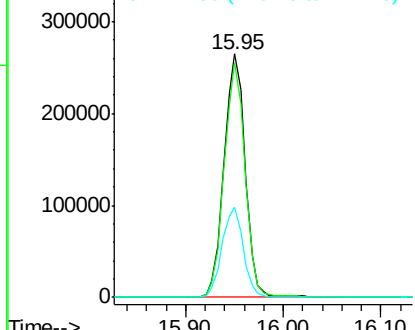



#44
 2-Fluorobiphenyl
 Concen: 101.851 ng
 RT: 13.08 min Scan# 1666
 Delta R.T. -0.02 min
 Lab File: BG034013.D
 Acq: 26 Apr 2018 8:32

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.3	30.0	45.0
170	25.5	19.5	29.3

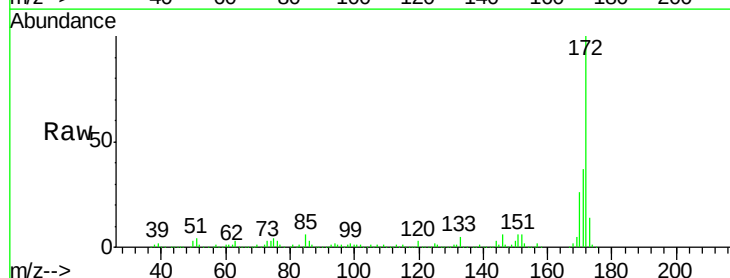

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

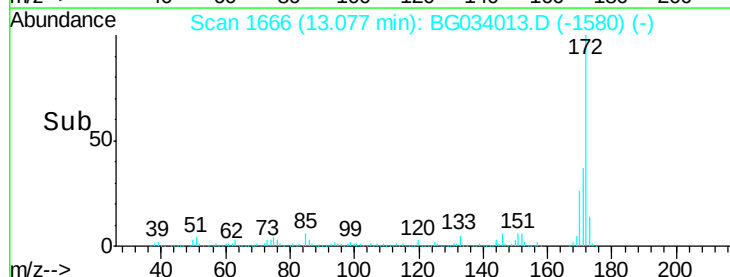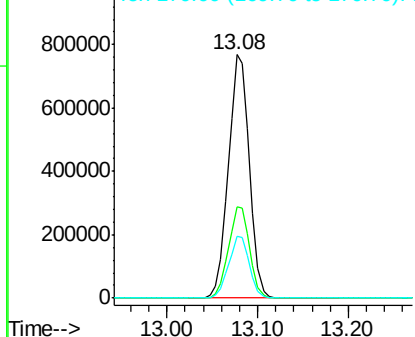


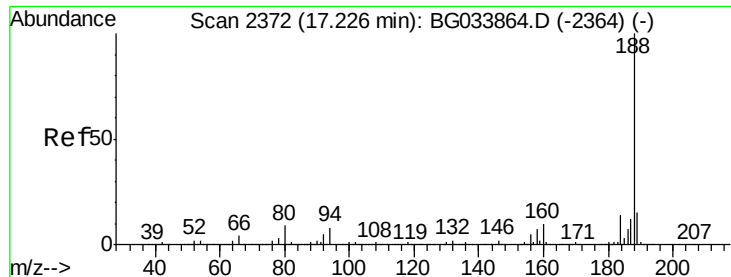




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.21 min Scan# 2369
Delta R.T. -0.02 min
Lab File: BG034013.D
Acq: 26 Apr 2018 8:32

Instrument :
BNA_G
ClientSampleId :
TP-3-4-5-WC-1

Tot Ion:188 Resp: 496960
Ion Ratio Lower Upper
188 100
94 6.5 6.9 10.3#
80 8.6 7.7 11.5

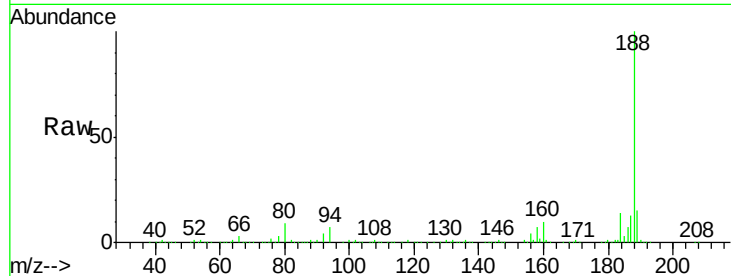


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

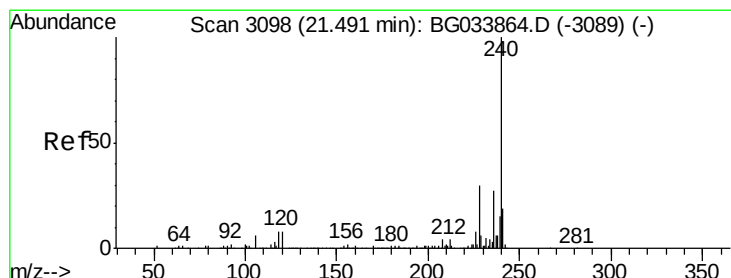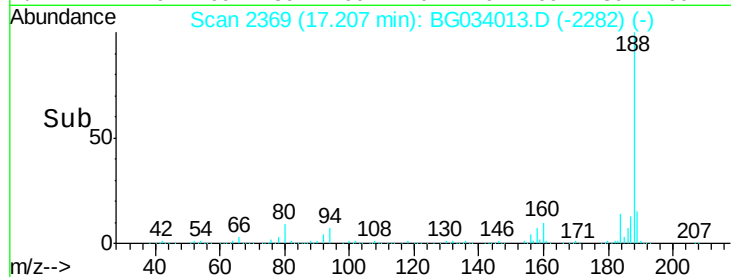
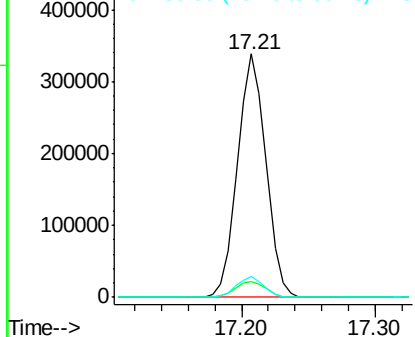



#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.46 min Scan# 3093
Delta R.T. -0.03 min
Lab File: BG034013.D
Acq: 26 Apr 2018 8:32

Tgt Ion:240 Resp: 560743
Ion Ratio Lower Upper
240 100
120 7.8 6.8 10.2
236 26.2 20.9 31.3

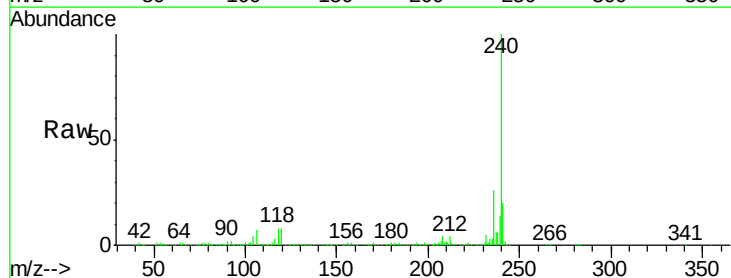

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

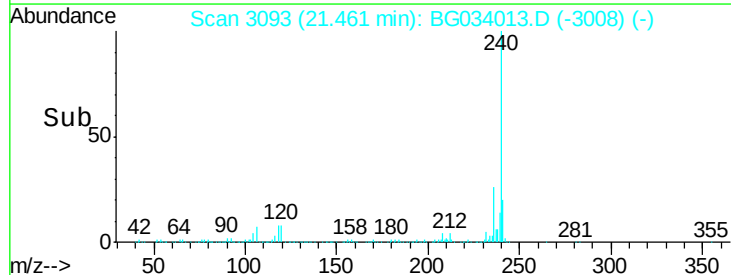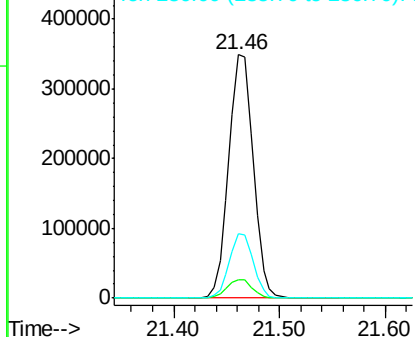

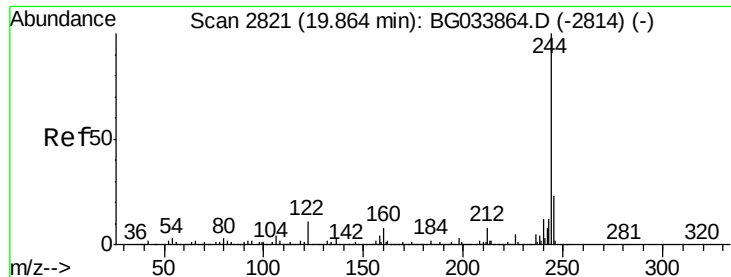

#78

Terphenyl-d14

Concen: 97.722 ng

RT: 19.85 min Scan# 2818

Delta R.T. -0.02 min

Lab File: BG034013.D

Acq: 26 Apr 2018 8:32

Instrument :

BNA_G

ClientSampleId :

TP-3-4-5-WC-1


Tot Ion:244 Resp: 2439085

Ion Ratio Lower Upper

244 100

212 9.3 5.8 8.8#




122 10.8 7.0 10.4#

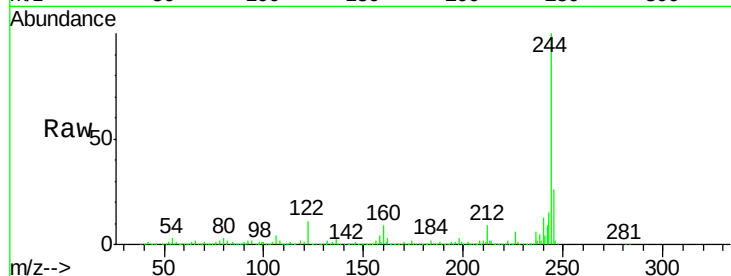

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

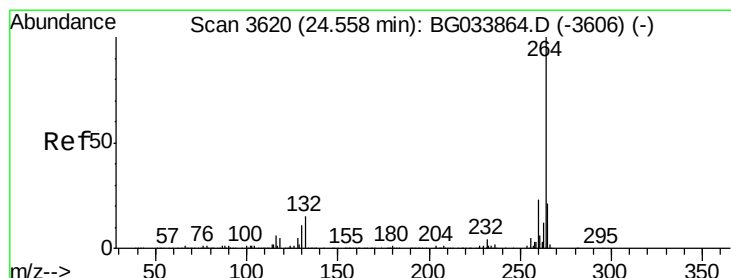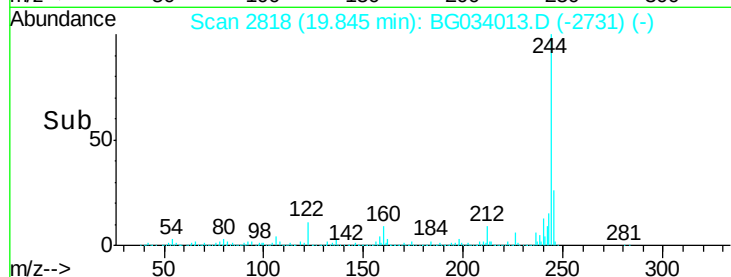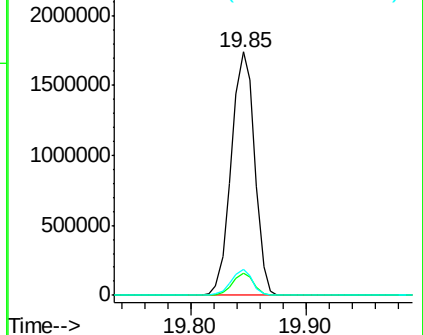

#86

Perylene-d12

Concen: 20.000 ng

RT: 24.52 min Scan# 3613

Delta R.T. -0.04 min

Lab File: BG034013.D

Acq: 26 Apr 2018 8:32


Tgt Ion:264 Resp: 551997

Ion Ratio Lower Upper

264 100

260 23.9 17.4 26.0

265 21.7 17.7 26.5

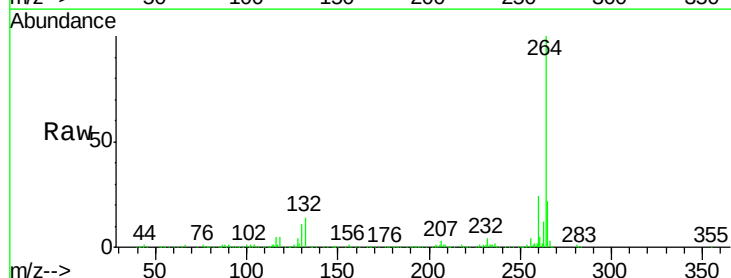

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

