


Data Path : Z:\HPCHEM1\BNA G\Data\BG042518\
 Data File : BG033984.D
 Acq On : 25 Apr 2018 13:25
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

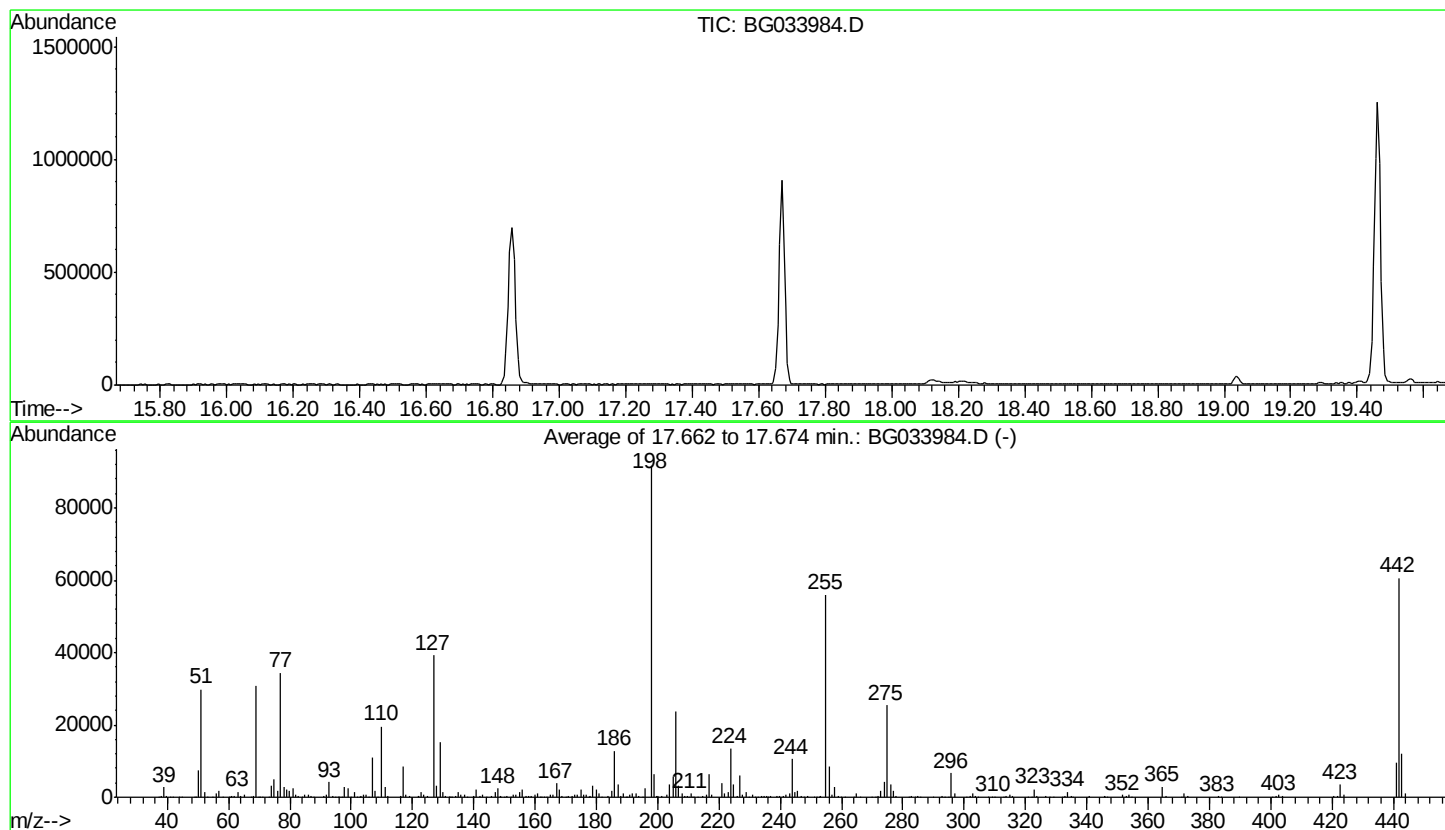

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	29914	PASS
68	69	0.00	2	0.9	279	PASS
69	198	0.00	100	33.5	30743	PASS
70	69	0.00	2	0.5	159	PASS
127	198	10	80	42.8	39232	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	91698	PASS
199	198	5	9	6.9	6294	PASS
275	198	10	60	27.7	25416	PASS
365	198	1	100	3.2	2943	PASS
441	443	0.01	100	79.8	9507	PASS
442	198	50	100	66.1	60624	PASS
443	442	15	24	19.7	11916	PASS