


Data Path : Z:\HPCHEM1\BNA G\Data\BG042518\
 Data File : BG034003.D
 Acq On : 26 Apr 2018 2:06
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

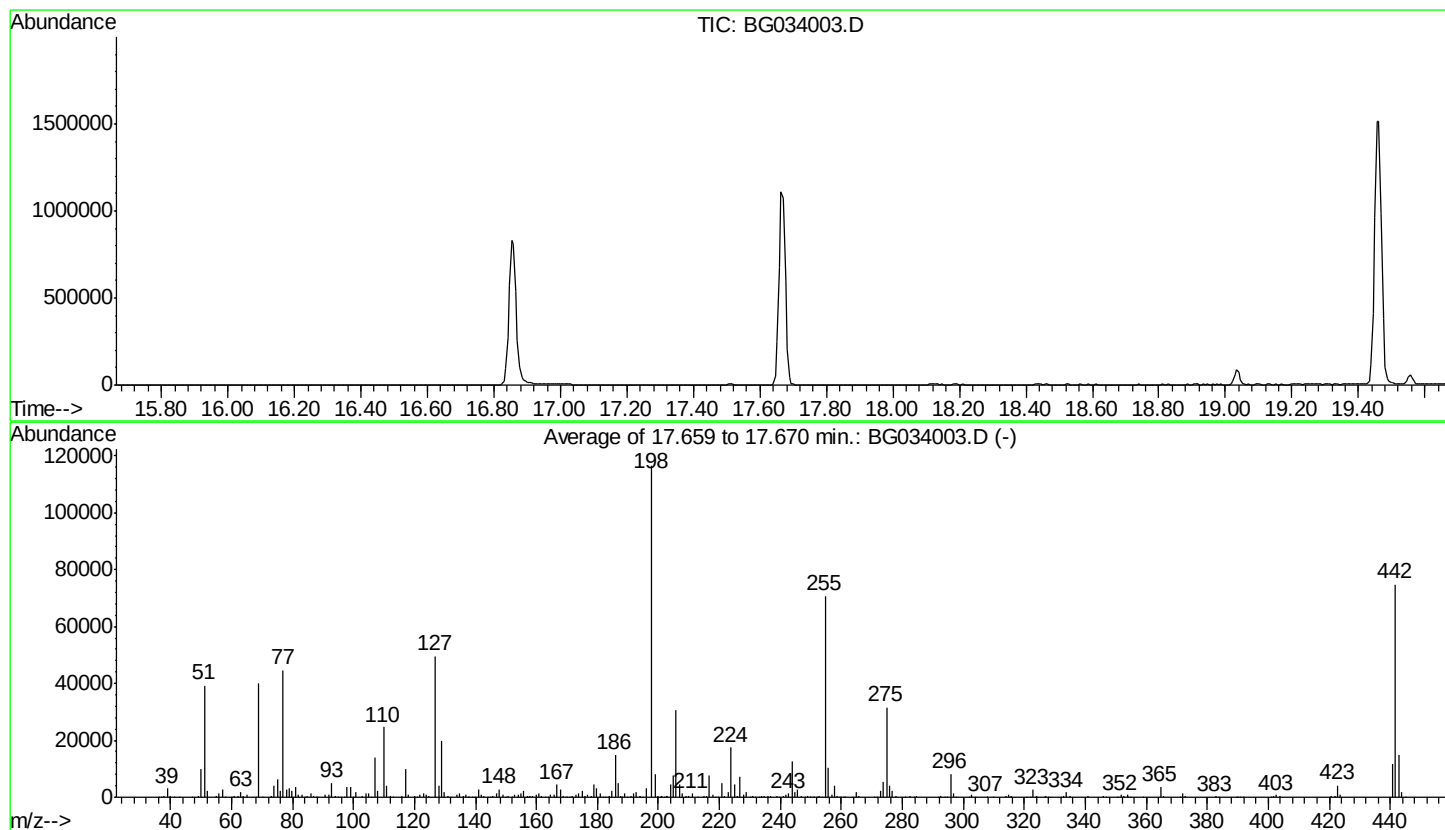

AutoFind: Scans 2446, 2447, 2448; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	39346	PASS
68	69	0.00	2	0.6	231	PASS
69	198	0.00	100	34.5	40189	PASS
70	69	0.00	2	0.6	236	PASS
127	198	10	80	42.7	49720	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	116560	PASS
199	198	5	9	7.1	8221	PASS
275	198	10	60	27.1	31578	PASS
365	198	1	100	3.2	3714	PASS
441	443	0.01	100	79.5	11816	PASS
442	198	50	100	64.2	74877	PASS
443	442	15	24	19.9	14865	PASS