
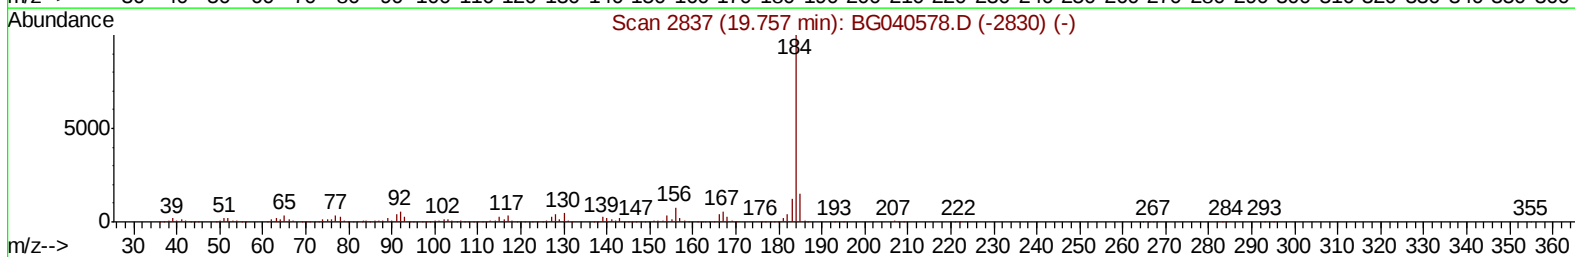
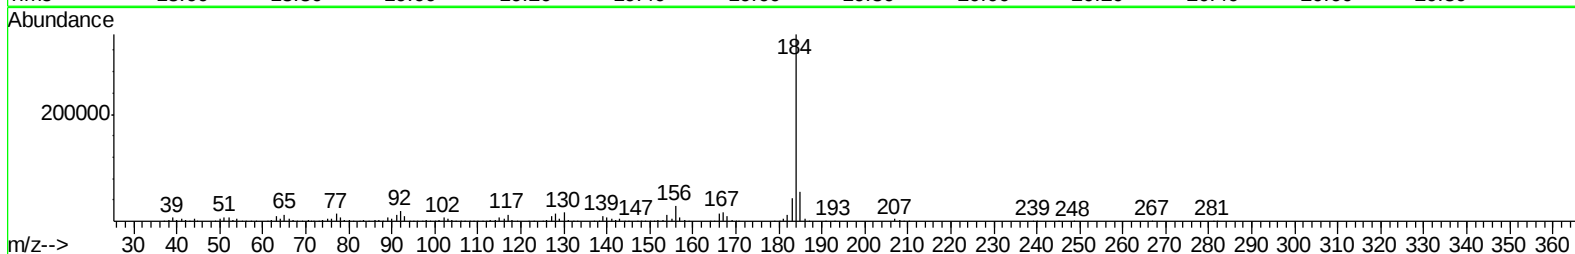


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042519\
 Data File : BG040603.D
 Acq On : 25 Apr 2019 9:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:51:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

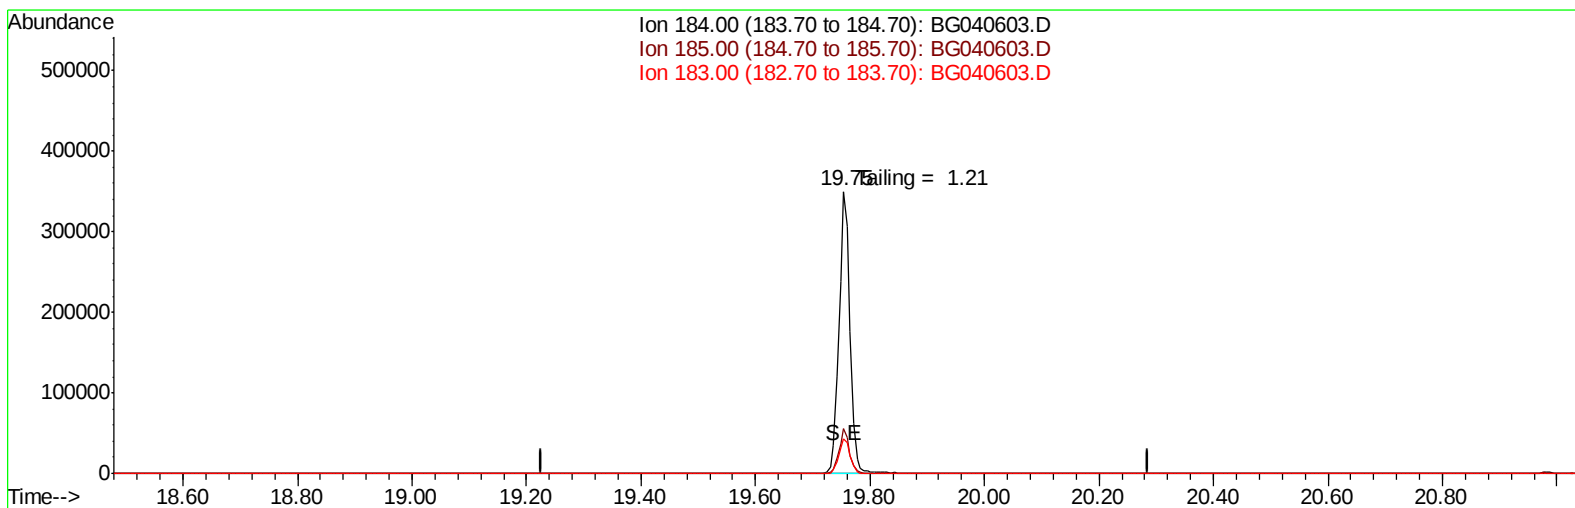

TIC: BG040603.D

(77) Benzidine




19.757min (-19.757) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	14.80	0.00#
183.00	12.70	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042519\
Data File : BG040603.D
Acq On : 25 Apr 2019 9:49
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:51:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

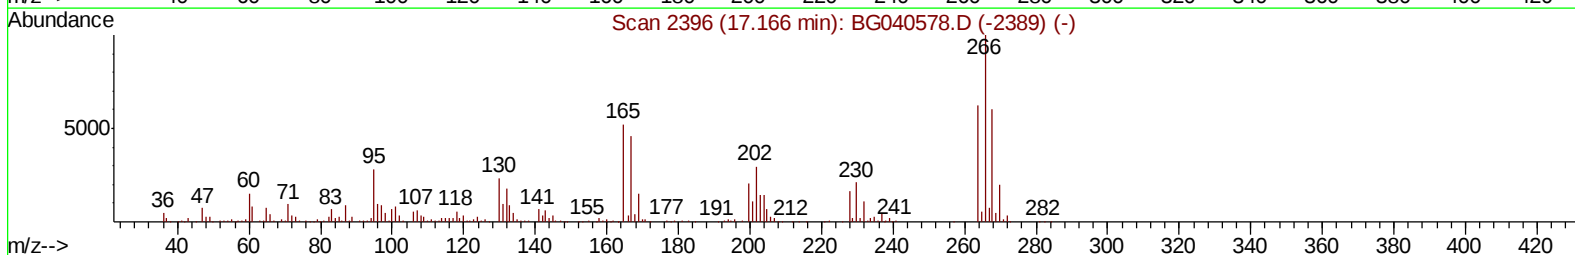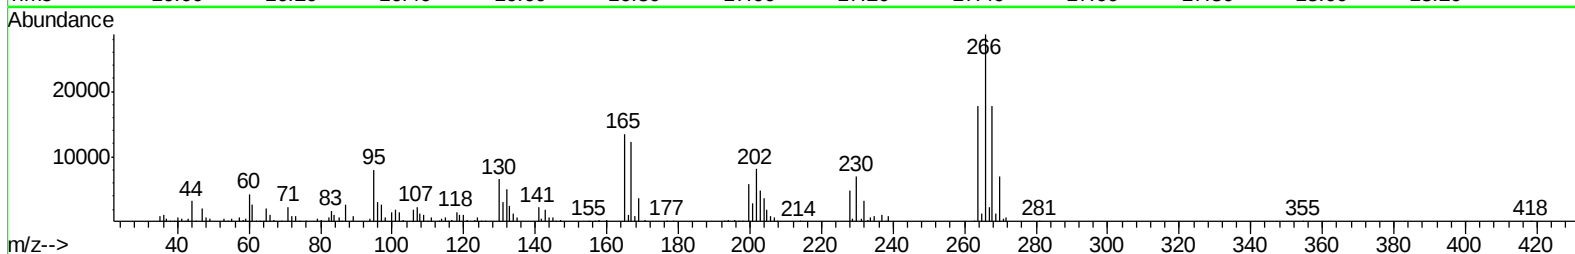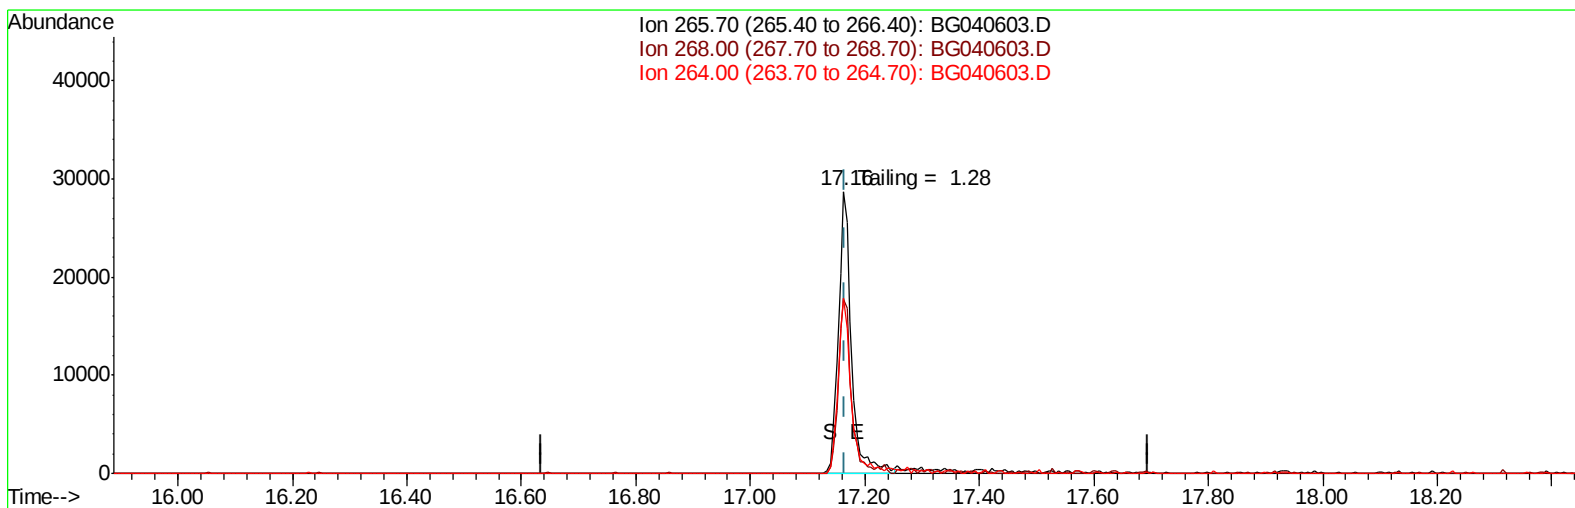

TIC: BG040603.D

(70) Pentachlorophenol (C)

17.163min (-0.003) 12652.09ng

response 45780

Ion	Exp%	Act%
265.70	100	100
268.00	65.40	62.00
264.00	62.50	62.11
0.00	0.00	0.00