


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042519\
 Data File : BG040603.D
 Acq On : 25 Apr 2019 9:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

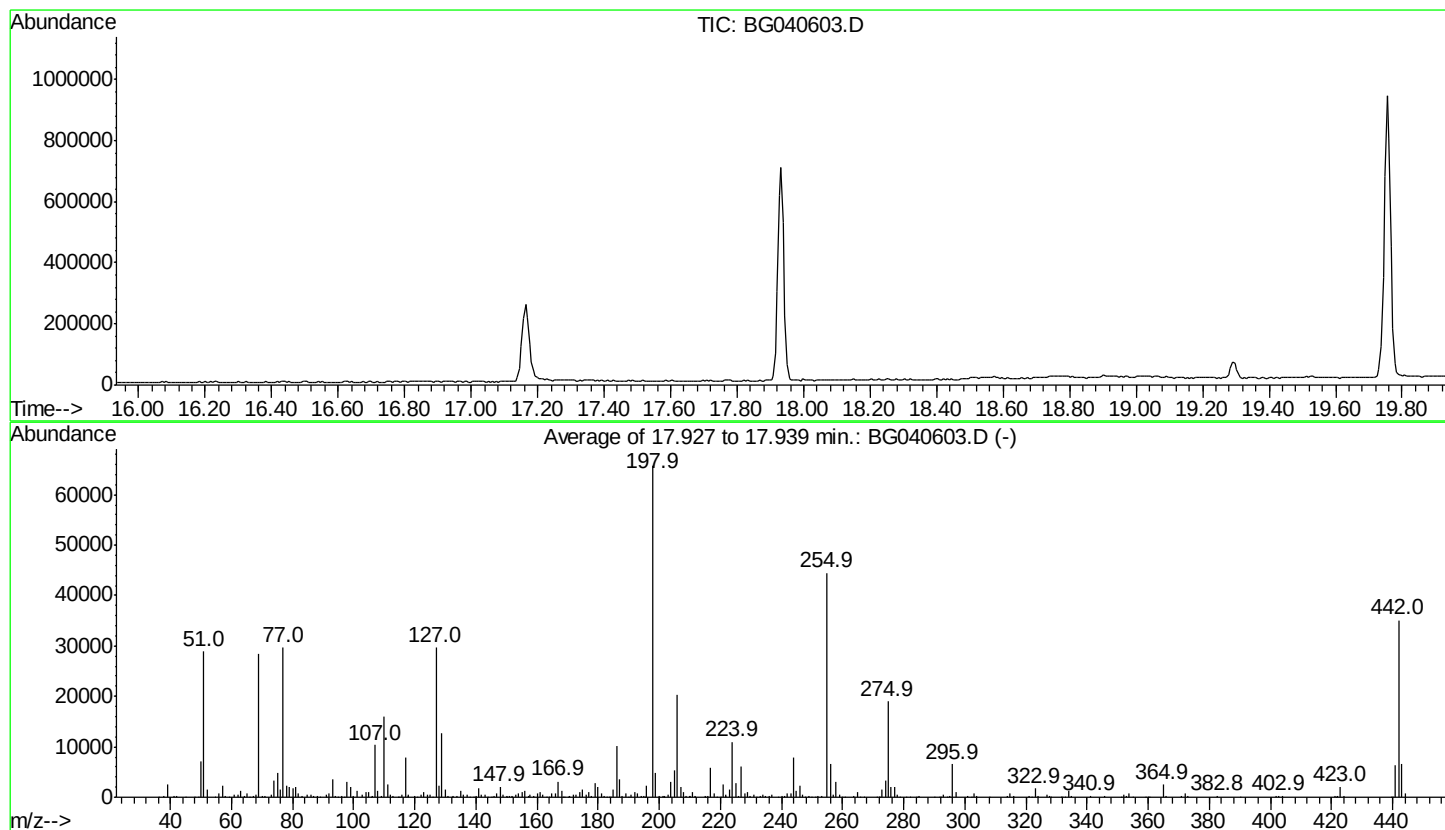

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	28925	PASS
68	69	0.00	2	1.6	446	PASS
69	198	0.00	100	43.3	28483	PASS
70	69	0.00	2	0.9	263	PASS
127	198	10	80	45.0	29584	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65765	PASS
199	198	5	9	7.5	4950	PASS
275	198	10	60	28.8	18973	PASS
365	198	1	100	3.8	2489	PASS
441	198	0.01	100	9.6	6335	PASS
442	198	50	100	53.4	35130	PASS
443	442	15	24	19.1	6720	PASS