
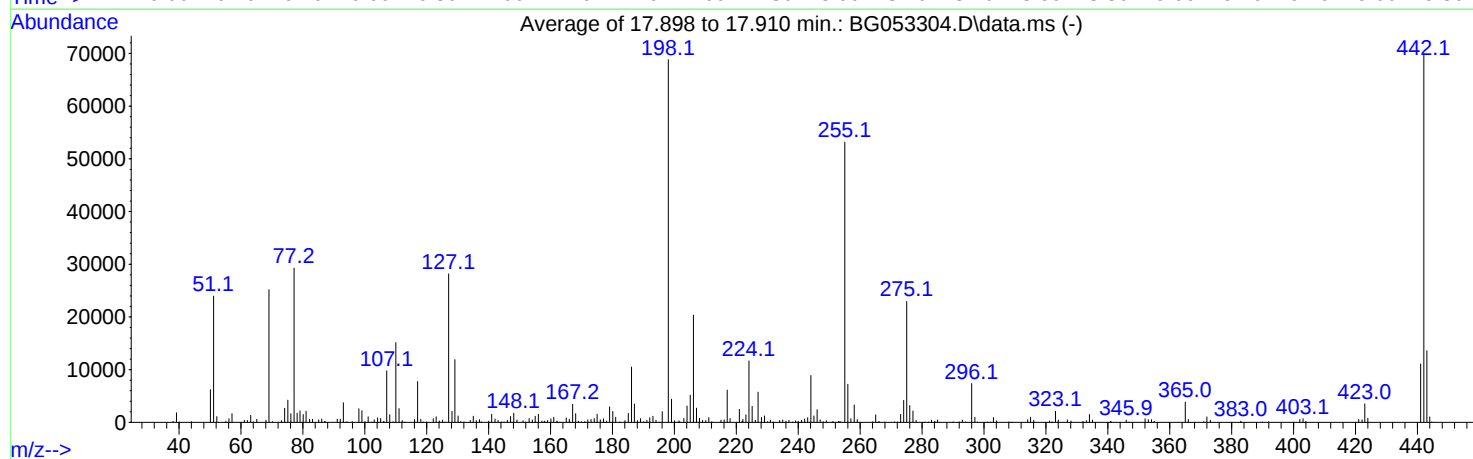


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042522\
 Data File : BG053304.D
 Acq On : 25 Apr 2022 11:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Apr 24 01:13:30 2022

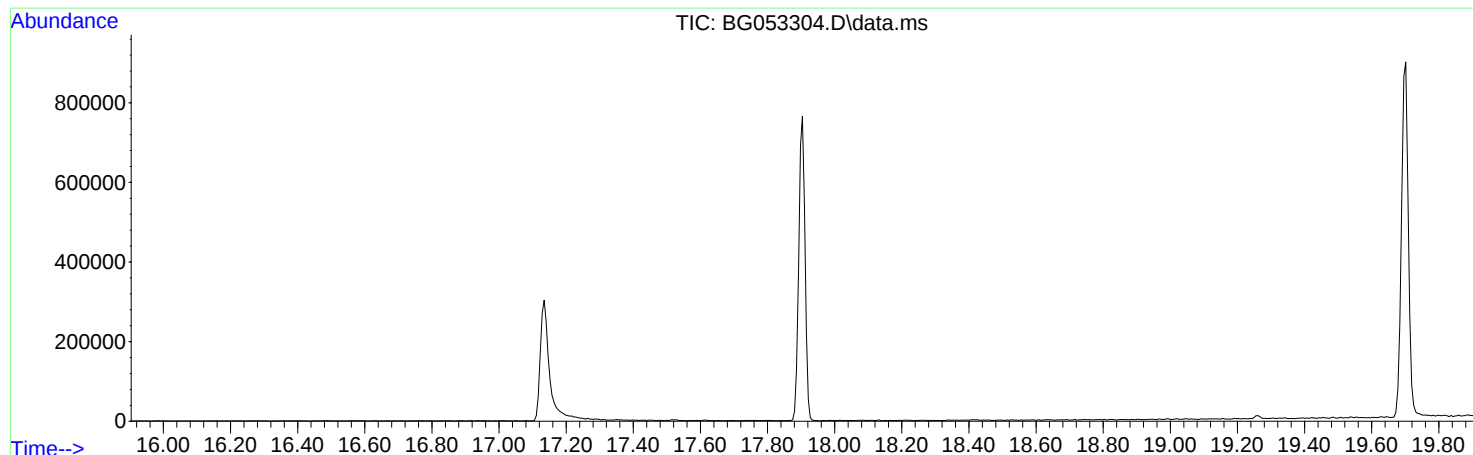




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	23949	PASS
68	69	0.00	2	1.7	418	PASS
69	198	0.00	100	36.6	25173	PASS
70	69	0.00	2	0.5	114	PASS
127	198	10	80	40.9	28187	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68837	PASS
199	198	5	9	6.4	4389	PASS
275	198	10	60	33.3	22955	PASS
365	198	1	100	5.6	3869	PASS
441	198	0.01	100	16.1	11081	PASS
442	442	50	100	100.0	69800	PASS
443	442	15	24	19.5	13611	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042522\
Data File : BG053304.D
Acq On : 25 Apr 2022 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 25 18:31:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

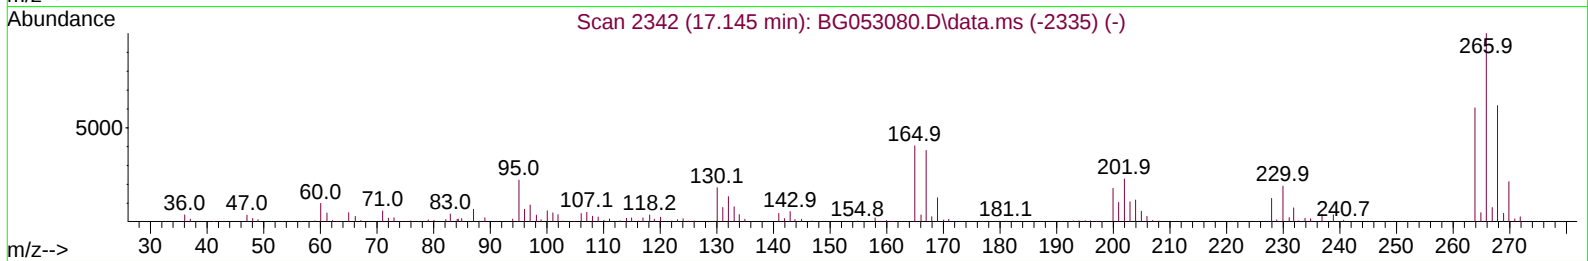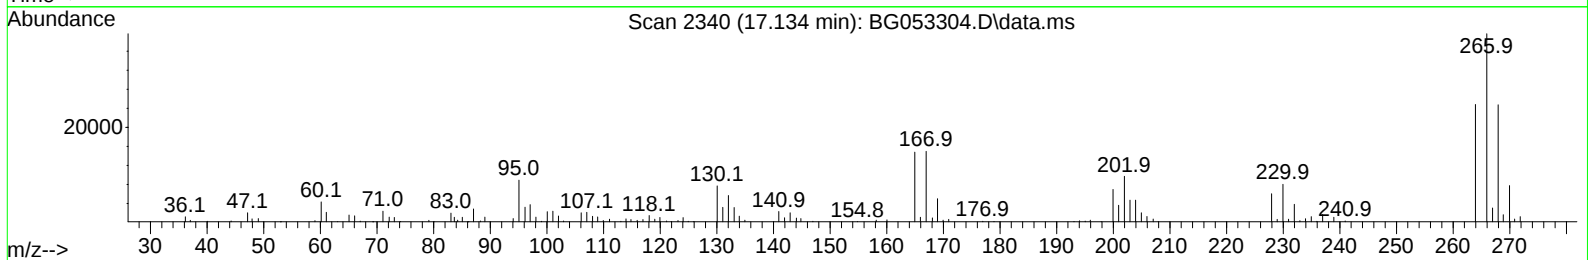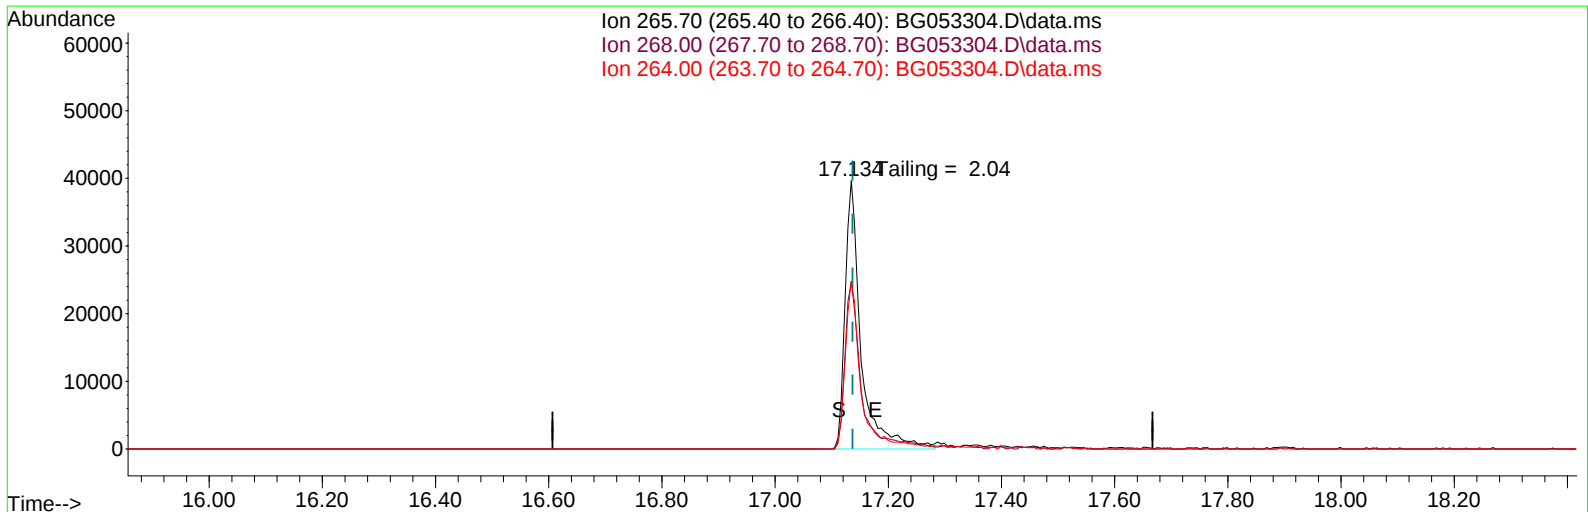

TIC: BG053304.D\data.ms

(70) Pentachlorophenol (C)

17.134min (-0.002) 38711.28 ng




response 77505

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	62.38
264.00	56.60	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042522\
Data File : BG053304.D
Acq On : 25 Apr 2022 11:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 25 18:31:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG040822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Apr 24 01:13:30 2022
Response via : Initial Calibration

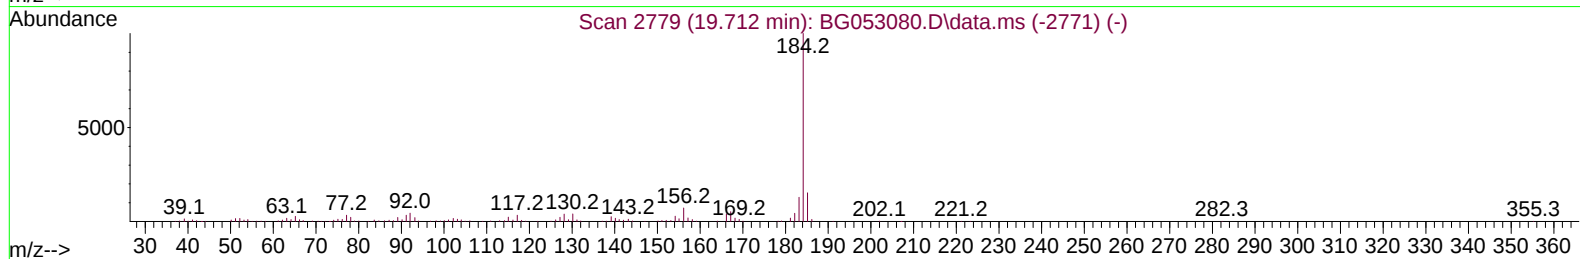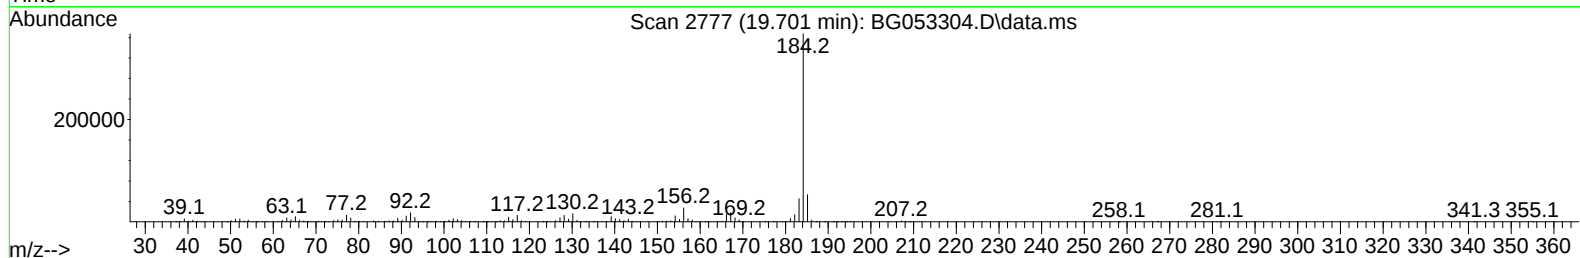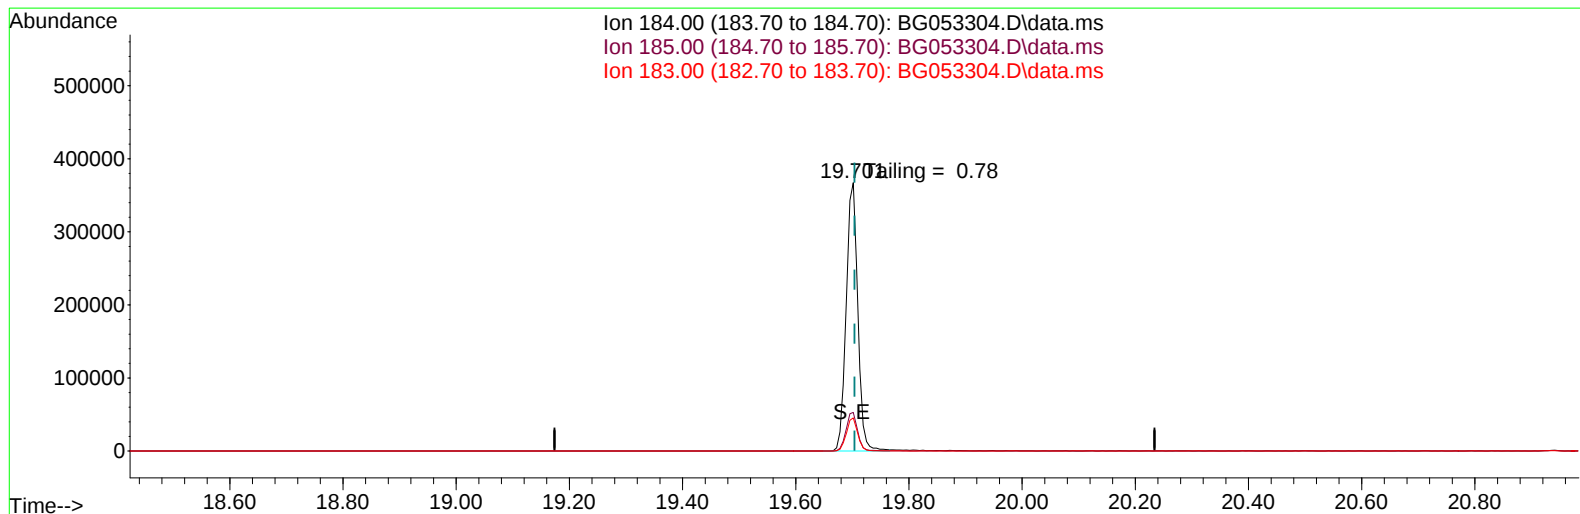

TIC: BG053304.D\data.ms

(77) Benzidine

19.701min (-0.002) 313583.36 ng

response 527875

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.38
183.00	11.80	12.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/25/2022	BNA_G	<u>BG053304.D</u>
Compound Name	Response	Retention Time
DDT	236663	20.93
DDD	1068	20.48
DDE	122	19.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1190	237853	0.50