
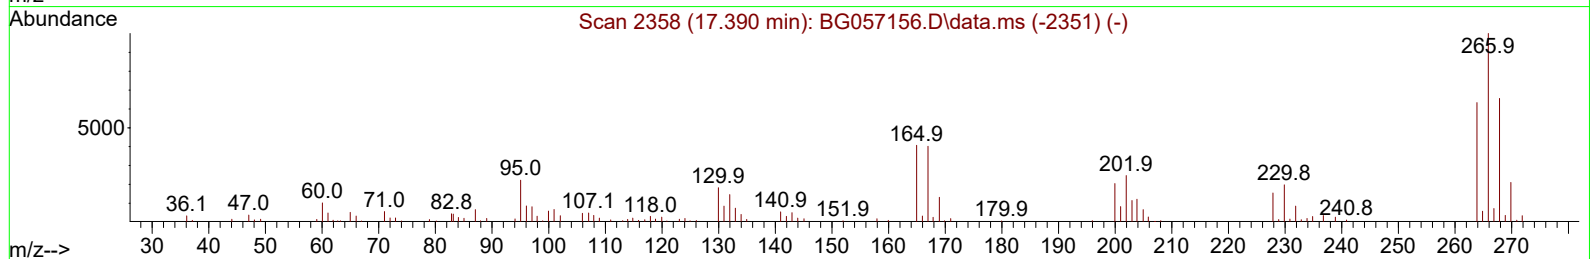
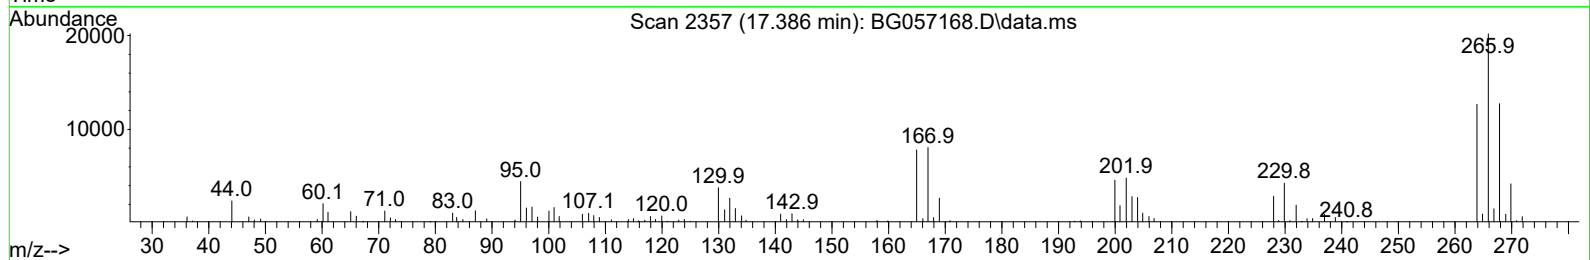


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042523\
Data File : BG057168.D
Acq On : 25 Apr 2023 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 00:15:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 04:59:02 2023
Response via : Initial Calibration

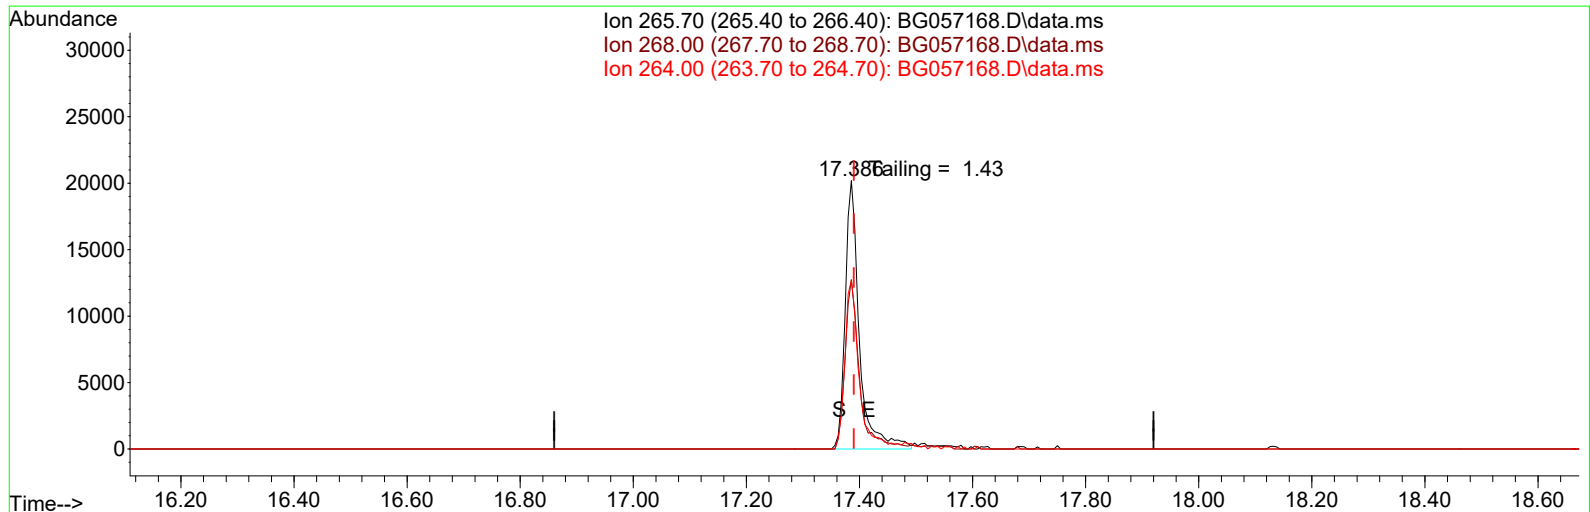

TIC: BG057168.D\data.ms

(70) Pentachlorophenol (C)




17.386min (-0.004) 42996.52 ng m

response 35143

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	63.09
264.00	63.40	62.74
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042523\  
Data File : BG057168.D  
Acq On    : 25 Apr 2023    9:06  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 26 00:15:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 04:59:02 2023
Response via : Initial Calibration

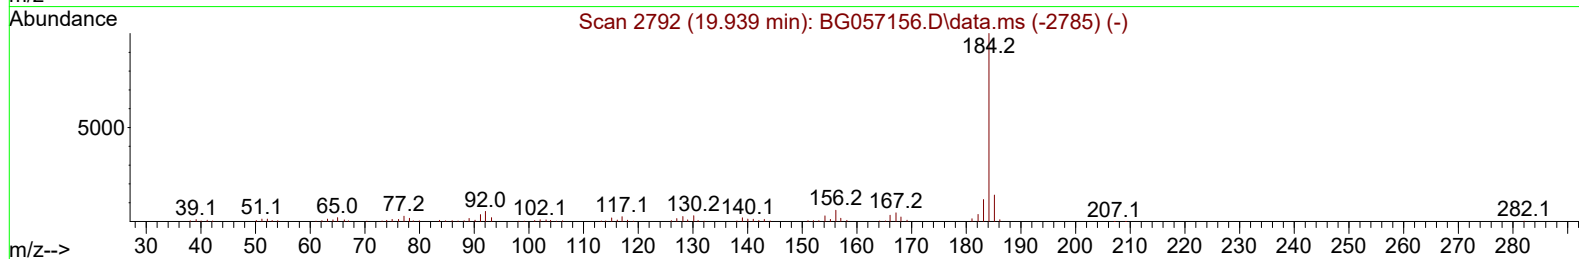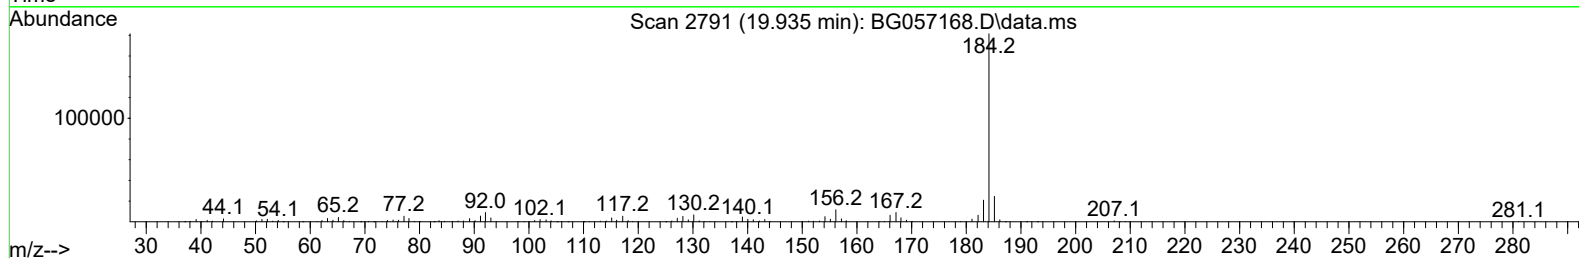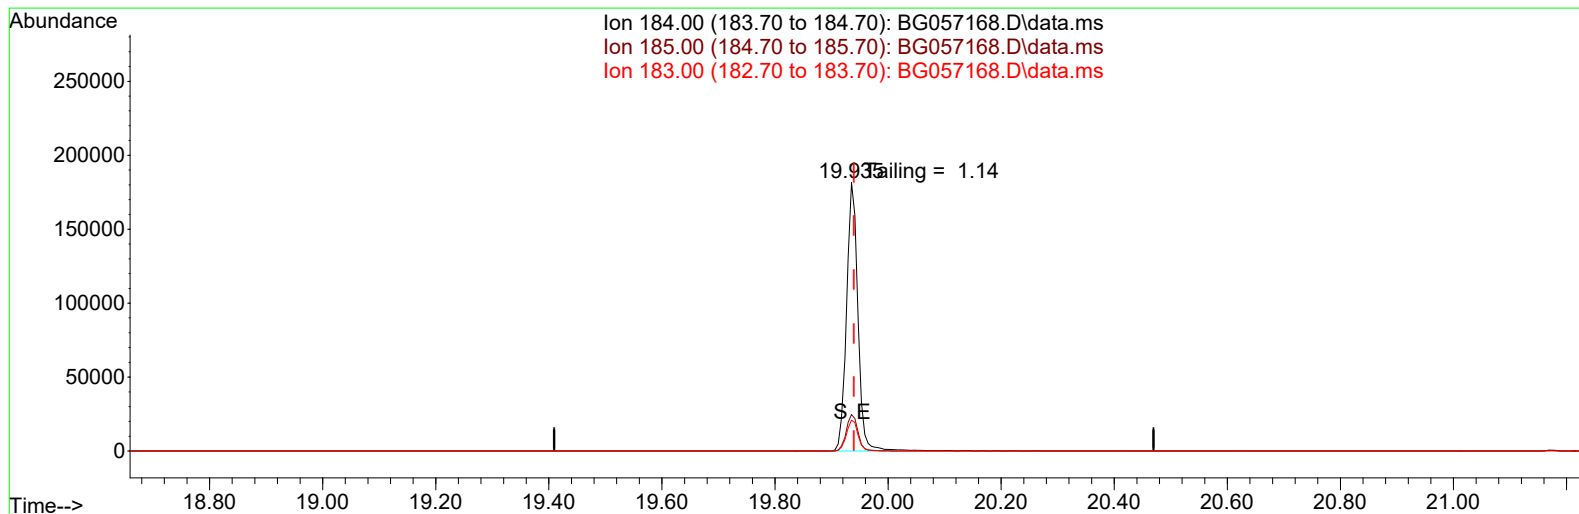

TIC: BG057168.D\data.ms

(77) Benzidine

19.935min (-0.004) 0.00 ng

response **252390**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.63
183.00	11.70	11.53
0.00	0.00	0.00