
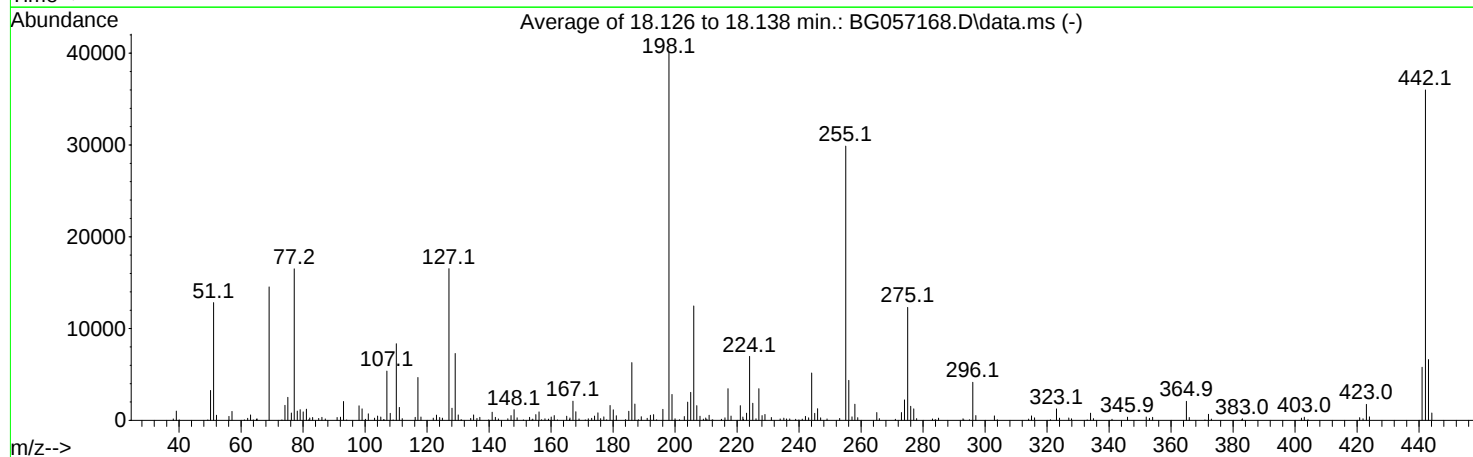


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042523\
Data File : BG057168.D
Acq On : 25 Apr 2023 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Apr 25 04:59:02 2023

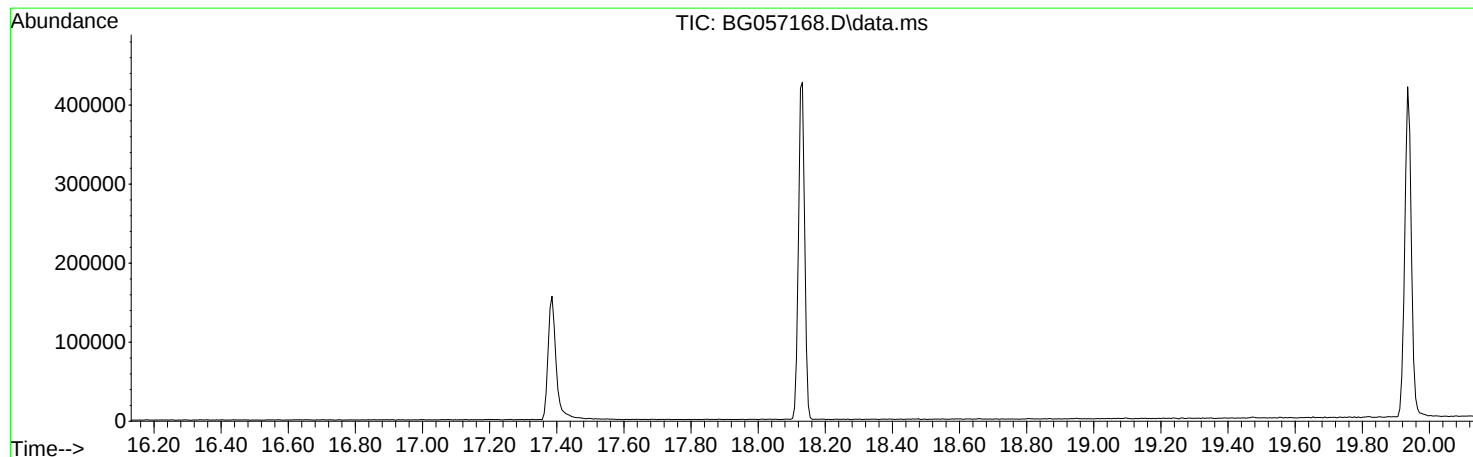




AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	12834	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.3	14533	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.2	16523	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	40077	PASS
199	198	5	9	7.1	2826	PASS
275	198	10	60	30.7	12311	PASS
365	198	1	100	5.2	2080	PASS
441	198	0.01	100	14.5	5796	PASS
442	442	50	100	100.0	35995	PASS
443	442	15	24	18.4	6629	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042523\
Data File : BG057168.D
Acq On : 25 Apr 2023 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 26 00:19:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 04:59:02 2023
Response via : Initial Calibration

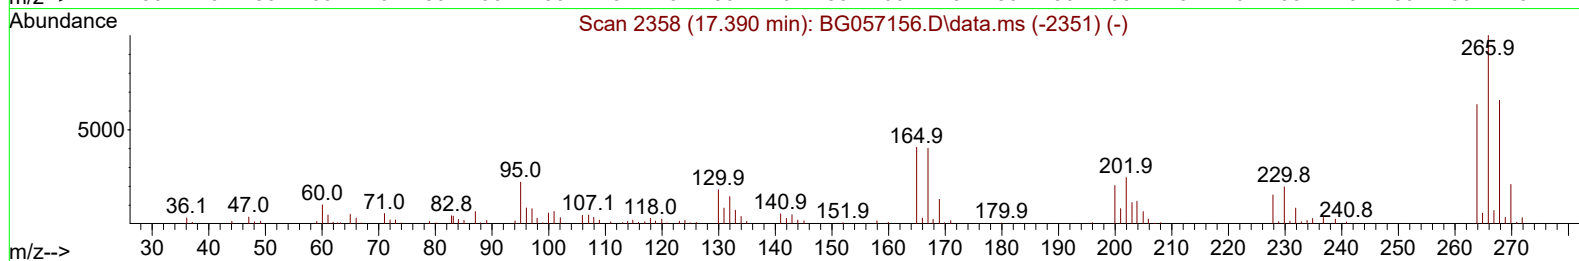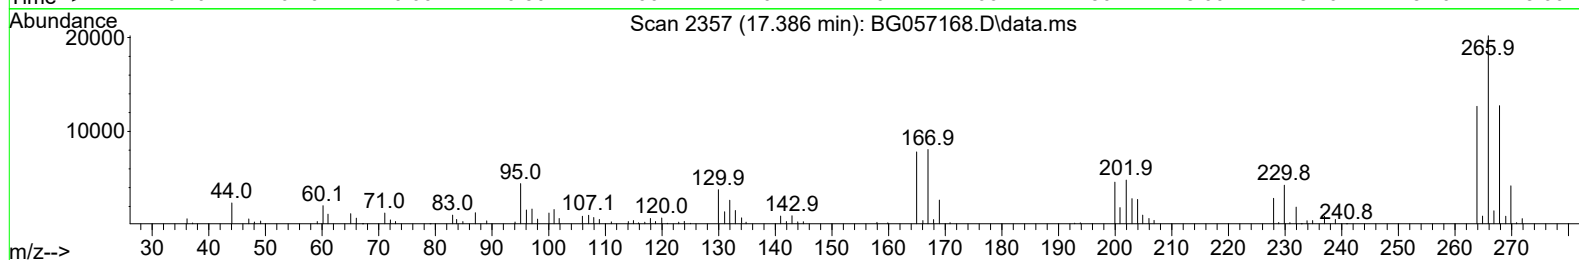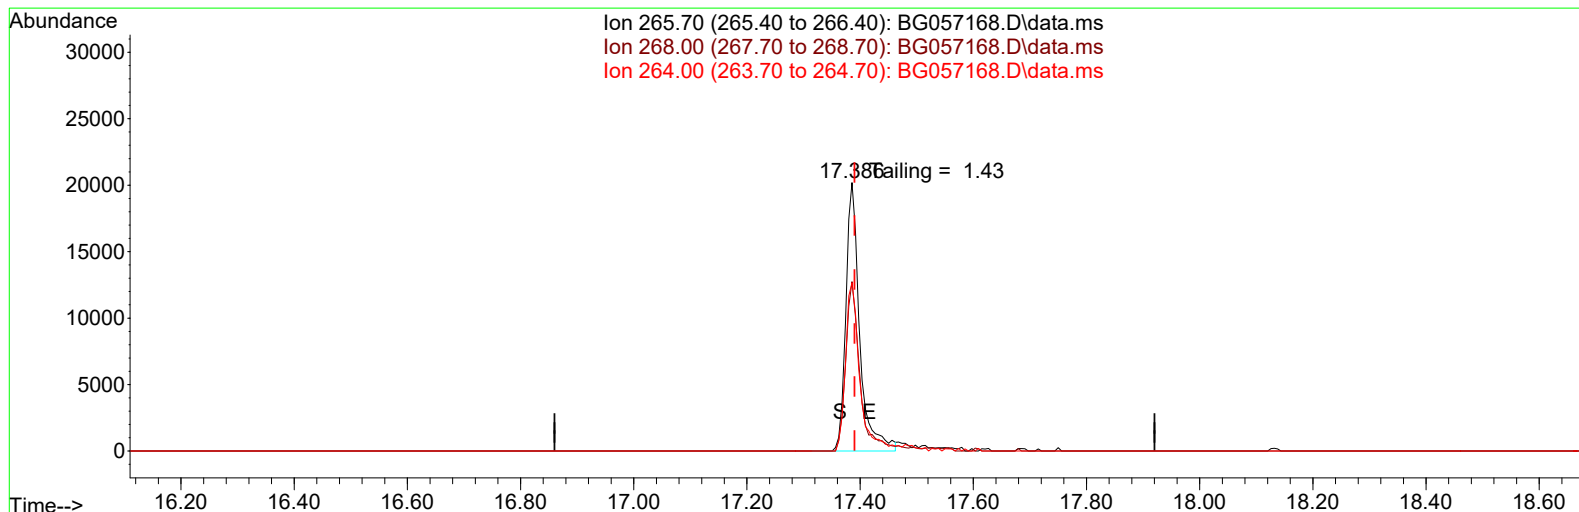

TIC: BG057168.D\data.ms

(70) Pentachlorophenol (C)

17.386min (-0.004) 41284.88 ng




response 33744

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.60	63.09
264.00	63.40	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042523\
Data File : BG057168.D
Acq On : 25 Apr 2023 9:06
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 26 00:19:07 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 25 04:59:02 2023
Response via : Initial Calibration

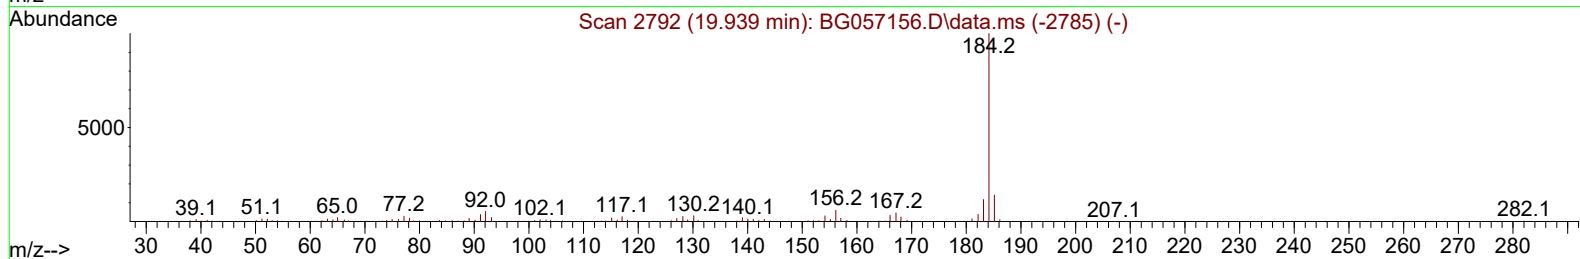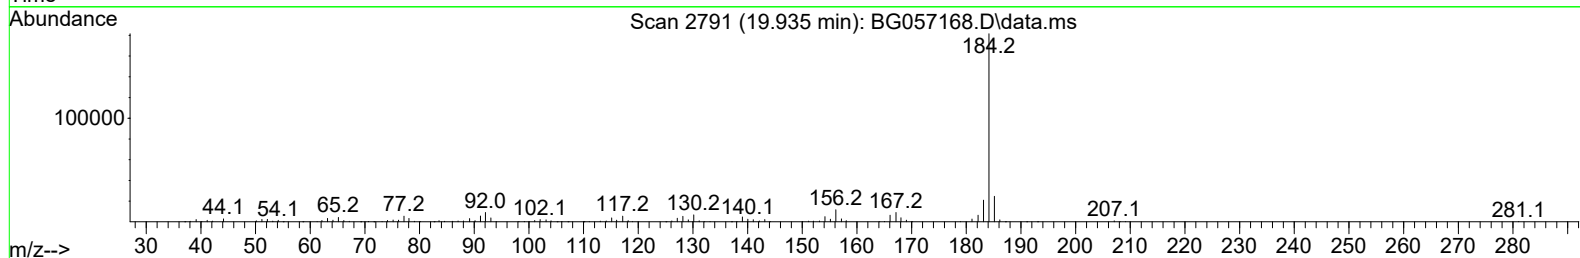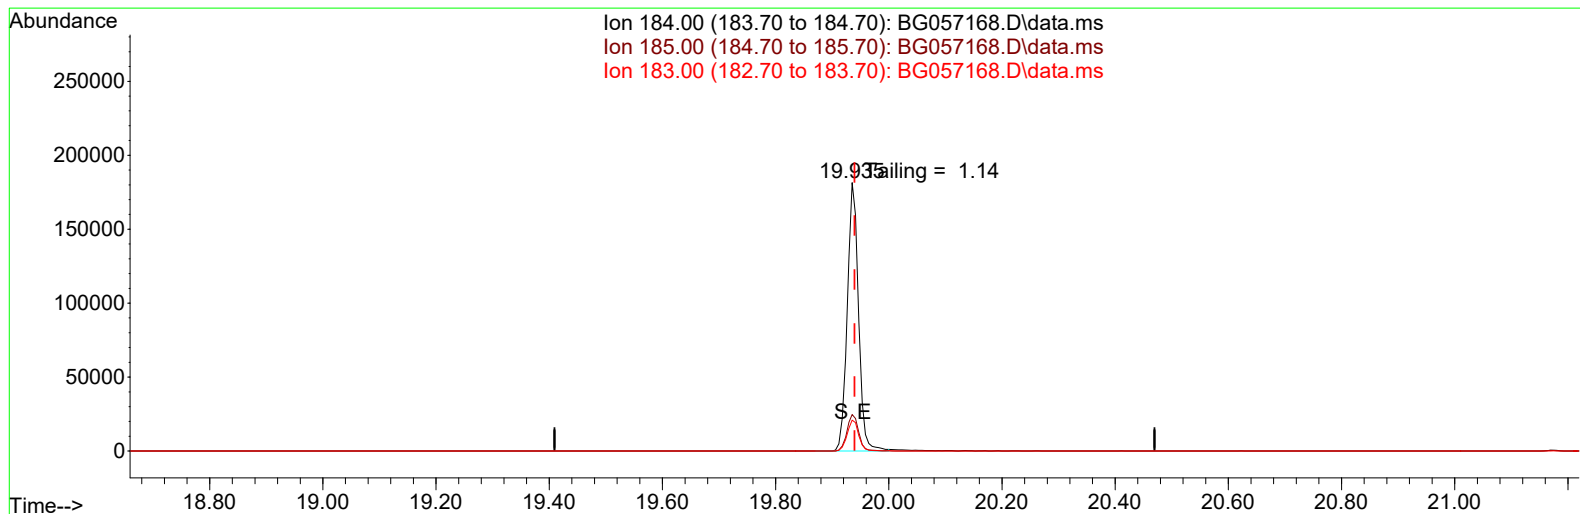

TIC: BG057168.D\data.ms

(77) Benzidine

19.935min (-0.004) 0.00 ng

response 252390

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.63
183.00	11.70	11.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/25/2023	BNA_G	<u>BG057168.D</u>
Compound Name	Response	Retention Time
DDT	114378	21.175
DDD	5431	20.717
DDE	218	20.211
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5649	120027	4.71

Instrument :
BNA_G
ClientSampleId :
DFTPP