


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042524\
Data File : BG061031.D
Acq On : 25 Apr 2024 9:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Apr 22 04:22:00 2024

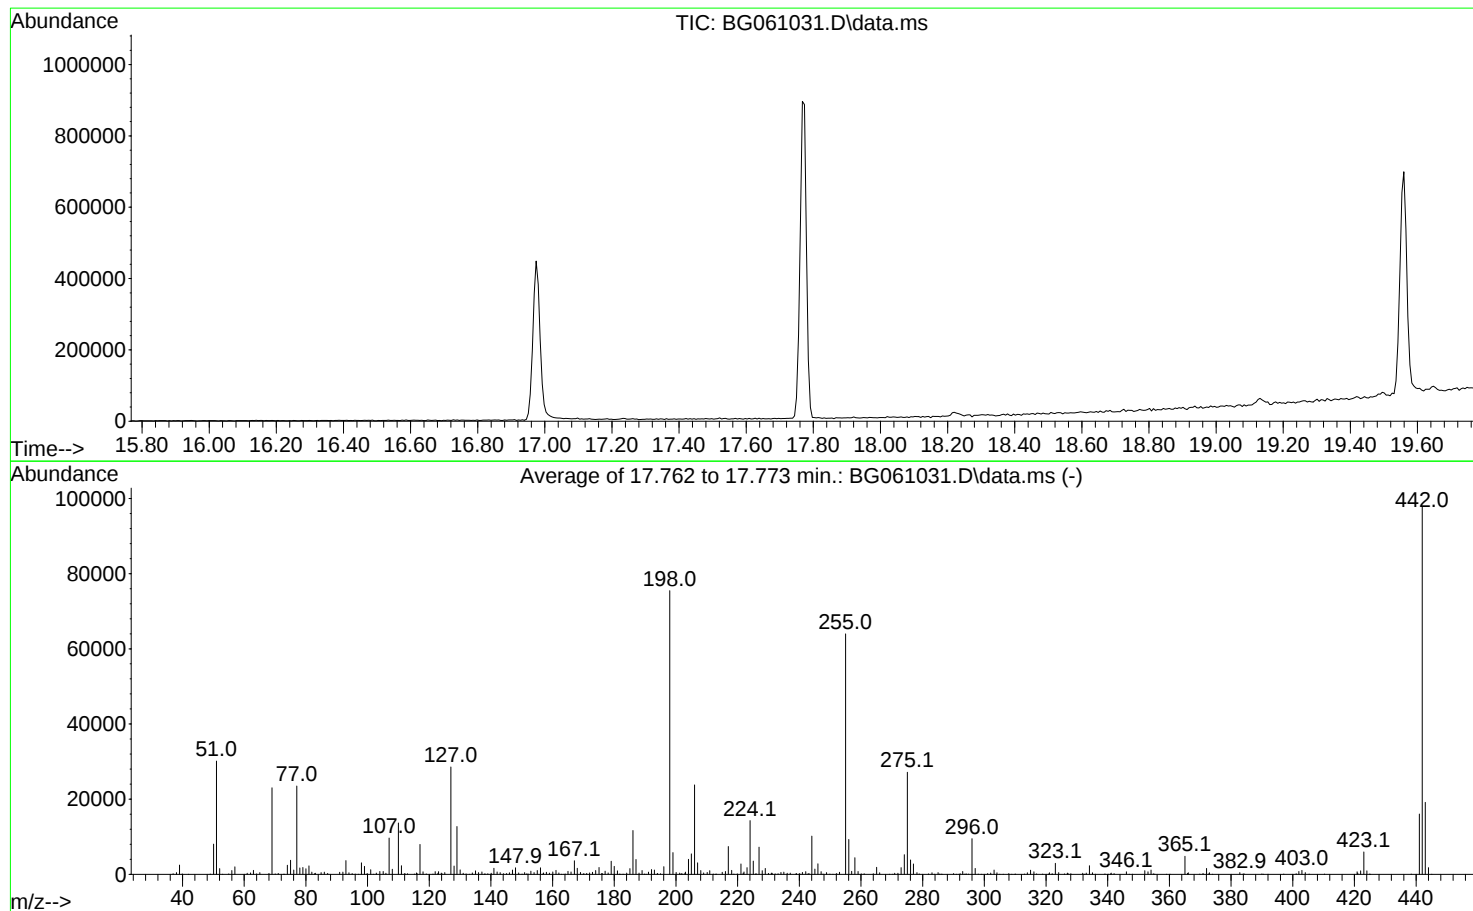




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	30120	PASS
68	69	0.00	2	1.2	268	PASS
69	198	0.00	100	30.5	23041	PASS
70	69	0.00	2	0.5	112	PASS
127	198	10	80	37.8	28557	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75472	PASS
199	198	5	9	7.7	5799	PASS
275	198	10	60	36.0	27141	PASS
365	198	1	100	6.4	4808	PASS
441	198	0.01	100	21.3	16066	PASS
442	442	50	100	100.0	97867	PASS
443	442	15	24	19.6	19146	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042524\
Data File : BG061031.D
Acq On : 25 Apr 2024 9:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 25 12:01:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

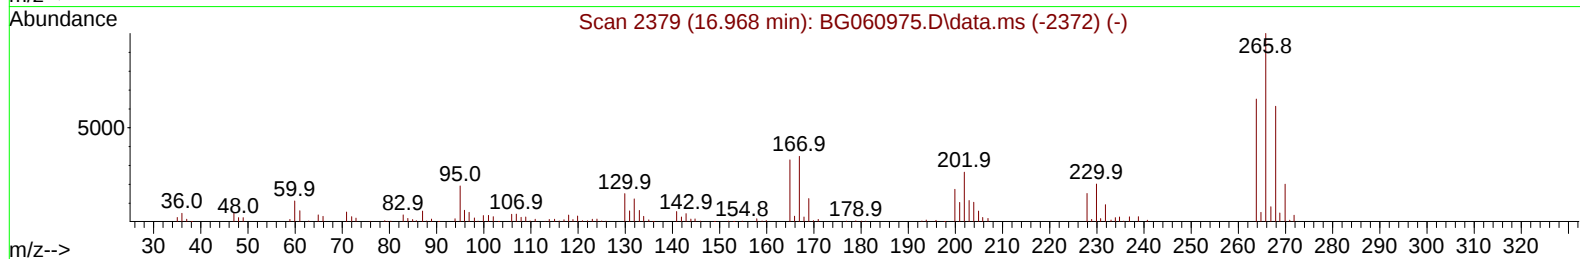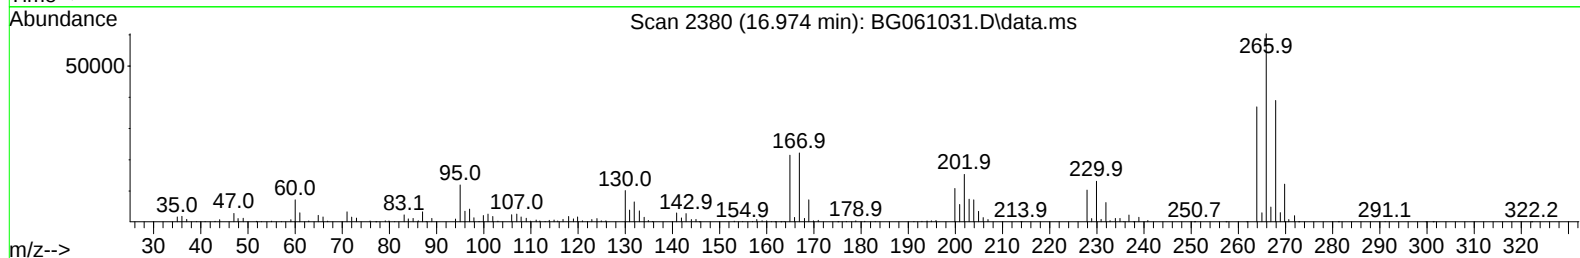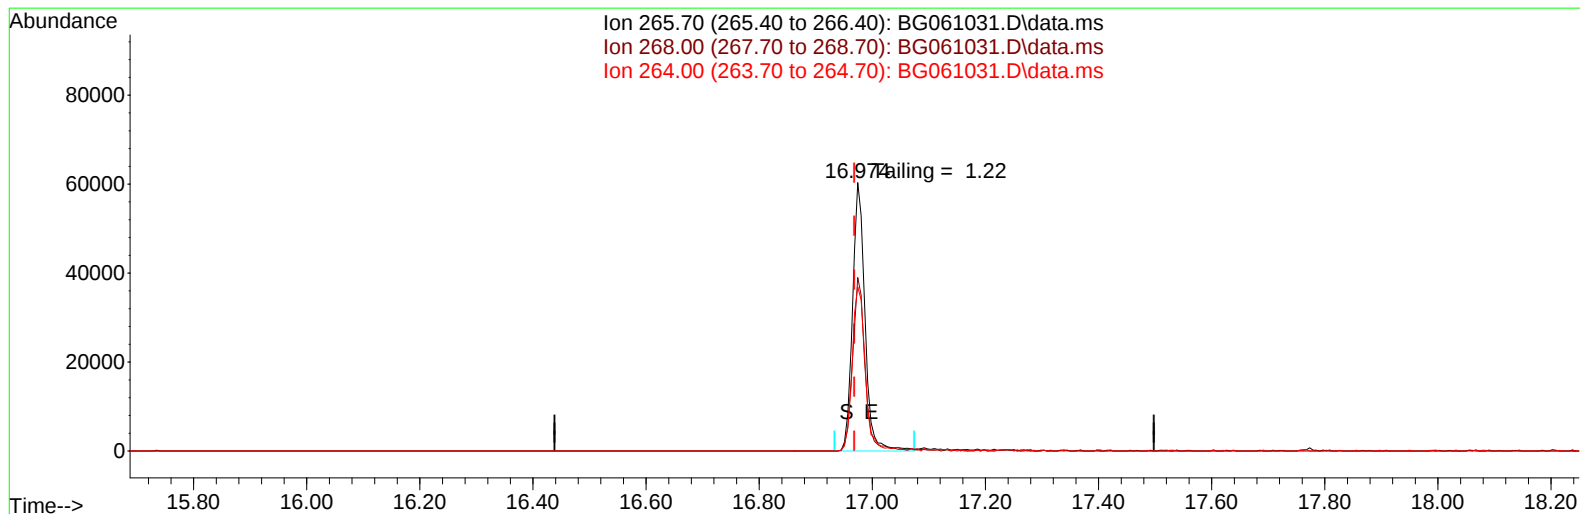

TIC: BG061031.D\data.ms

(70) Pentachlorophenol (C)

16.974min (+ 0.006) 17722.42 ng




response 92666

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.40	64.62
264.00	65.20	61.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042524\
Data File : BG061031.D
Acq On : 25 Apr 2024 9:46
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Apr 25 12:01:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG042024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 22 04:22:00 2024
Response via : Initial Calibration

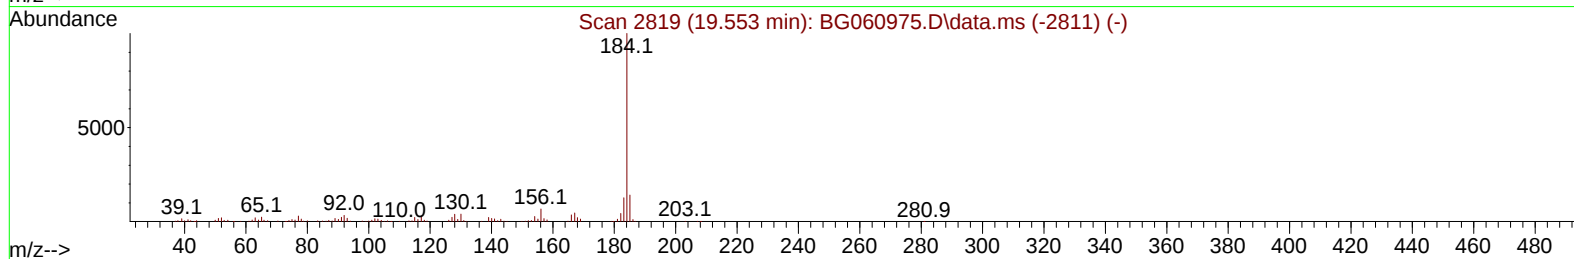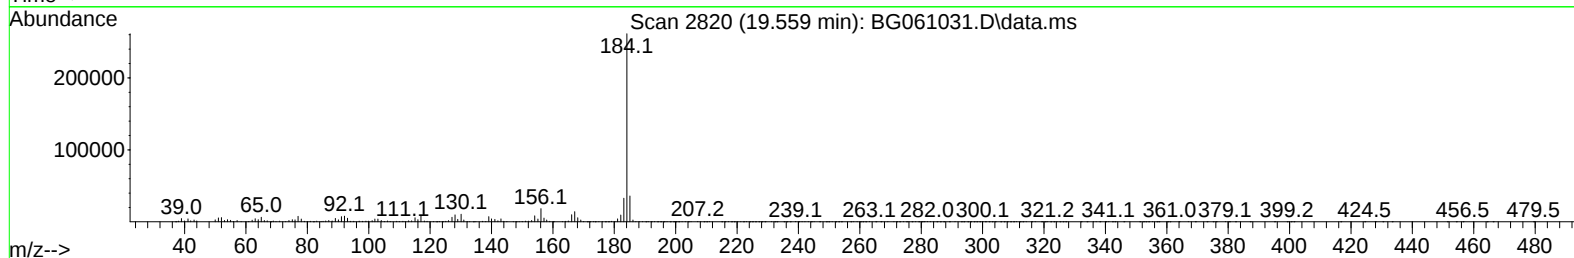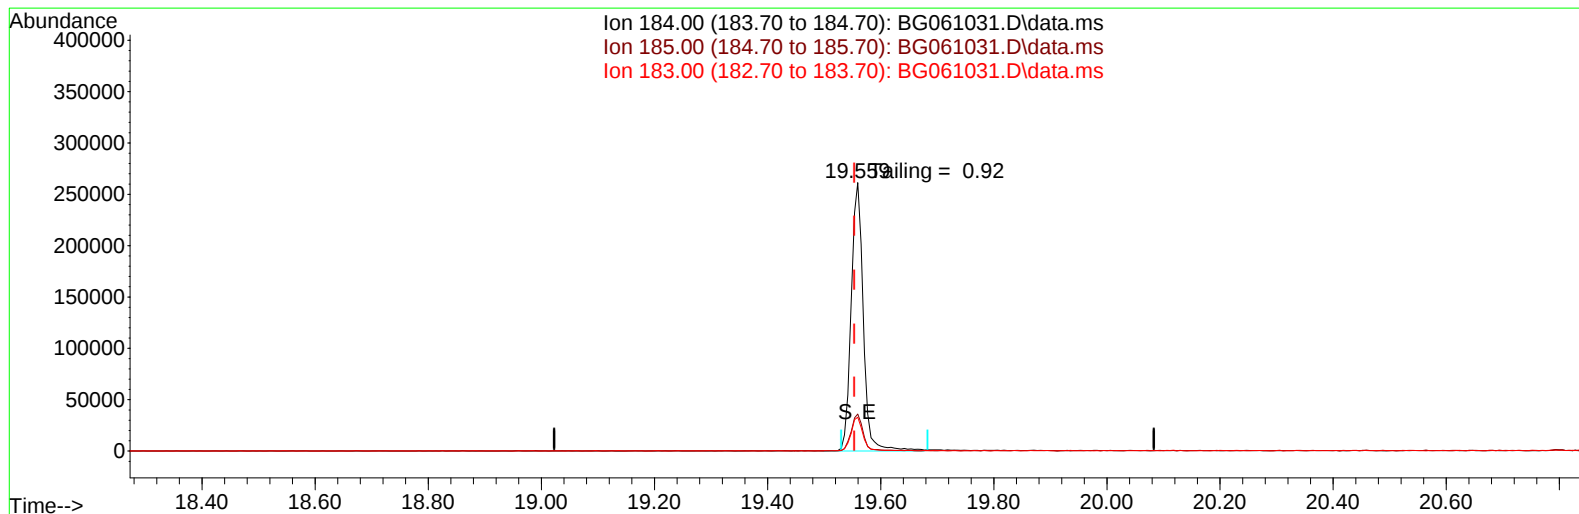

TIC: BG061031.D\data.ms

(77) Benzidine

19.559min (+ 0.006) 35628.01 ng

response 380245

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.79
183.00	12.70	12.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/25/2024	BNA_G	<u>BG061031.D</u>
Compound Name	Response	Retention Time
DDT	257328	20.799
DDD	15140	20.353
DDE	2242	19.853
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17382	274710	6.33

Instrument :
BNA_G
ClientSampleId :
DFTPP