


Data Path : Z:\HPCHEM1\BNA G\Data\BG042618\
 Data File : BG034015.D
 Acq On : 26 Apr 2018 17:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG041918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 19 13:56:22 2018

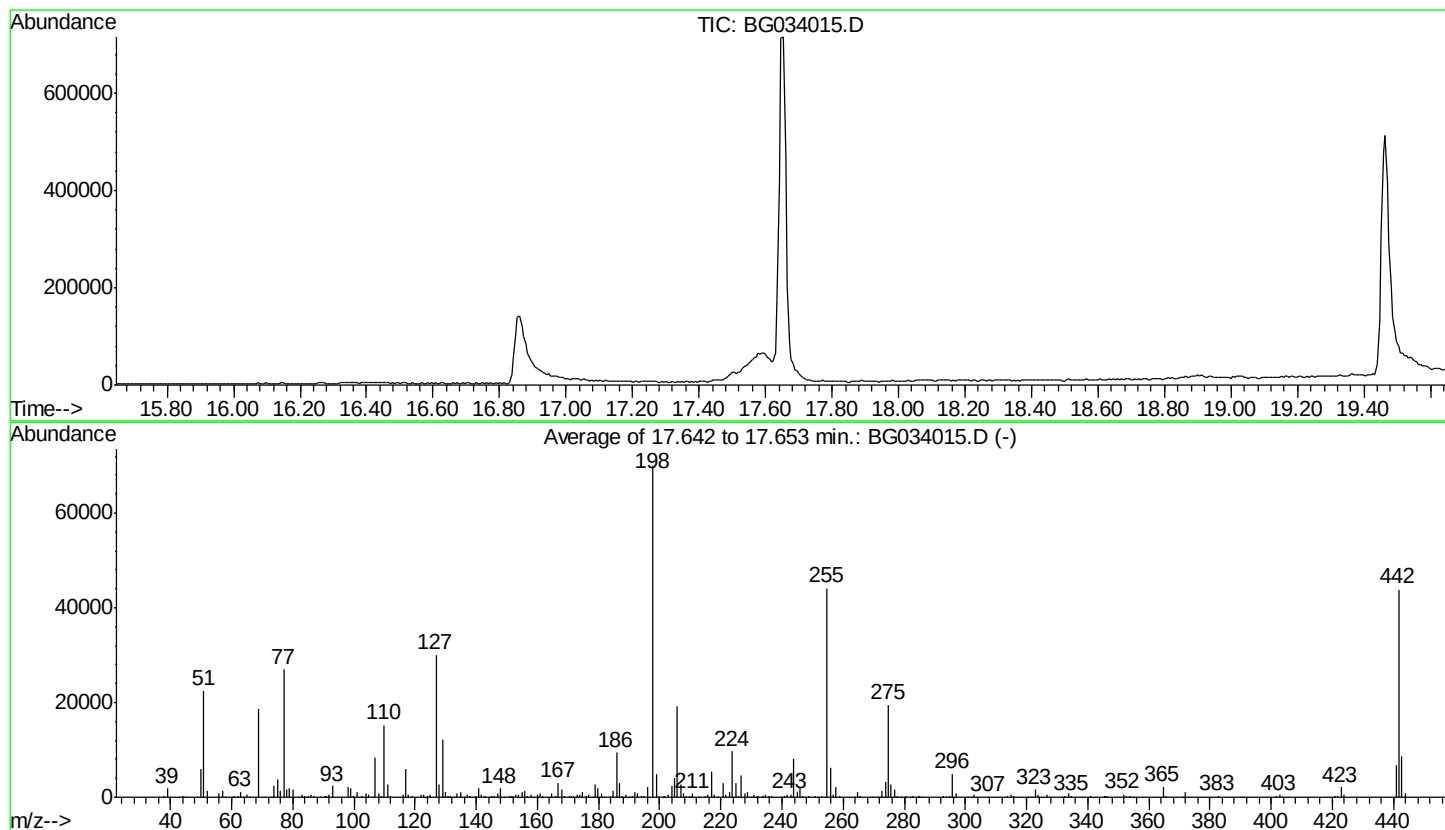

AutoFind: Scans 2443, 2444, 2445; Background Corrected with Scan 2437

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.1	22497	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.8	18754	PASS
70	69	0.00	2	0.4	70	PASS
127	198	10	80	43.0	30101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69989	PASS
199	198	5	9	6.9	4840	PASS
275	198	10	60	27.9	19544	PASS
365	198	1	100	3.2	2258	PASS
441	443	0.01	100	79.5	6819	PASS
442	198	50	100	62.7	43866	PASS
443	442	15	24	19.6	8577	PASS