


Data Path : Z:\HPCHEM1\BNA G\Data\BG042618\  
 Data File : BG034034.D  
 Acq On : 27 Apr 2018 6:16  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG041918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Apr 19 13:56:22 2018

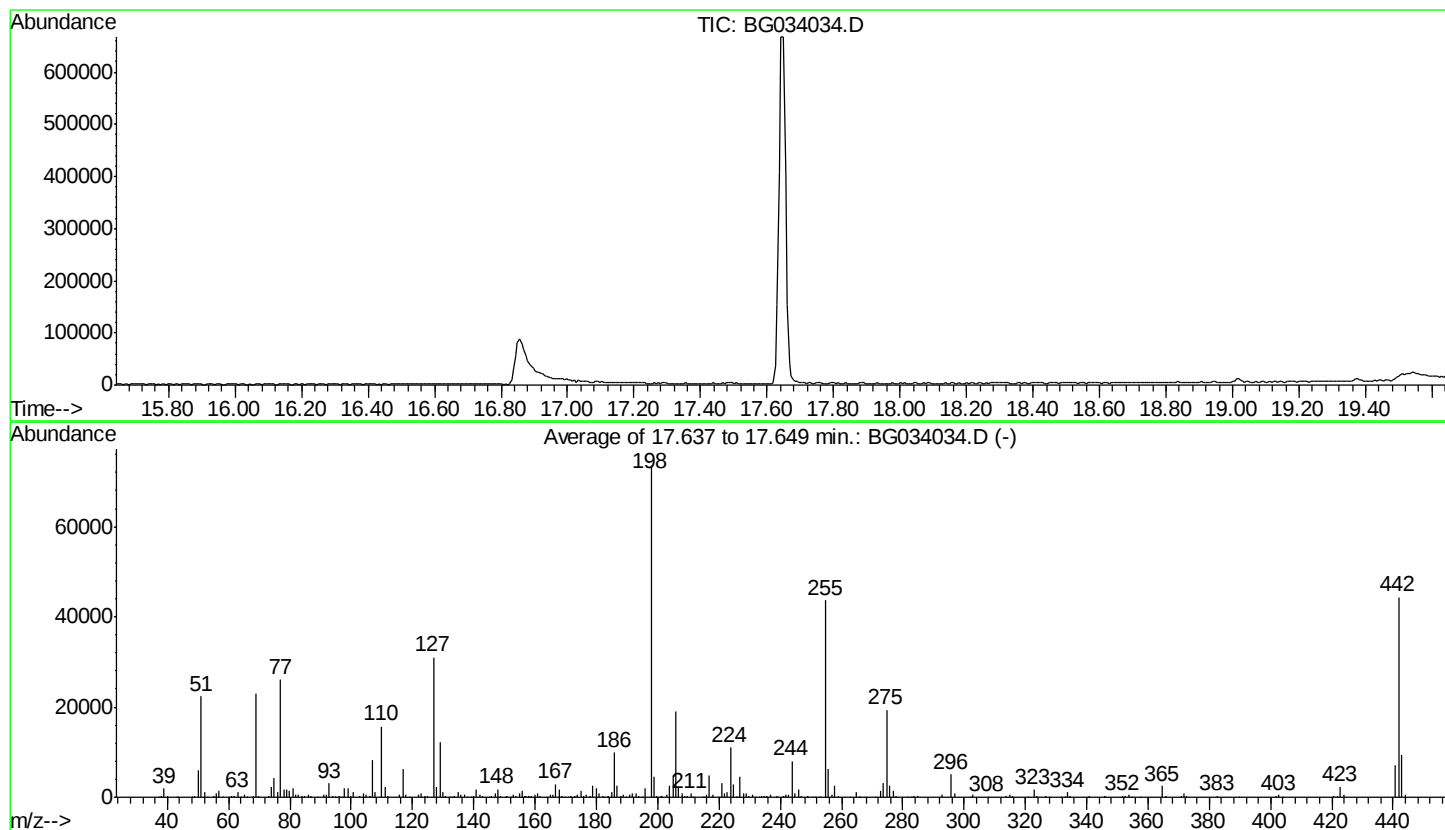

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2436

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 30.4      | 22384   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.9       | 216     | PASS             |
| 69          | 198          | 0.00         | 100          | 31.3      | 23022   | PASS             |
| 70          | 69           | 0.00         | 2            | 1.0       | 221     | PASS             |
| 127         | 198          | 10           | 80           | 42.2      | 31048   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 73522   | PASS             |
| 199         | 198          | 5            | 9            | 6.2       | 4568    | PASS             |
| 275         | 198          | 10           | 60           | 26.3      | 19347   | PASS             |
| 365         | 198          | 1            | 100          | 3.3       | 2454    | PASS             |
| 441         | 443          | 0.01         | 100          | 73.8      | 6980    | PASS             |
| 442         | 198          | 50           | 100          | 60.2      | 44280   | PASS             |
| 443         | 442          | 15           | 24           | 21.4      | 9457    | PASS             |