

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042619\
 Data File : BG040644.D
 Acq On : 27 Apr 2019 1:40
 Operator : JU/SJ
 Sample : K2198-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OK-01-042519

Quant Time: Apr 27 04:41:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	49913	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	191190	20.00	ng	0.00
39) Acenaphthene-d10	14.79	164	137025	20.00	ng	0.00
64) Phenanthrene-d10	17.53	188	390191	20.00	ng	0.00
76) Chrysene-d12	21.82	240	406753	20.00	ng	0.00
87) Perylene-d12	25.20	264	422085	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	360842	127.44	ng	0.00
7) Phenol-d6	7.29	99	476967	109.40	ng	0.00
23) Nitrobenzene-d5	9.33	82	430911	104.14	ng	0.00
42) 2,4,6-Tribromophenol	16.27	330	300417	159.50	ng	0.00
45) 2-Fluorobiphenyl	13.41	172	870121	91.71	ng	0.00
79) Terphenyl-d14	20.13	244	1871089	101.91	ng	0.00
Target Compounds						
9) Benzaldehyde	7.28	77	626	Below Cal		Qvalue # 6
19) n-Nitroso-di-n-propylamine	9.33	70	63750	16.244	ng	# 84
51) 2,6-Dinitrotoluene	14.79	165	18506	8.271	ng	# 15
54) 2,4-Dinitrophenol	14.84	184	65	7.062	ng	# 21
57) 2,4-Dinitrotoluene	14.79	165	18506	6.087	ng	# 17
65) 4,6-Dinitro-2-methylphenol	16.02	198	58	7.127	ng	# 28
67) 4-Bromophenyl-phenylether	16.27	248	23250	4.783	ng	# 1
77) Benzydine	20.13	184	36546	3.281	ng	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG042619\
Data File : BG040644.D
Acq On : 27 Apr 2019 1:40
Operator : JU/SJ
Sample : K2198-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OK-01-042519

Quant Time: Apr 27 04:41:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

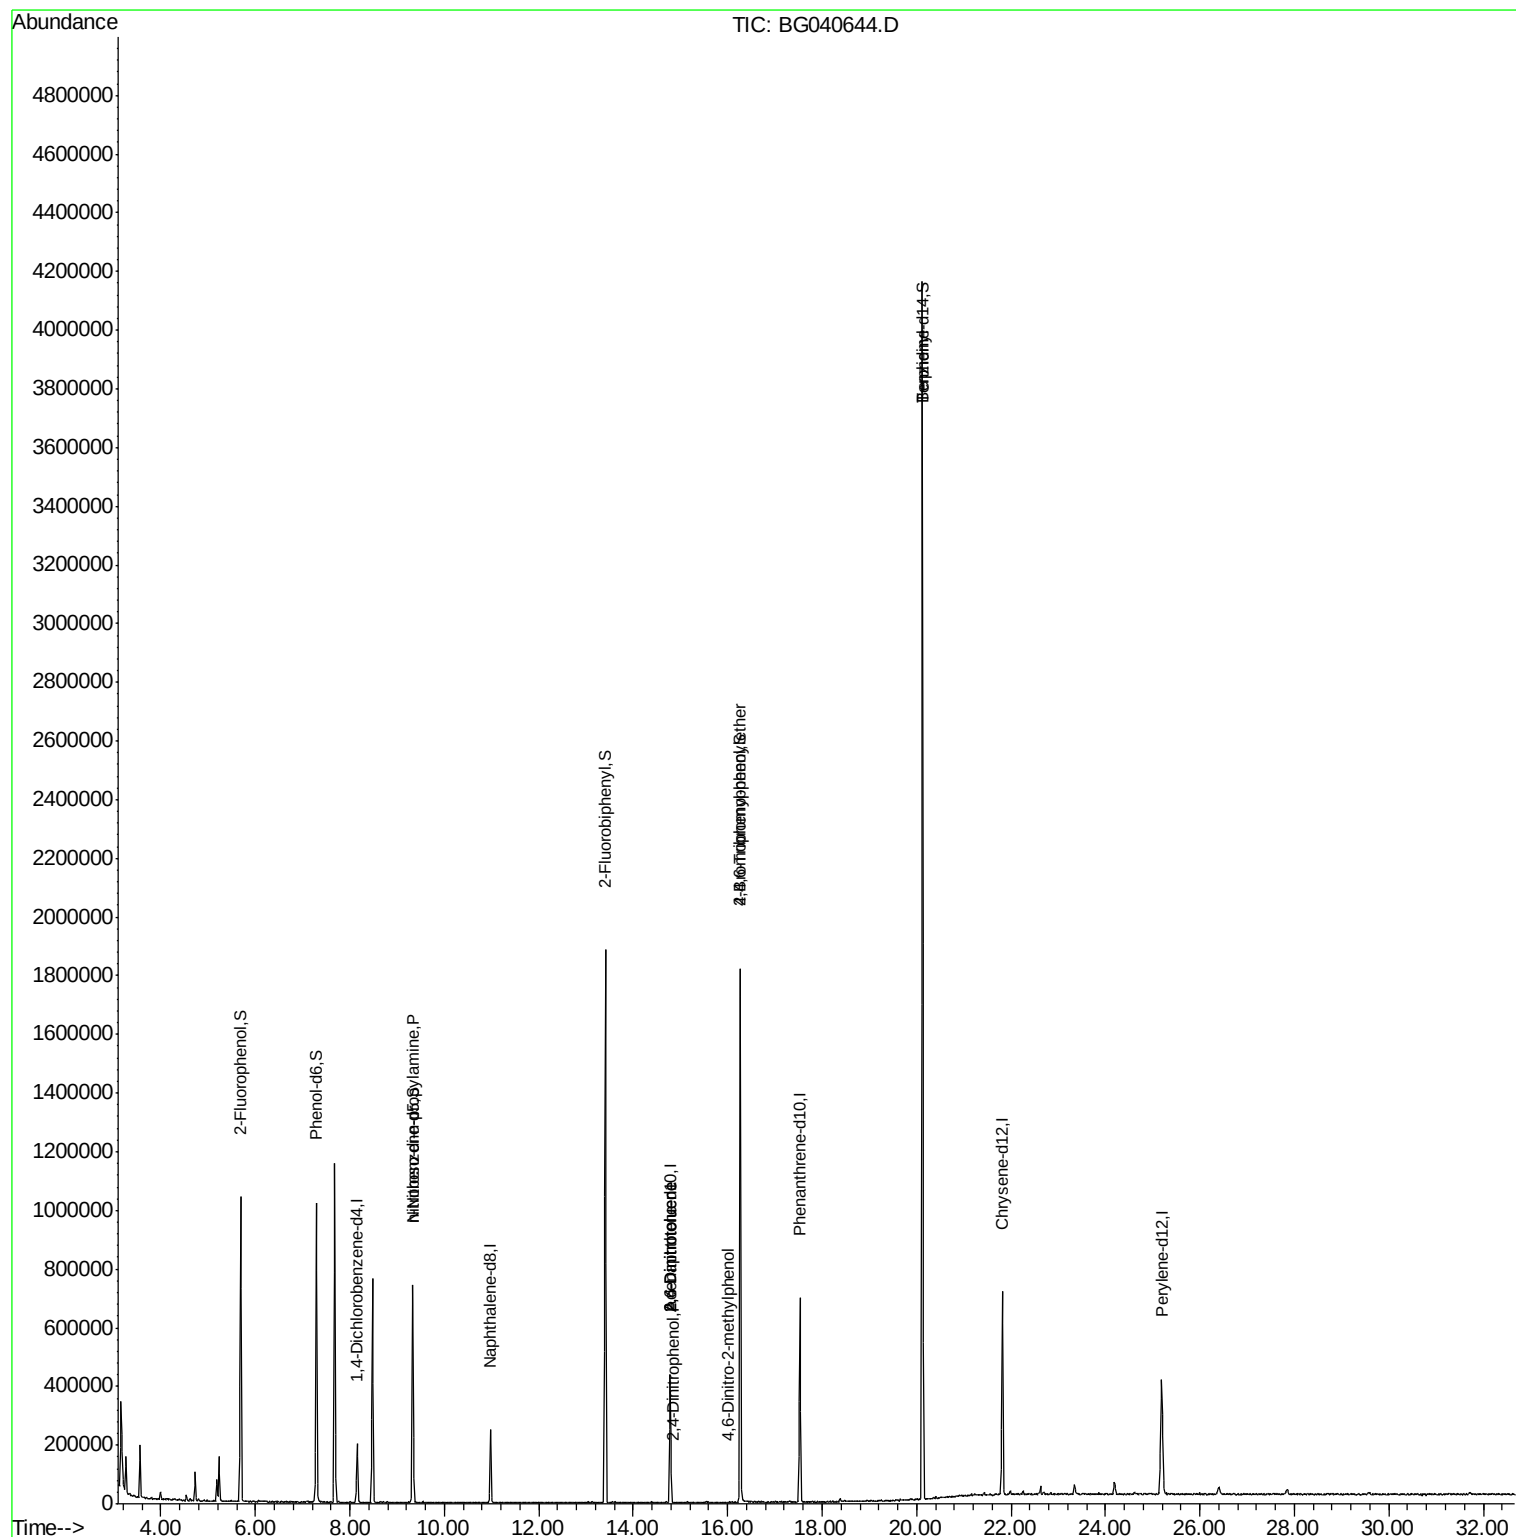




#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.16 min Scan# 863
 Delta R.T. -0.00 min
 Lab File: BG040644.D
 Acq: 27 Apr 2019 1:40

Instrument :
 BNA_G
 ClientSampleId :
 OK-01-042519

Tot Ion	Ratio	Lower	Upper
152	100		
150	135.9	120.2	180.2
115	60.5	46.2	69.2

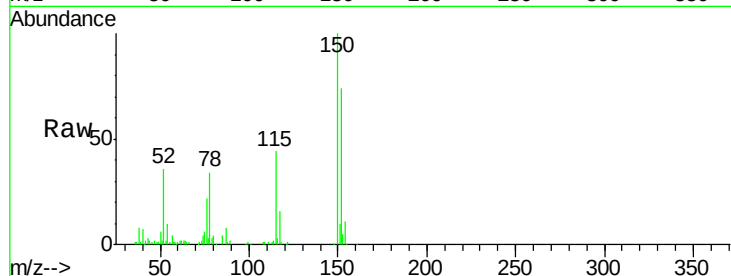


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

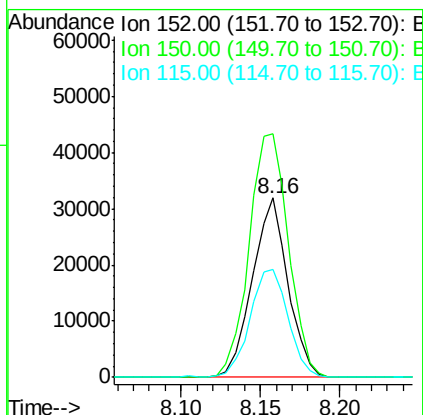



#5


2-Fluorophenol
 Concen: 127.438 ng
 RT: 5.69 min Scan# 443
 Delta R.T. 0.01 min
 Lab File: BG040644.D
 Acq: 27 Apr 2019 1:40

Tgt Ion	Ratio	Lower	Upper
112	100		
64	77.6	61.4	92.0
63	44.3	37.8	56.6



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

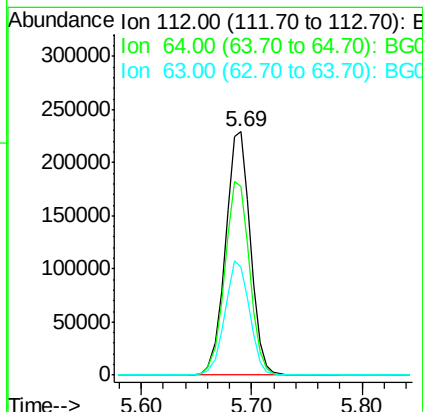



#7

Phenol-d6

Concen: 109.403 ng

RT: 7.29 min Scan# 716

Delta R.T. -0.00 min

Lab File: BG040644.D

Acq: 27 Apr 2019 1:40

Instrument :

BNA_G

ClientSampleId :

OK-01-042519





Tot Ion: 99 Resp: 476967

Ion Ratio Lower Upper

99 100

42 27.4 21.8 32.8

71 47.6 38.6 57.8

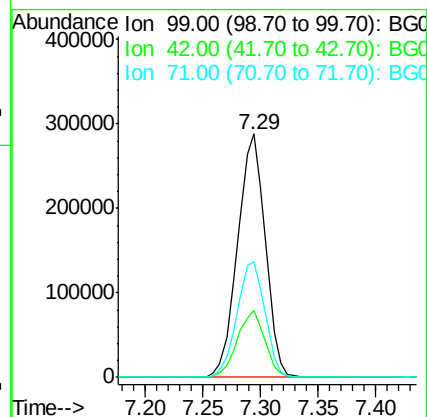

#19

n-Nitroso-di-n-propylamine

Concen: 16.244 ng

RT: 9.33 min Scan# 1063

Delta R.T. 0.36 min

Lab File: BG040644.D

Acq: 27 Apr 2019 1:40

Tgt Ion: 70 Resp: 63750




Ion Ratio Lower Upper


70 100

42 63.5 57.1 85.7

101 0.0 7.8 11.8#

130 1.5 14.6 21.8#

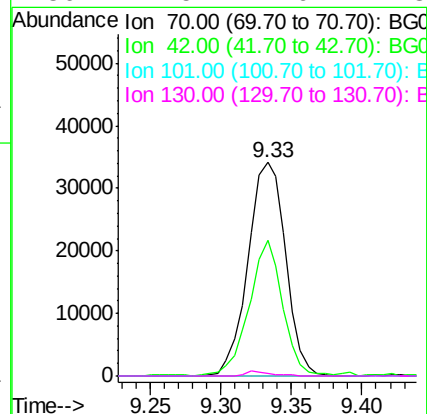







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.98 min Scan# 1344
Delta R.T. -0.00 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40

Instrument :
BNA_G
ClientSampleId :
OK-01-042519

Tot Ion:136	Resp:	191190
Ion Ratio	Lower	Upper
136 100		
137 12.3	9.7	14.5
54 10.1	8.6	12.8
68 6.5	4.8	7.2

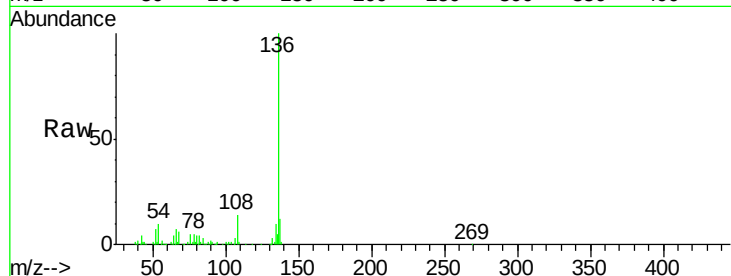


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


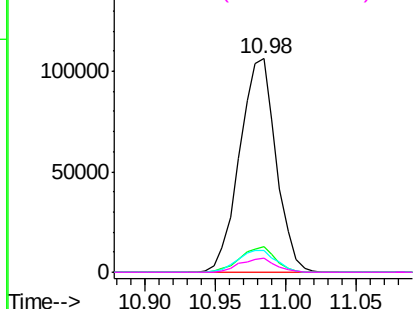



#23
Nitrobenzene-d5
Concen: 104.141 ng
RT: 9.33 min Scan# 1063
Delta R.T. -0.01 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40

Tgt Ion: 82	Resp: 430911
Ion Ratio	Lower Upper
82 100	
128 34.4	28.9 43.3
54 58.6	47.2 70.8

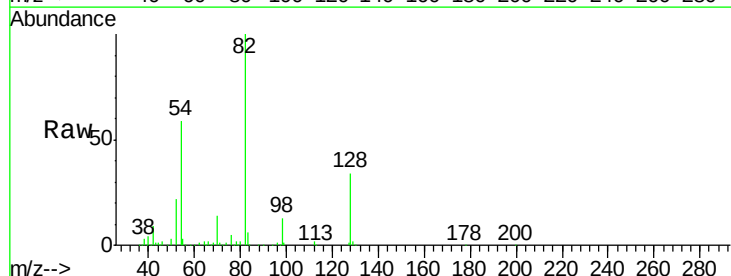

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

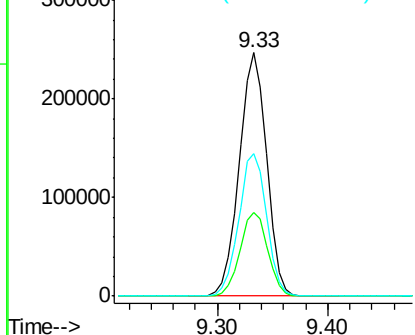


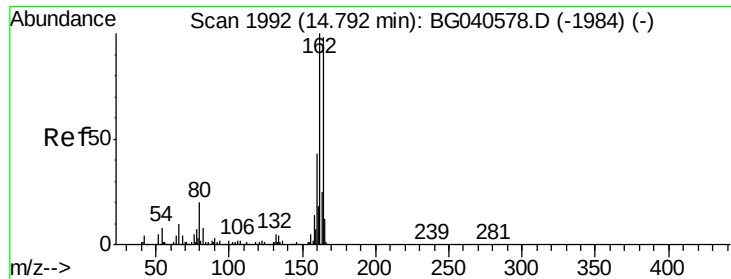




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.79 min Scan# 1991
Delta R.T. -0.01 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40

Instrument :
BNA_G
ClientSampleId :
OK-01-042519

Tot Ion:164 Resp: 137025
Ion Ratio Lower Upper
164 100
162 104.3 81.9 122.9
160 48.2 35.4 53.2




Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

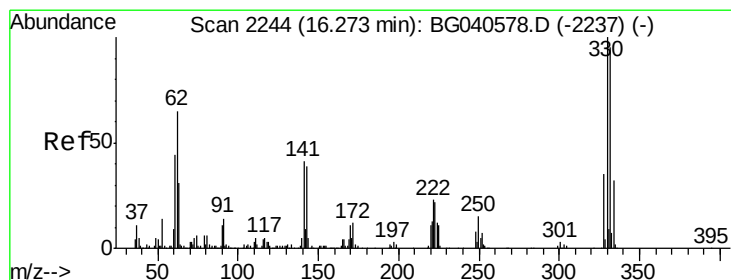
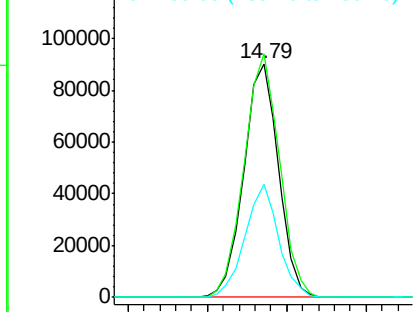



#42
2,4,6-Tribromophenol
Concen: 159.504 ng
RT: 16.27 min Scan# 2244
Delta R.T. -0.00 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40

Tgt Ion:330 Resp: 300417
Ion Ratio Lower Upper
330 100
332 96.6 75.9 113.9
141 40.5 32.4 48.6



Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E




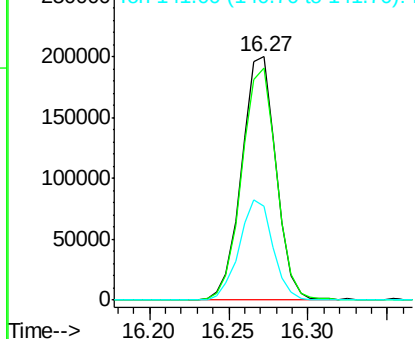




#45
2-Fluorobiphenyl
Concen: 91.708 ng
RT: 13.41 min Scan# 1757
Delta R.T. -0.01 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40




Instrument :
BNA_G
ClientSampleId :
OK-01-042519


Tot Ion	Ratio	Lower	Upper
172	100		
171	37.6	29.4	44.2
170	25.3	19.9	29.9

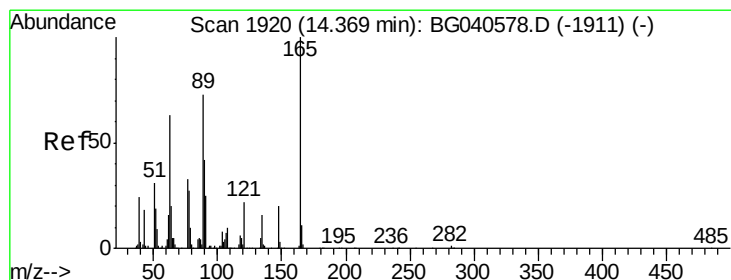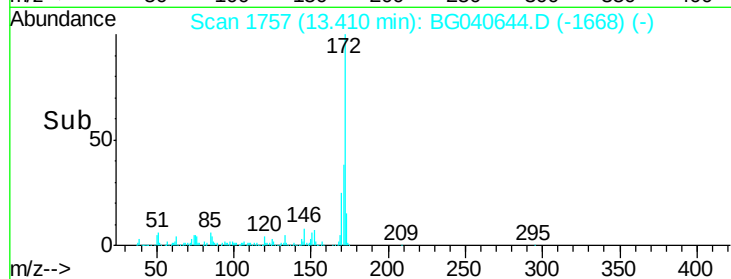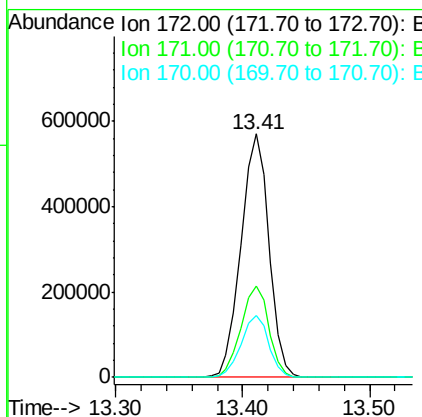

#51
2,6-Dinitrotoluene
Concen: 8.271 ng
RT: 14.79 min Scan# 1991
Delta R.T. 0.42 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40

Tgt Ion	Ratio	Lower	Upper
165	100		
63	2.3	61.0	91.4#
89	2.4	58.6	87.8#


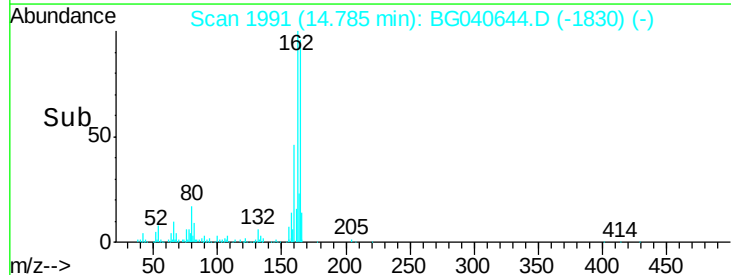
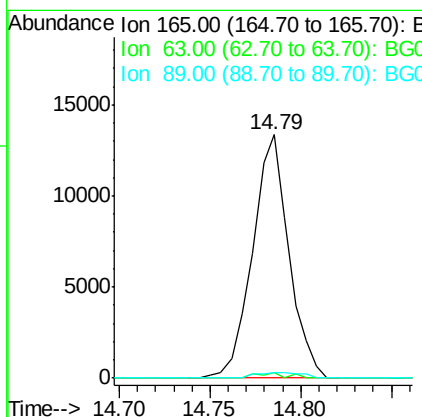



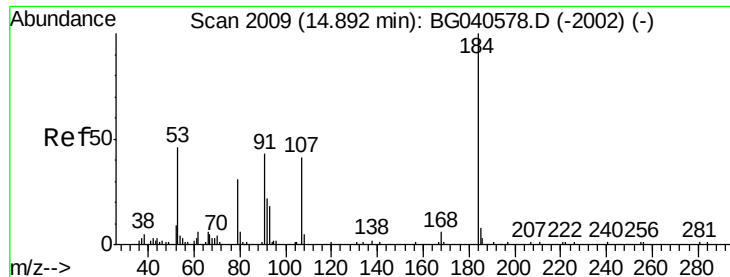

#54
2,4-Dinitrophenol
Concen: 7.062 ng
RT: 14.84 min Scan# 2001
Delta R.T. -0.05 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40




Instrument :
BNA_G
ClientSampleId :
OK-01-042519


Tot Ion:184 Resp: 65
Ion Ratio Lower Upper
184 100
63 0.0 51.8 77.6#
154 0.0 43.6 65.4#

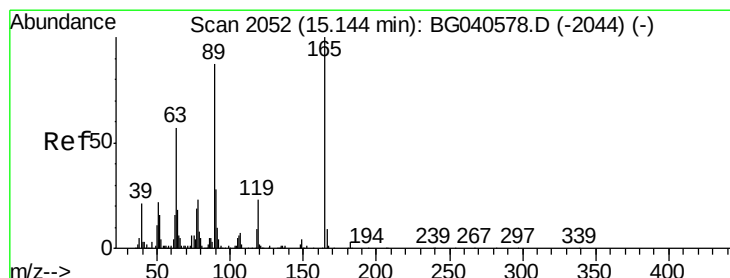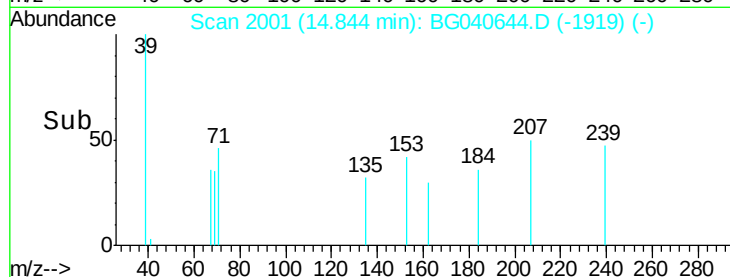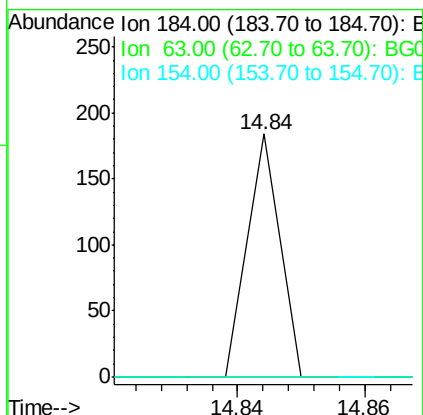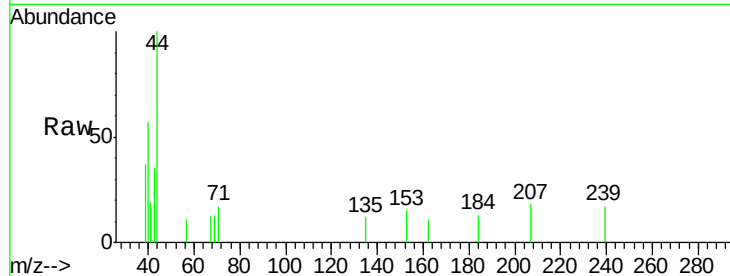

#57
2,4-Dinitrotoluene
Concen: 6.087 ng
RT: 14.79 min Scan# 1991
Delta R.T. -0.36 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40

Tgt Ion:165 Resp: 18506
Ion Ratio Lower Upper
165 100
63 2.3 45.8 68.8#
89 2.4 69.4 104.2#
182 0.0 2.2 3.4#


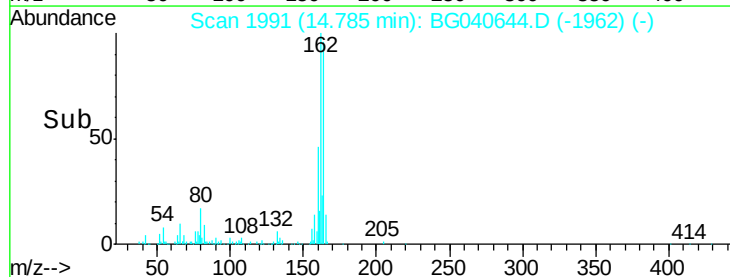
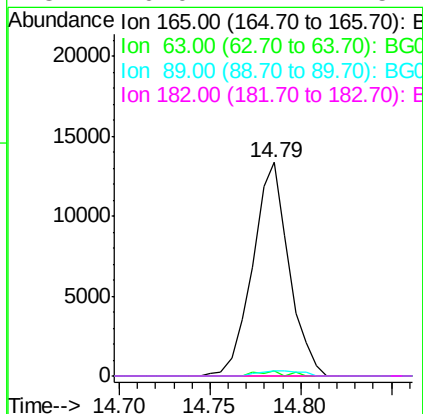
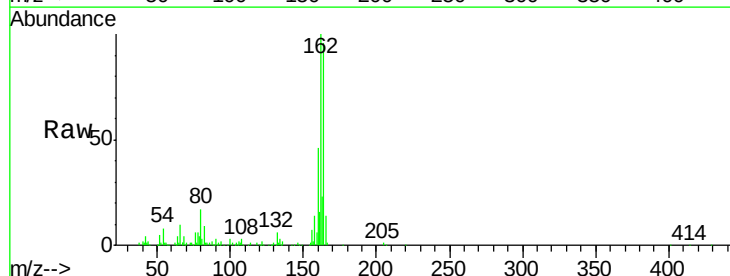


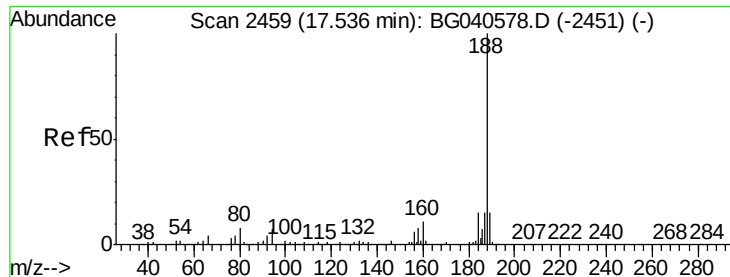

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.53 min Scan# 2458
Delta R.T. -0.01 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40




Instrument :
BNA_G
ClientSampleId :
OK-01-042519


Tot Ion	Ratio	Lower	Upper
188	100		
94	6.3	5.6	8.4
80	8.2	6.4	9.6

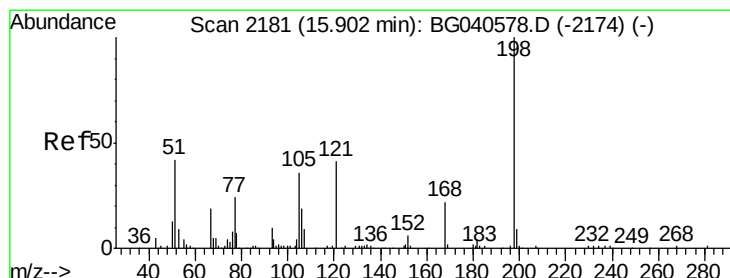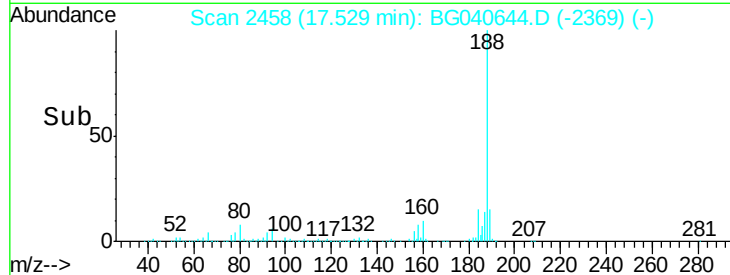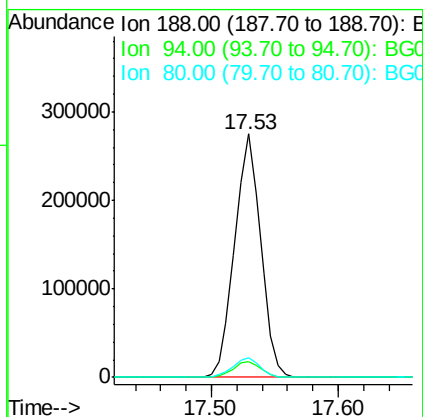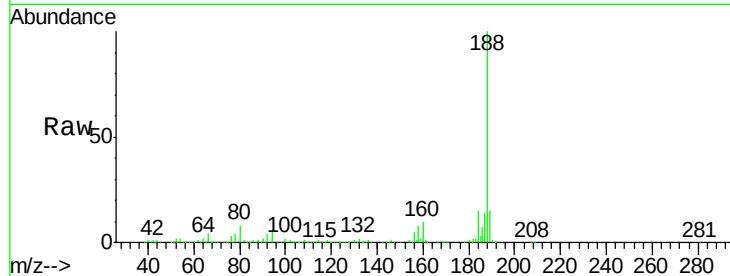

#65
4,6-Dinitro-2-methylphenol
Concen: 7.127 ng
RT: 16.02 min Scan# 2201
Delta R.T. 0.12 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40

Tgt Ion	Ratio	Lower	Upper
198	100		
51	0.0	35.9	75.9#
105	0.0	21.2	61.2#

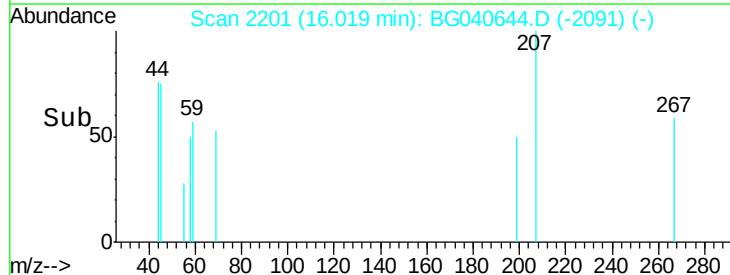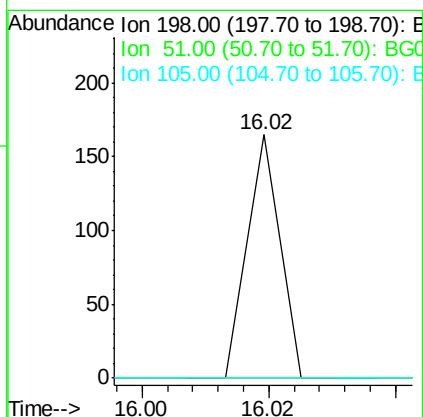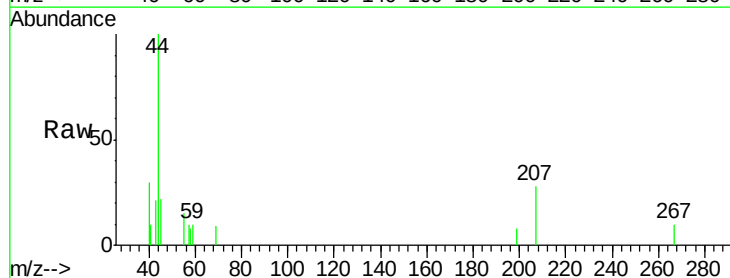


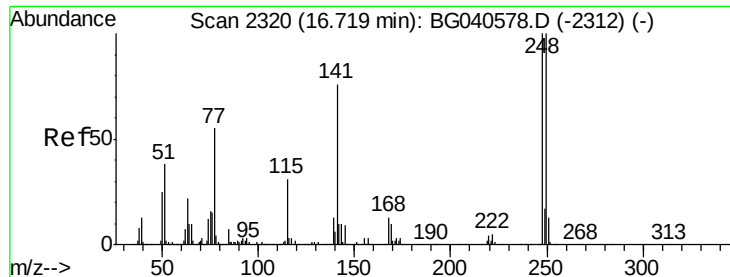




#67
 4-Bromophenyl-phenylether
 Concen: 4.783 ng
 RT: 16.27 min Scan# 2244
 Delta R.T. -0.45 min
 Lab File: BG040644.D
 Acq: 27 Apr 2019 1:40

Instrument :
 BNA_G
 ClientSampleId :
 OK-01-042519

Tot Ion:248 Resp: 23250
 Ion Ratio Lower Upper
 248 100
 250 173.1 79.8 119.6#
 141 489.7 60.8 91.2#

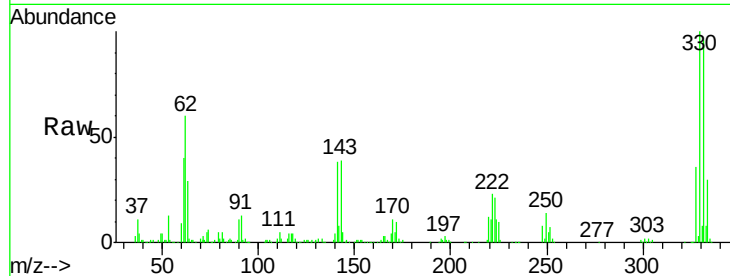


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

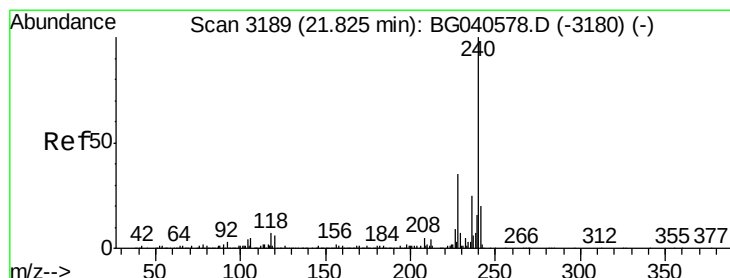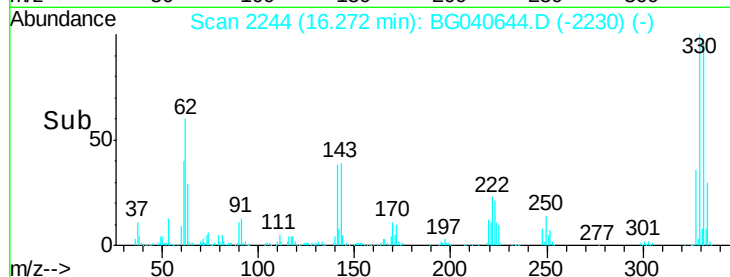
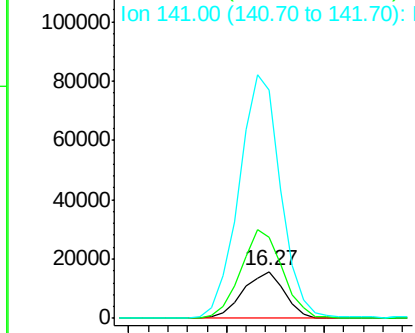



#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.82 min Scan# 3188
 Delta R.T. -0.01 min
 Lab File: BG040644.D
 Acq: 27 Apr 2019 1:40

Tgt Ion:240 Resp: 406753
 Ion Ratio Lower Upper
 240 100
 120 6.1 5.0 7.6
 236 25.6 20.3 30.5

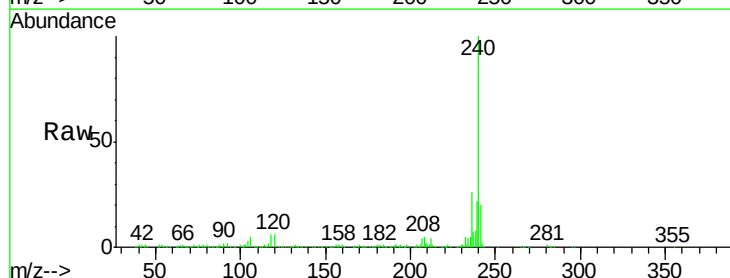

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

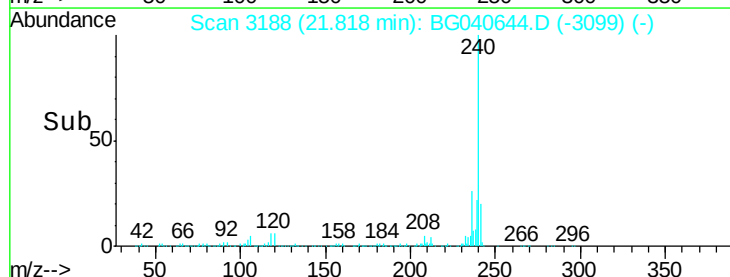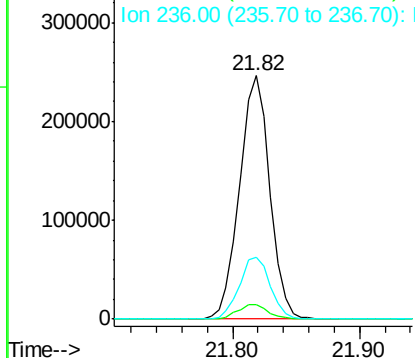

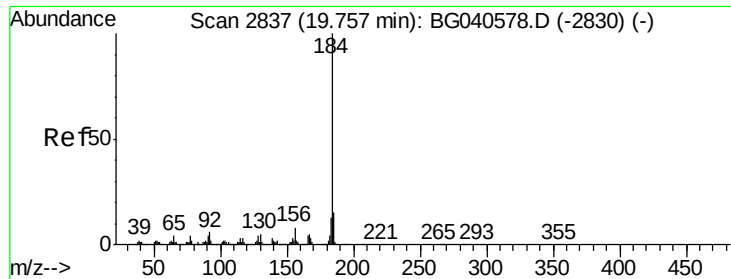

#77

Benzidine

Concen: 3.281 ng

RT: 20.13 min Scan# 2900

Delta R.T. 0.37 min

Lab File: BG040644.D

Acq: 27 Apr 2019 1:40

Instrument :

BNA_G

ClientSampleId :

OK-01-042519


Tot Ion:184 Resp: 36546

Ion Ratio Lower Upper

184 100

185 17.5 11.8 17.8




183 9.2 10.2 15.2#

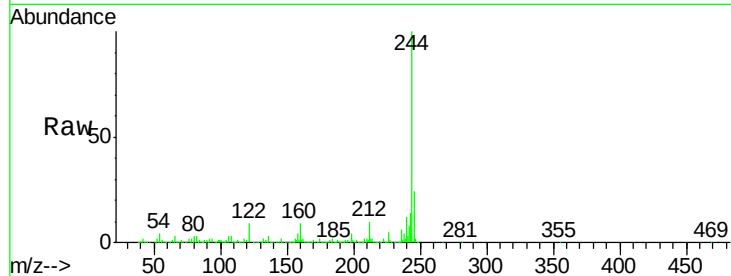

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

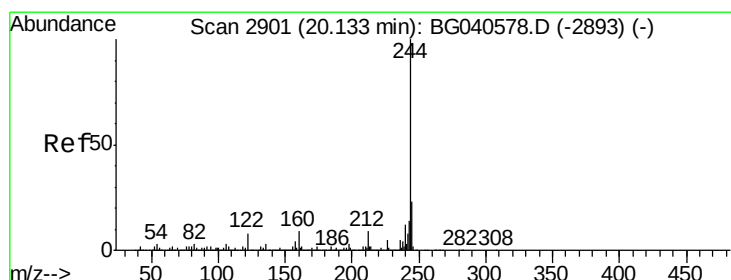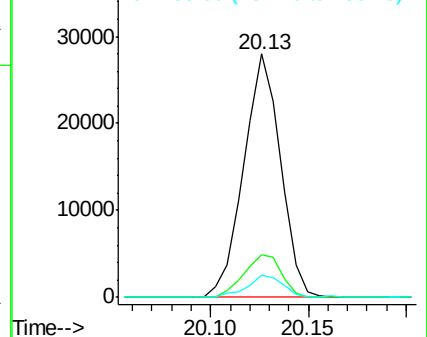

#79

Terphenyl-d14

Concen: 101.911 ng

RT: 20.13 min Scan# 2900

Delta R.T. -0.01 min

Lab File: BG040644.D

Acq: 27 Apr 2019 1:40


Tgt Ion:244 Resp: 1871089

Ion Ratio Lower Upper

244 100

212 9.7 7.2 10.8



122 8.7 6.6 10.0




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

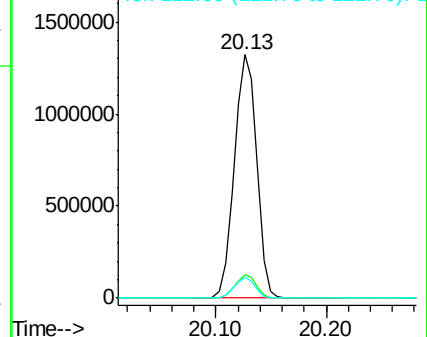

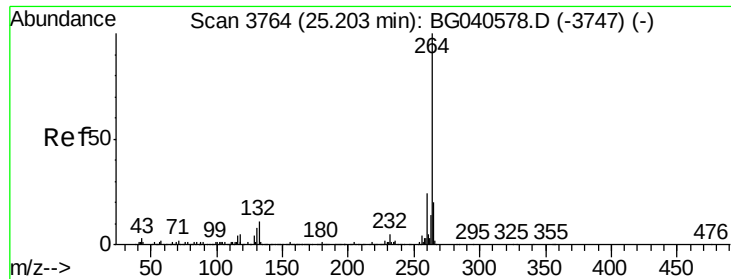

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.20 min Scan# 3763
Delta R.T. -0.01 min
Lab File: BG040644.D
Acq: 27 Apr 2019 1:40

Instrument :
BNA_G
ClientSampleId :
OK-01-042519

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.2	28.8
265	19.0	16.6	25.0

