
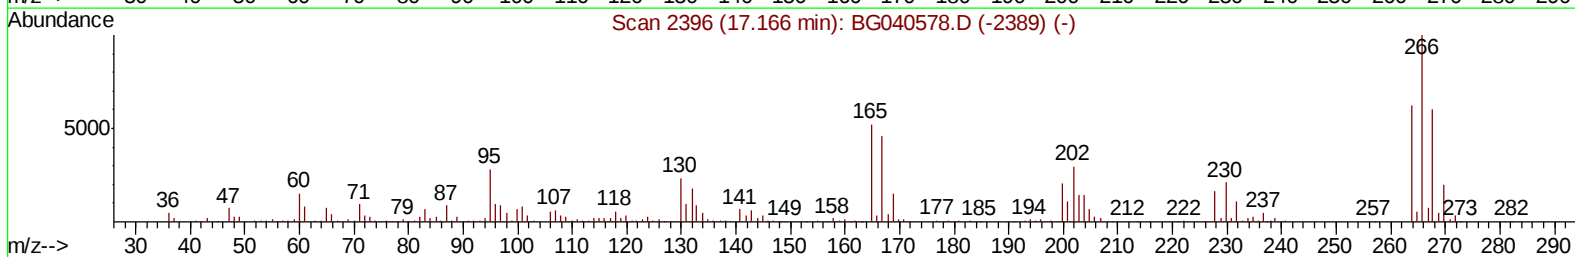
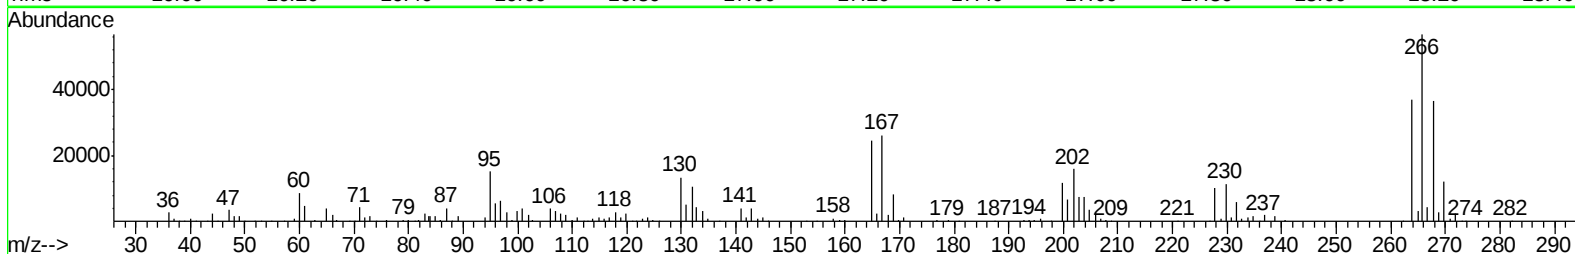


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042619\
Data File : BG040621.D
Acq On : 26 Apr 2019 9:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:52:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

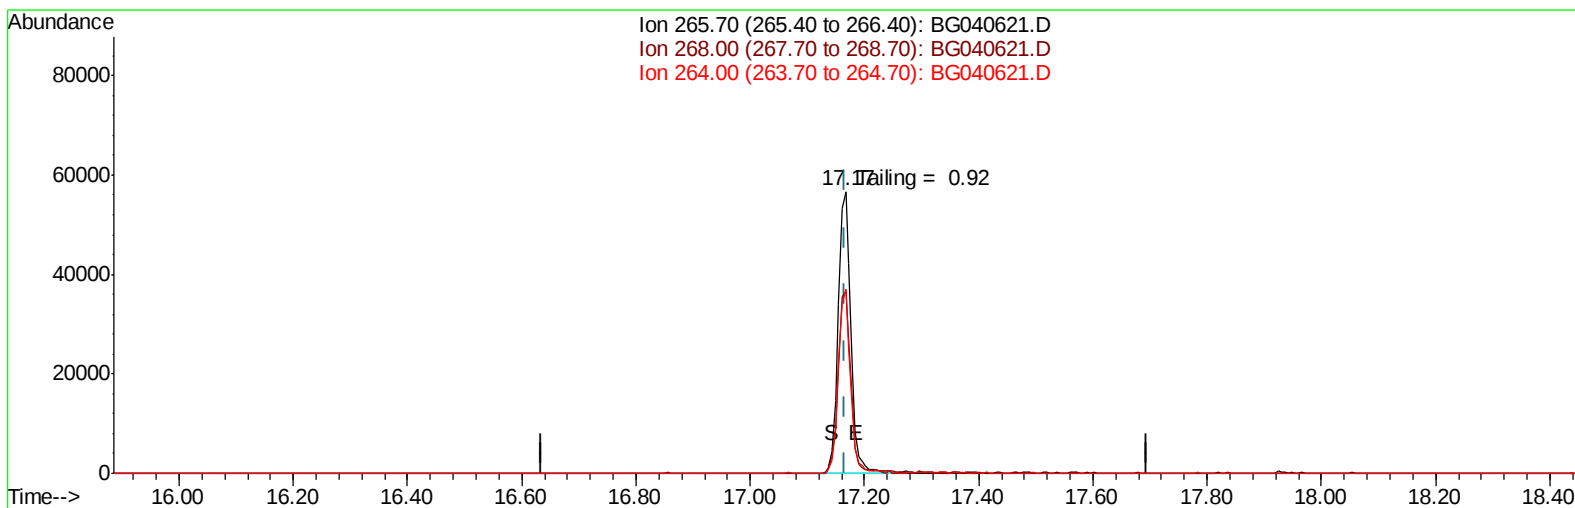

TIC: BG040621.D

(70) Pentachlorophenol (C)




17.167min (+0.001) 24747.16ng

response 87679

Ion	Exp%	Act%
265.70	100	100
268.00	65.40	70.04
264.00	62.50	65.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042619\
Data File : BG040621.D
Acq On : 26 Apr 2019 9:55
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:52:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

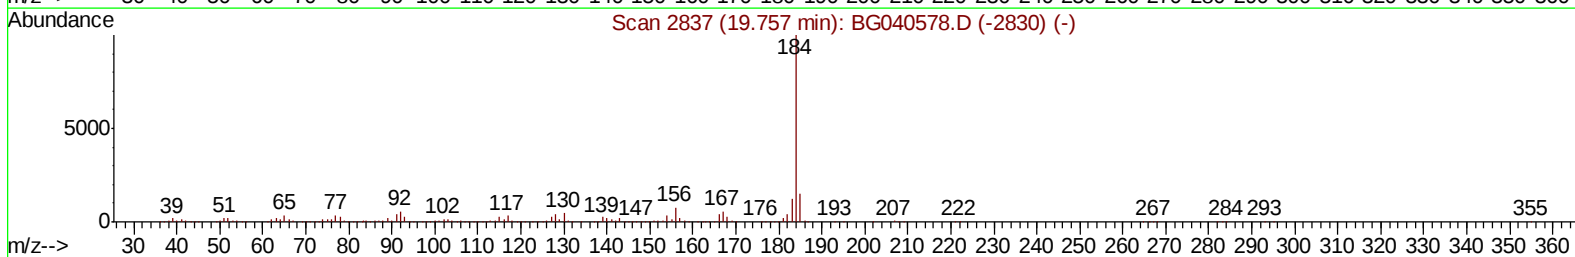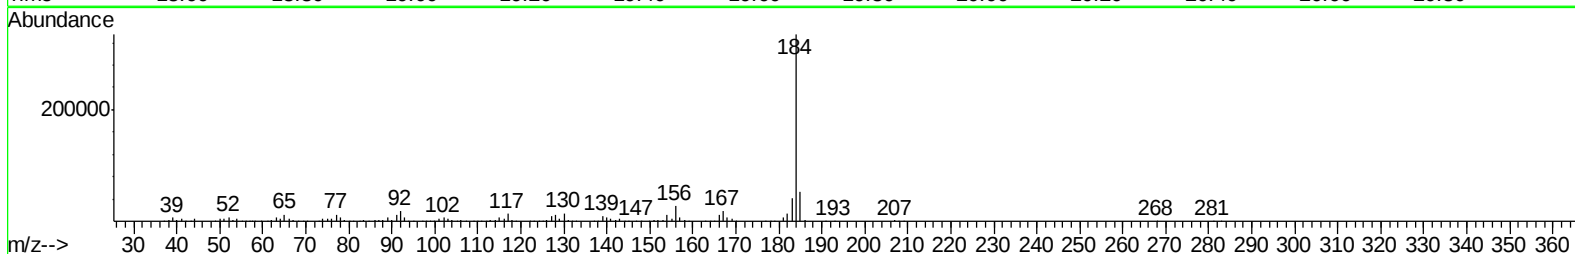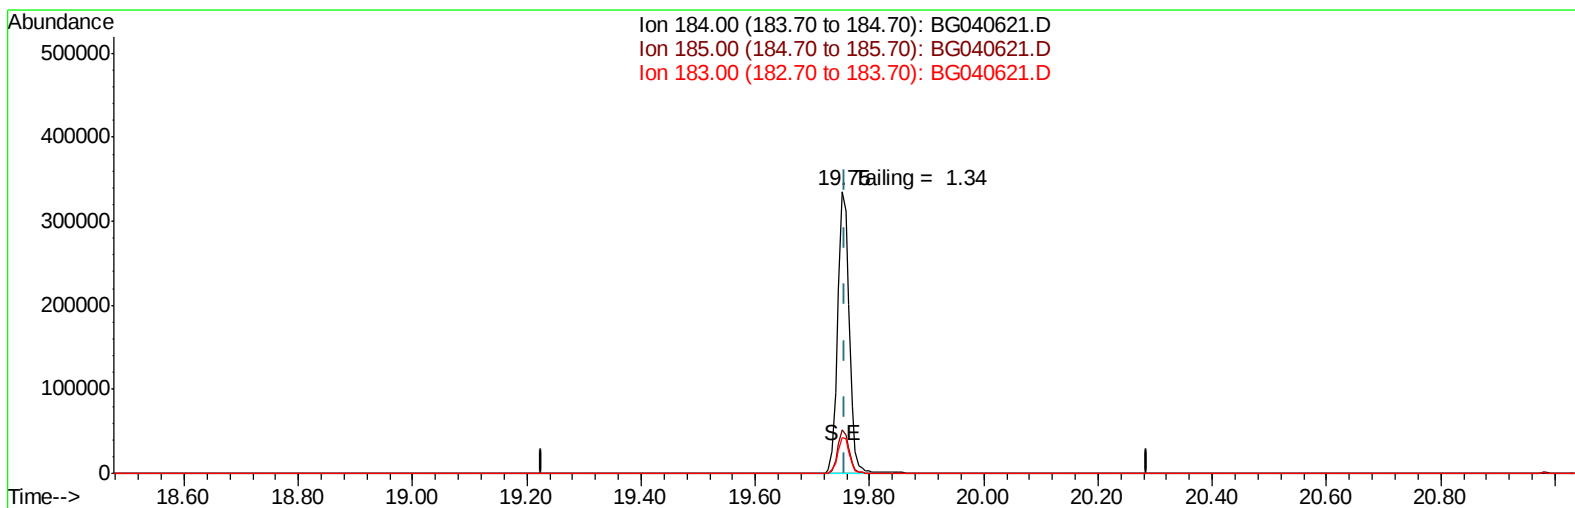

TIC: BG040621.D

(77) Benzidine

19.752min (-0.005) 252361.46ng

response 469865

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.58
183.00	12.70	12.54
0.00	0.00	0.00