
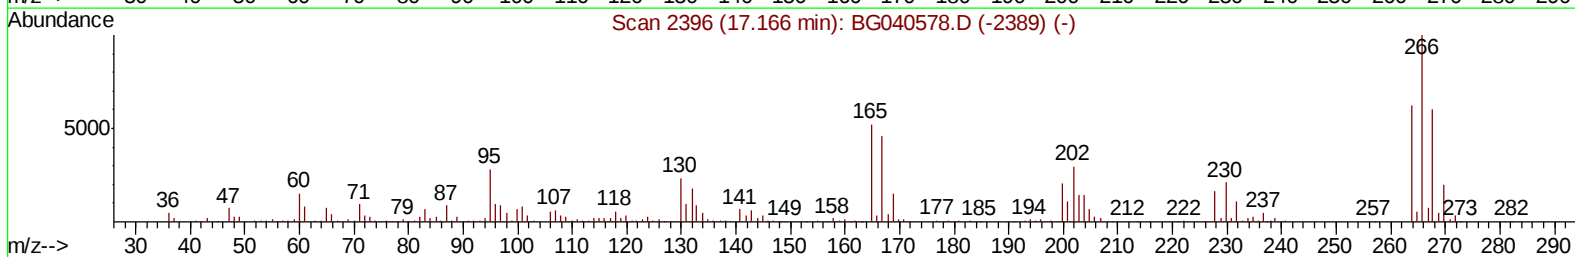
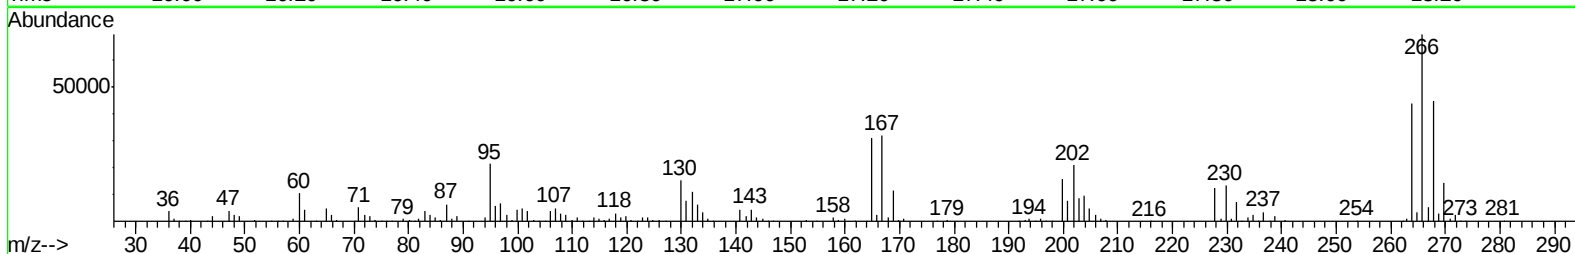


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042619\
Data File : BG040639.D
Acq On : 26 Apr 2019 22:30
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:54:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

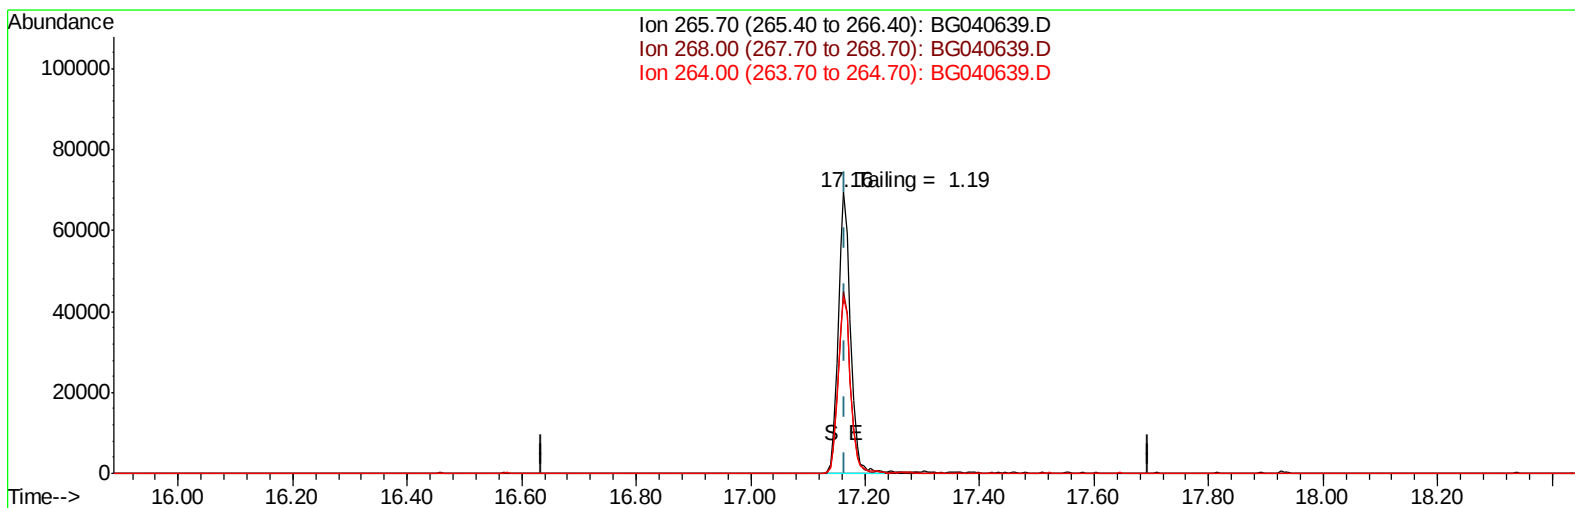

TIC: BG040639.D

(70) Pentachlorophenol (C)




17.163min (-0.003) 26088.47ng

response 104231

Ion	Exp%	Act%
265.70	100	100
268.00	65.40	68.84
264.00	62.50	68.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG042619\
 Data File : BG040639.D
 Acq On : 26 Apr 2019 22:30
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:54:18 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

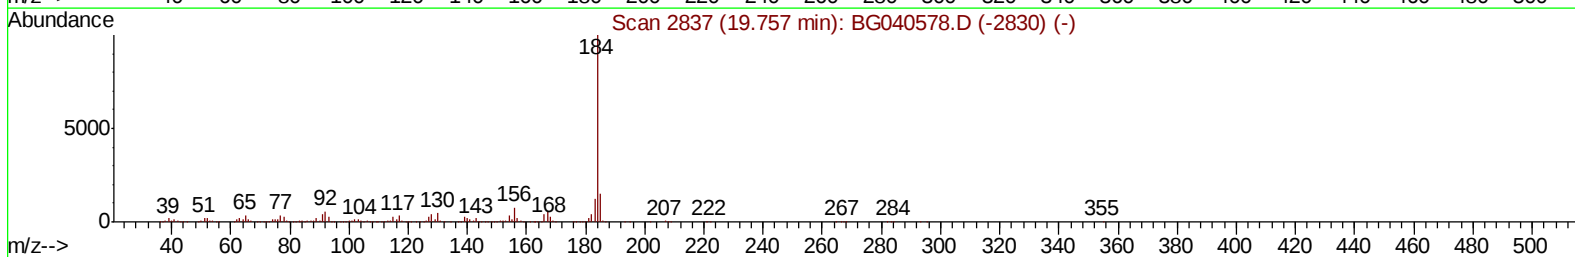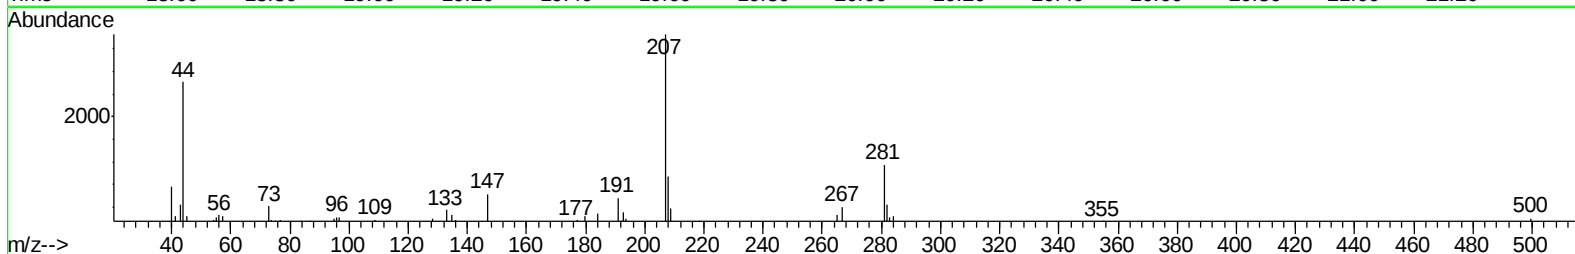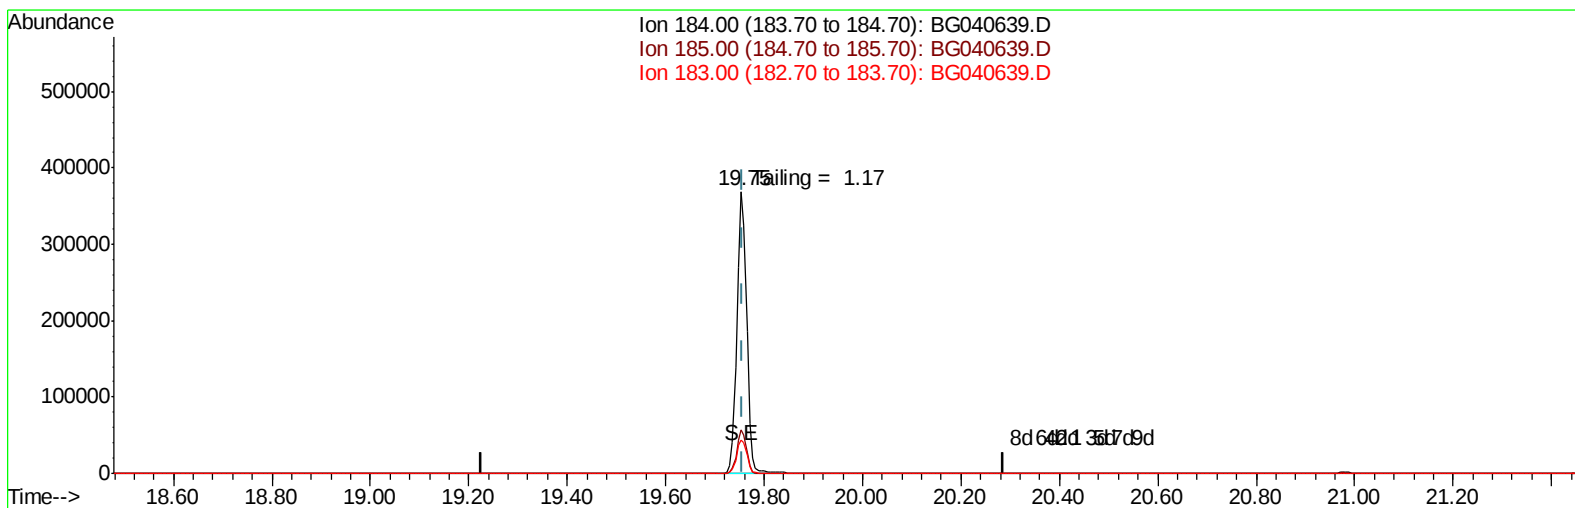

TIC: BG040639.D

(77) Benzidine

20.435min (+0.678) 79.55ng

response 159

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	0.00#
183.00	12.70	0.00#
0.00	0.00	0.00