

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042619\
 Data File : BG040635.D
 Acq On : 26 Apr 2019 18:44
 Operator : JU/SJ
 Sample : K2566-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 S37-0014

Quant Time: Apr 27 04:06:24 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	55018	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	237581	20.00	ng	0.00
39) Acenaphthene-d10	14.78	164	174384	20.00	ng	0.00
64) Phenanthrene-d10	17.53	188	454250	20.00	ng	0.00
76) Chrysene-d12	21.82	240	456928	20.00	ng	0.00
87) Perylene-d12	25.21	264	482949	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	144134	46.18	ng	0.00
7) Phenol-d6	7.29	99	135819	28.26	ng	0.00
23) Nitrobenzene-d5	9.34	82	393447	76.52	ng	0.00
42) 2,4,6-Tribromophenol	16.27	330	276637	115.41	ng	0.00
45) 2-Fluorobiphenyl	13.41	172	857846	71.04	ng	0.00
79) Terphenyl-d14	20.13	244	1590215	77.10	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042619\
Data File : BG040635.D
Acq On : 26 Apr 2019 18:44
Operator : JU/SJ
Sample : K2566-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
S37-0014

Quant Time: Apr 27 04:06:24 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

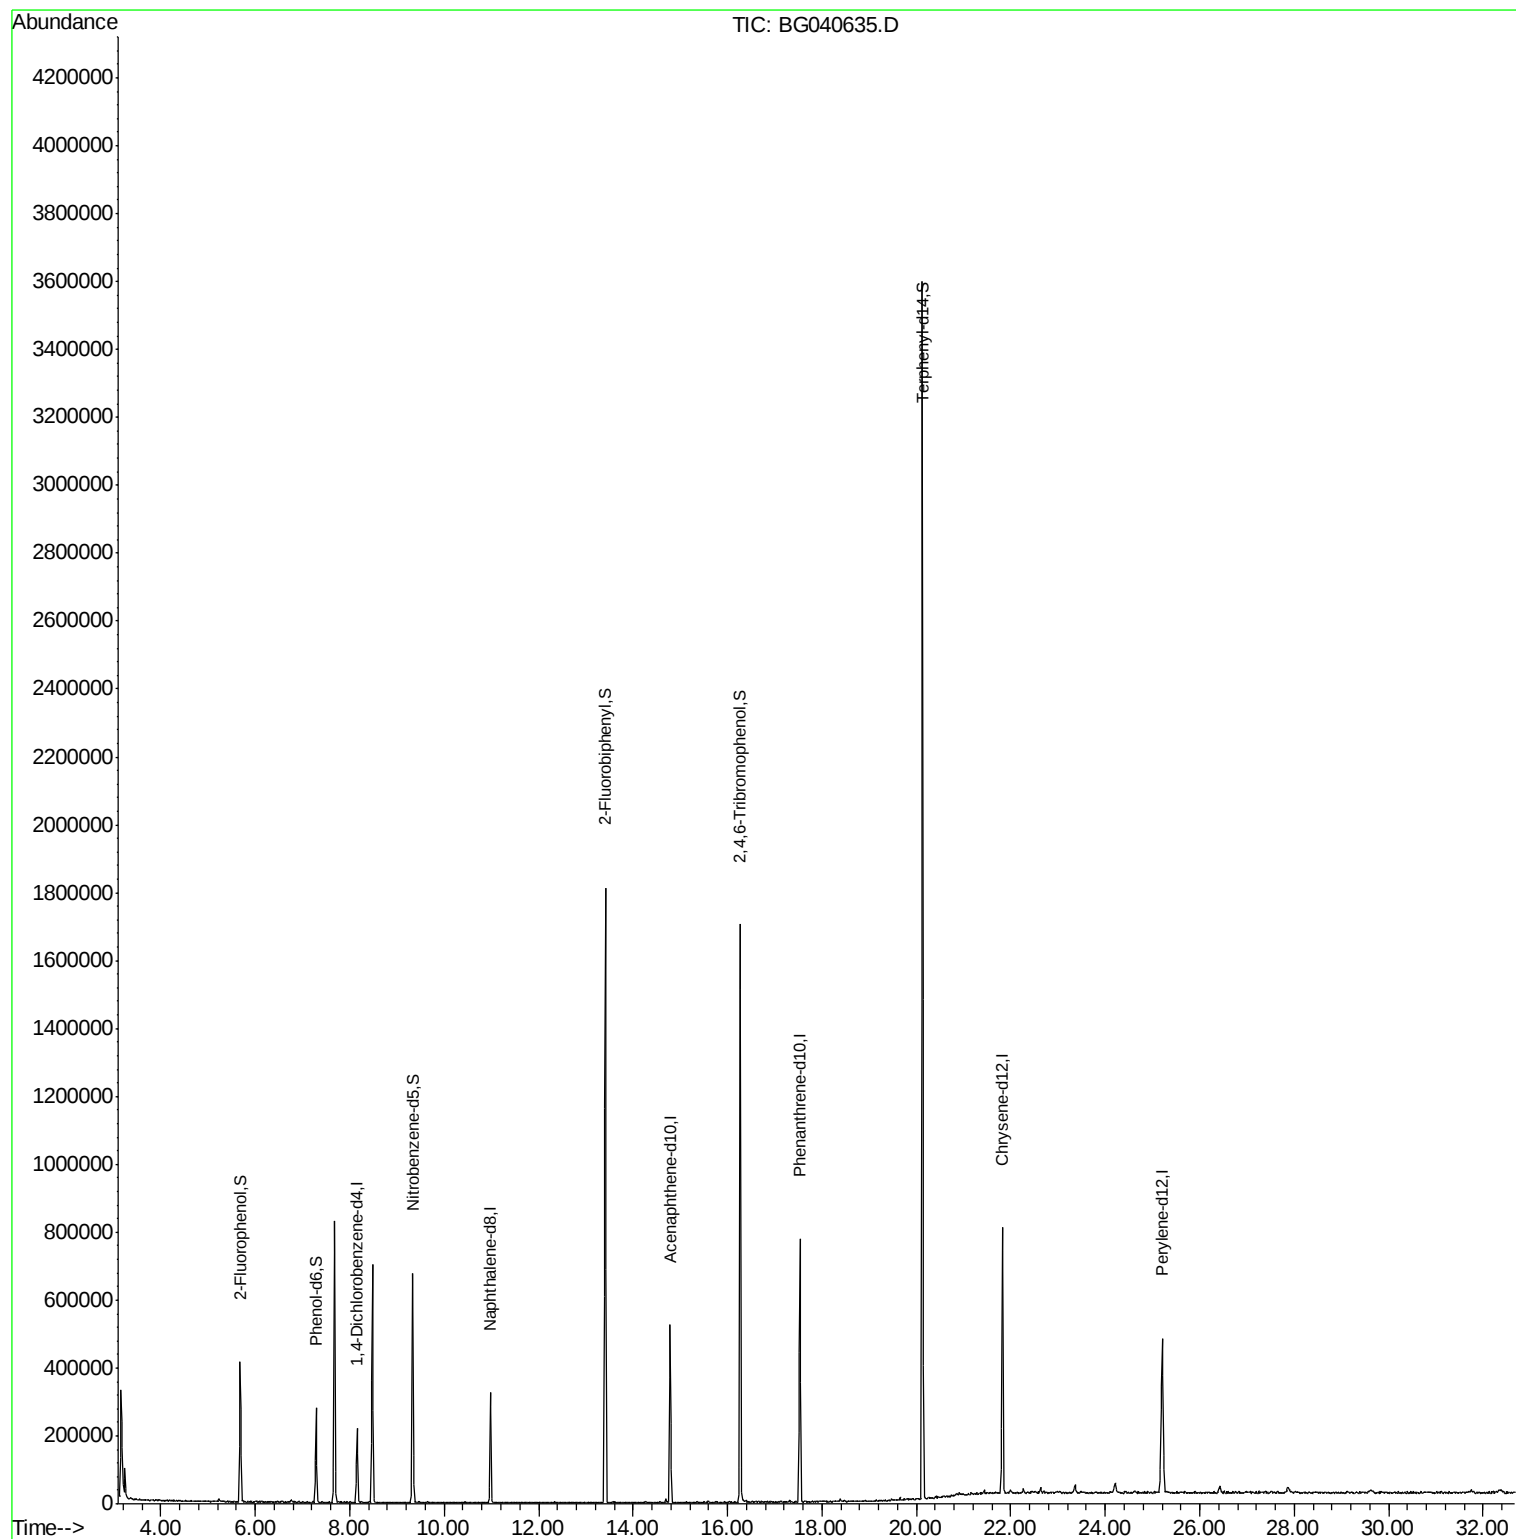

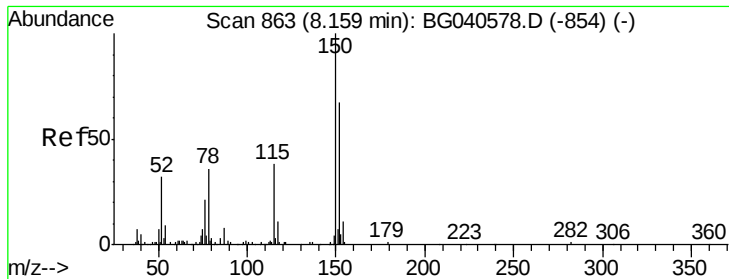


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.16 min Scan# 863
Delta R.T. 0.00 min
Lab File: BG040635.D
Acq: 26 Apr 2019 18:44

Instrument :
BNA_G
ClientSampleId :
S37-0014

Tgt Ion:152 Resp: 55018
Ion Ratio Lower Upper
152 100
150 137.5 120.2 180.2
115 55.9 46.2 69.2

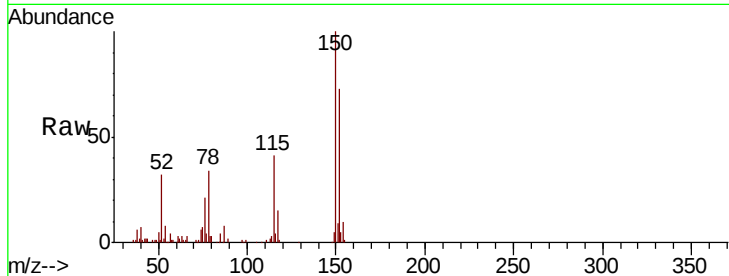


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

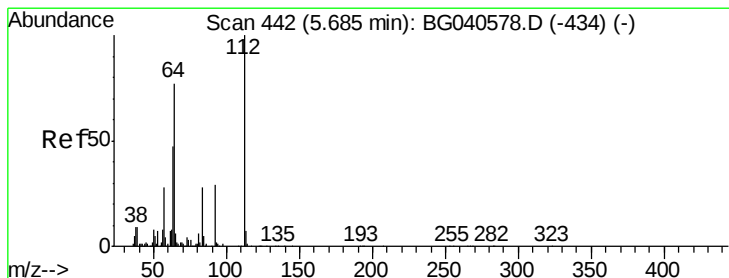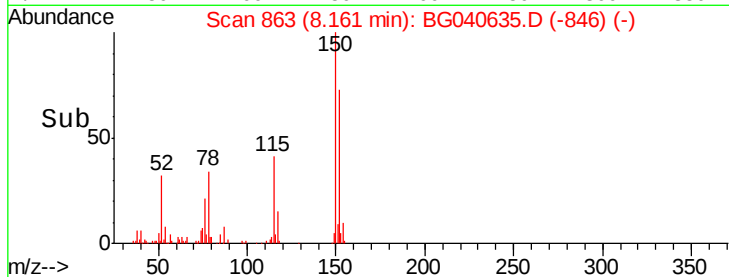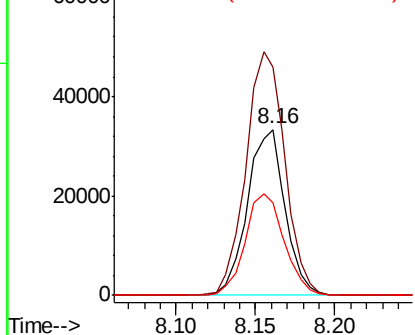



#5


2-Fluorophenol
Concen: 46.180 ng
RT: 5.69 min Scan# 442
Delta R.T. 0.00 min
Lab File: BG040635.D
Acq: 26 Apr 2019 18:44

Tgt Ion:112 Resp: 144134
Ion Ratio Lower Upper
112 100
64 75.7 61.4 92.0
63 43.0 37.8 56.6

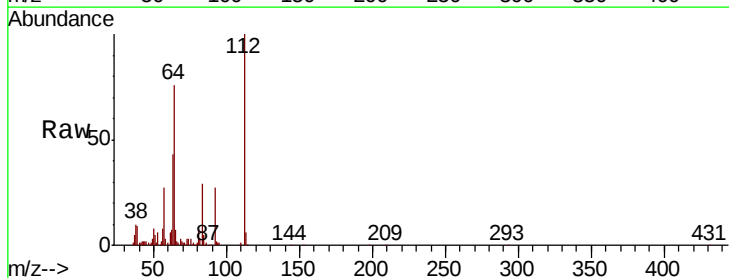

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

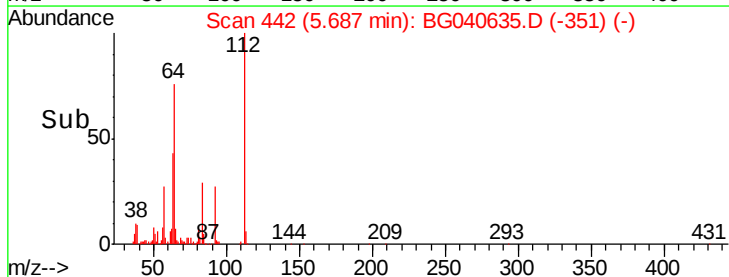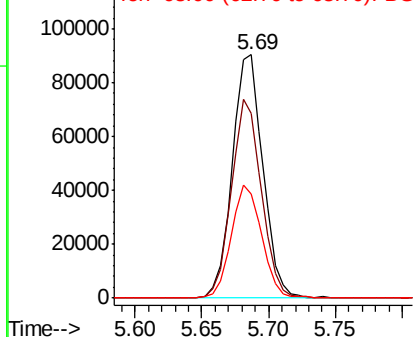

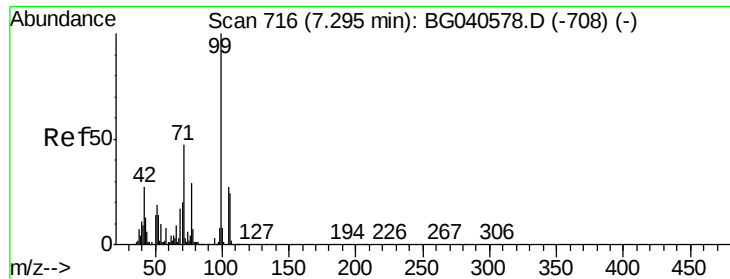

#7

Phenol-d6

Concen: 28.262 ng

RT: 7.29 min Scan# 714

Delta R.T. -0.01 min

Lab File: BG040635.D

Acq: 26 Apr 2019 18:44

Instrument :

BNA_G

ClientSampleId :

S37-0014


Tgt Ion: 99 Resp: 135819

Ion Ratio Lower Upper




99 100

42 28.3 21.8 32.8

71 49.1 38.6 57.8

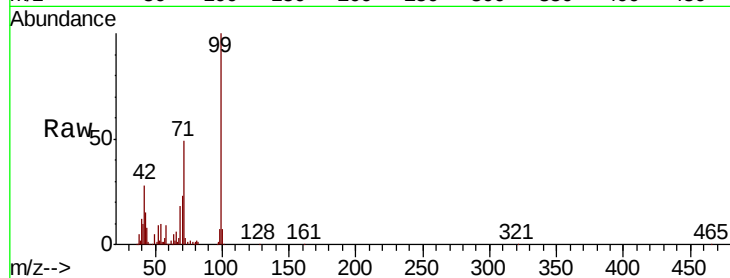

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

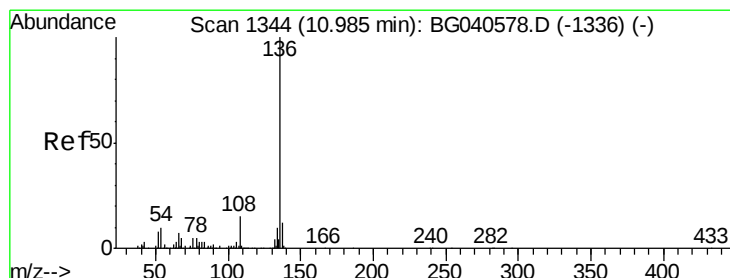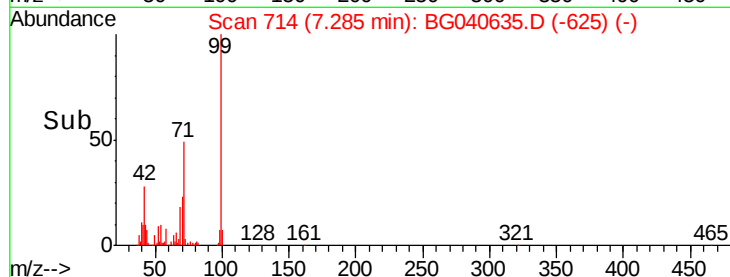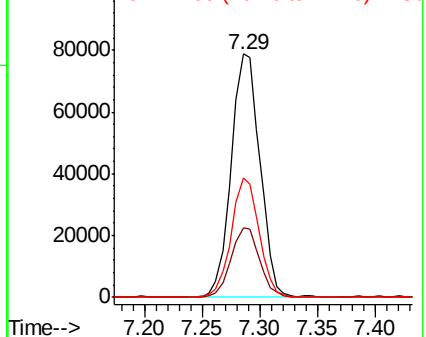

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.98 min Scan# 1343

Delta R.T. -0.00 min

Lab File: BG040635.D

Acq: 26 Apr 2019 18:44

Tgt Ion: 136 Resp: 237581


Ion Ratio Lower Upper

136 100



137 11.0 9.7 14.5


54 11.0 8.6 12.8

68 5.2 4.8 7.2

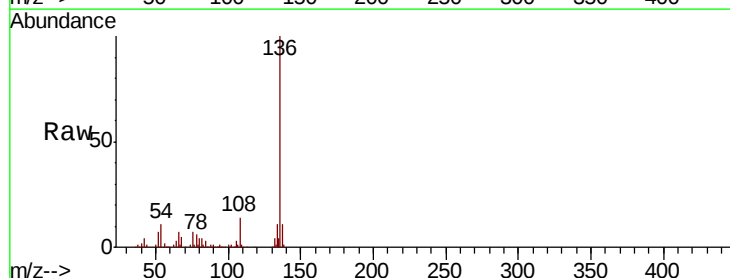

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

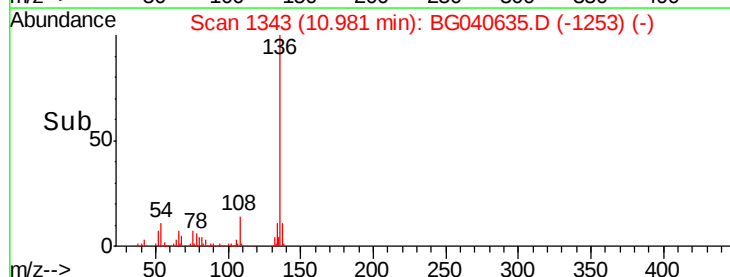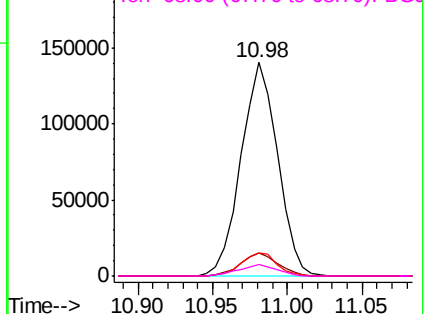


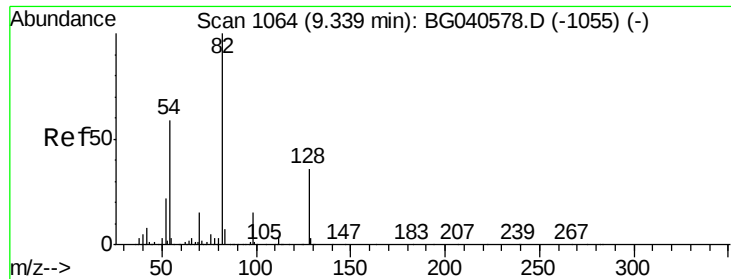




#23
Nitrobenzene-d5
Concen: 76.520 ng
RT: 9.34 min Scan# 1063
Delta R.T. -0.00 min
Lab File: BG040635.D
Acq: 26 Apr 2019 18:44

Instrument :
BNA_G
ClientSampleId :
S37-0014

Tgt Ion	Ratio	Lower	Upper
82	100		
128	33.2	28.9	43.3
54	59.4	47.2	70.8

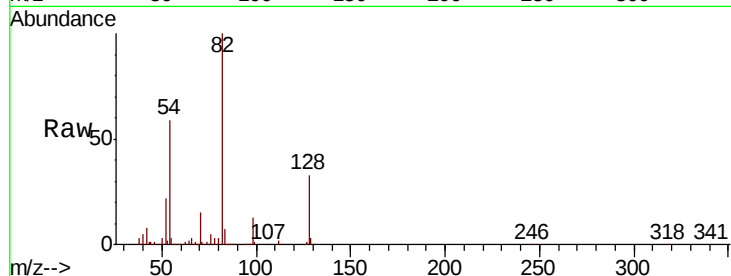


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

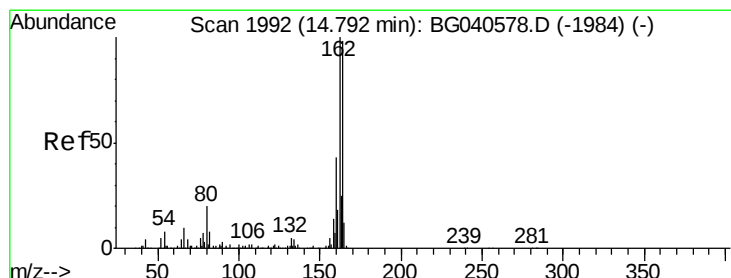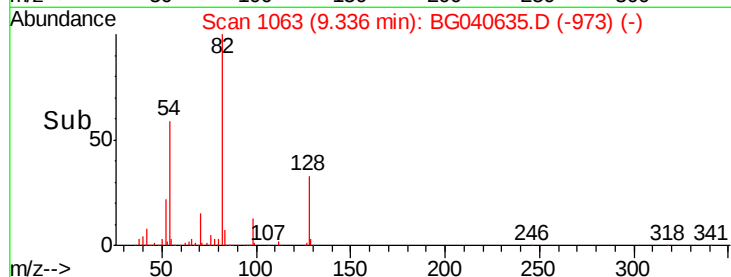
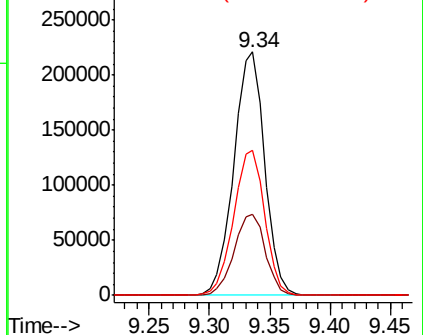


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.78 min Scan# 1990
Delta R.T. -0.01 min
Lab File: BG040635.D
Acq: 26 Apr 2019 18:44

Tgt Ion	Ratio	Lower	Upper
164	100		
162	102.6	81.9	122.9
160	43.7	35.4	53.2

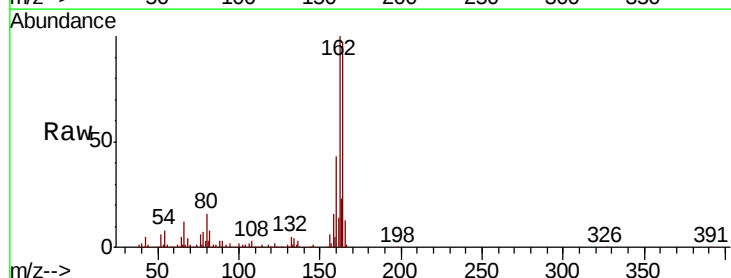

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC



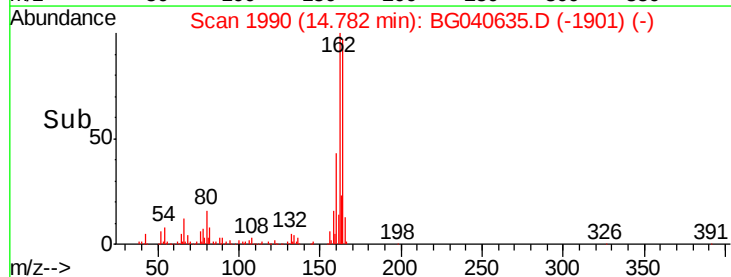
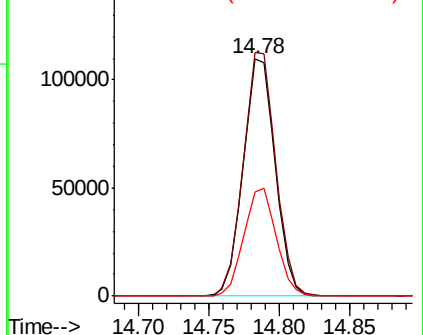




#42
 2,4,6-Tribromophenol
 Concen: 115.412 ng
 RT: 16.27 min Scan# 2244
 Delta R.T. 0.00 min
 Lab File: BG040635.D
 Acq: 26 Apr 2019 18:44




Instrument :
 BNA_G
 ClientSampleId :
 S37-0014


Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.5	75.9	113.9
141	41.0	32.4	48.6

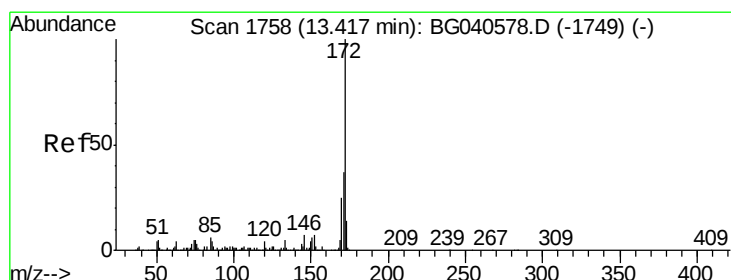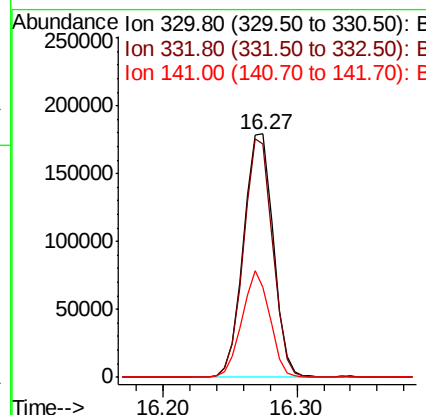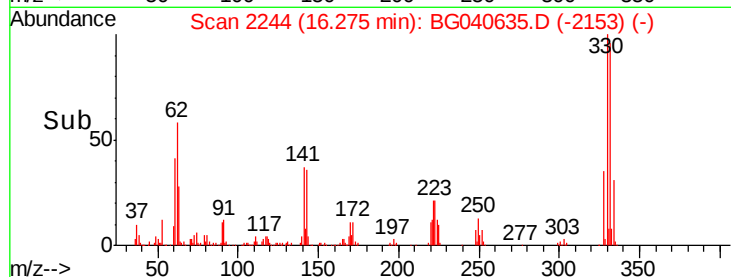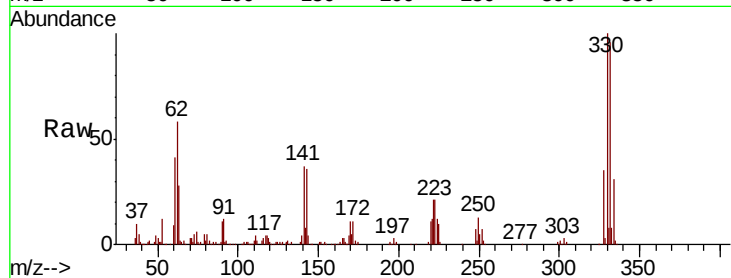

#45
 2-Fluorobiphenyl
 Concen: 71.044 ng
 RT: 13.41 min Scan# 1757
 Delta R.T. -0.00 min
 Lab File: BG040635.D
 Acq: 26 Apr 2019 18:44

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.5	29.4	44.2
170	25.6	19.9	29.9

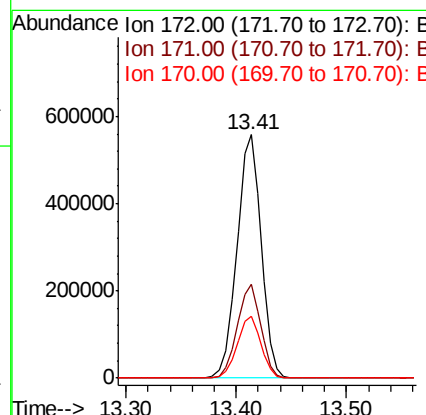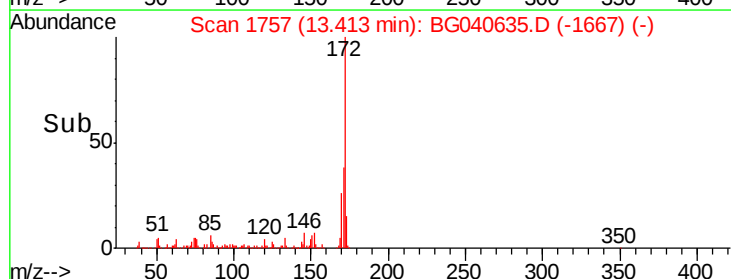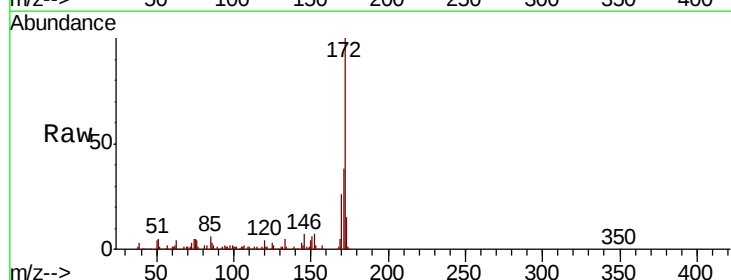

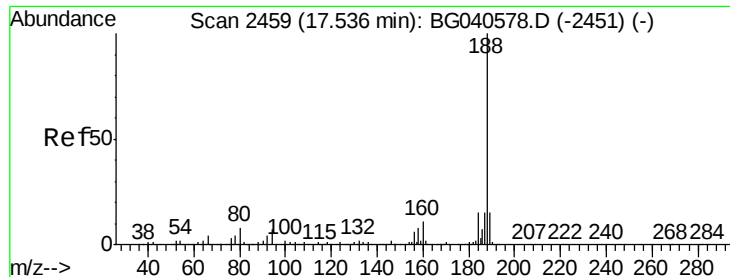

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.53 min Scan# 2458

Delta R.T. -0.00 min

Lab File: BG040635.D

Acq: 26 Apr 2019 18:44

Instrument :

BNA_G

ClientSampleId :

S37-0014


Tgt Ion:188 Resp: 454250

Ion Ratio Lower Upper

188 100

94 6.8 5.6 8.4




80 8.1 6.4 9.6

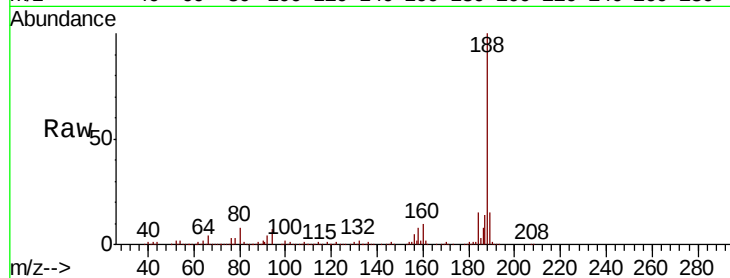

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

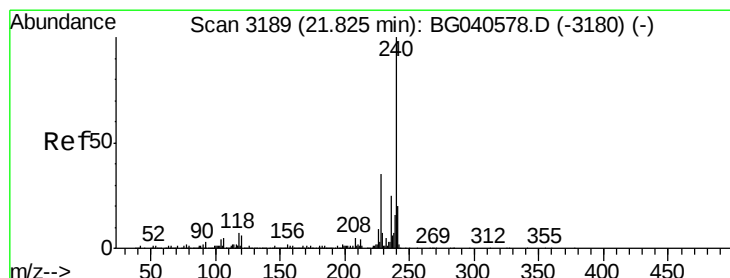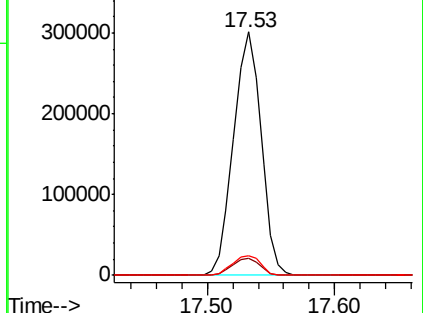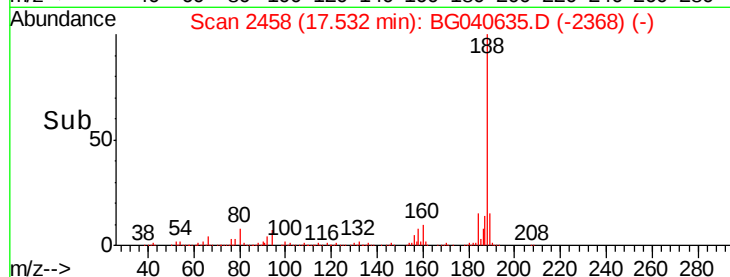

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.82 min Scan# 3188

Delta R.T. -0.00 min

Lab File: BG040635.D

Acq: 26 Apr 2019 18:44


Tgt Ion:240 Resp: 456928

Ion Ratio Lower Upper

240 100

120 6.2 5.0 7.6



236 25.6 20.3 30.5

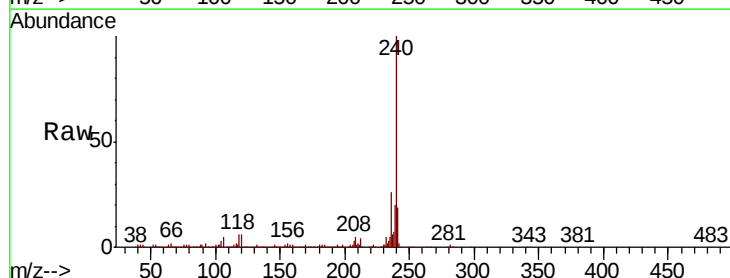


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

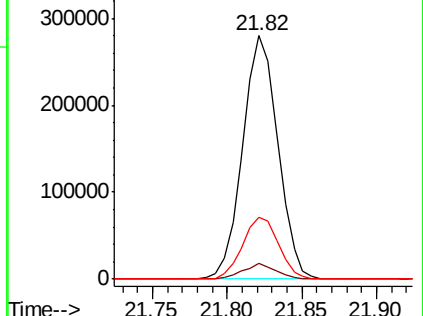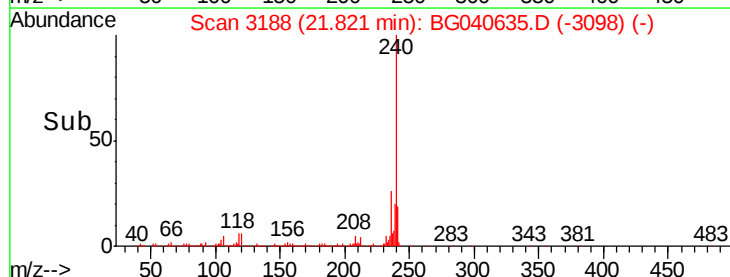

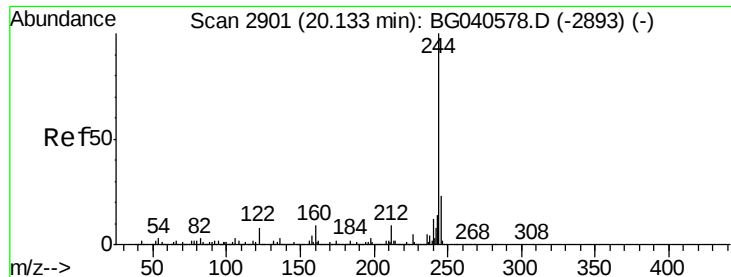

#79

Terphenyl-d14

Concen: 77.102 ng

RT: 20.13 min Scan# 2900

Delta R.T. -0.00 min

Lab File: BG040635.D

Acq: 26 Apr 2019 18:44

Instrument :

BNA_G

ClientSampleId :

S37-0014


Tgt Ion:244 Resp: 1590215

Ion Ratio Lower Upper

244 100

212 9.4 7.2 10.8




122 7.8 6.6 10.0

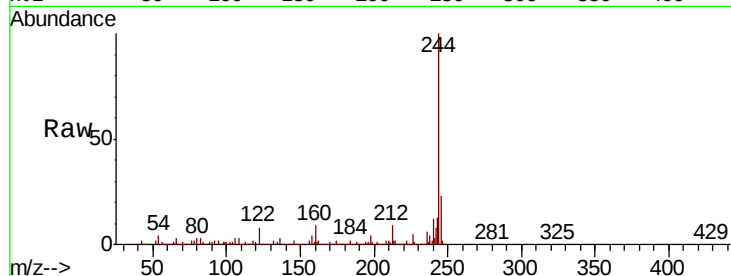

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

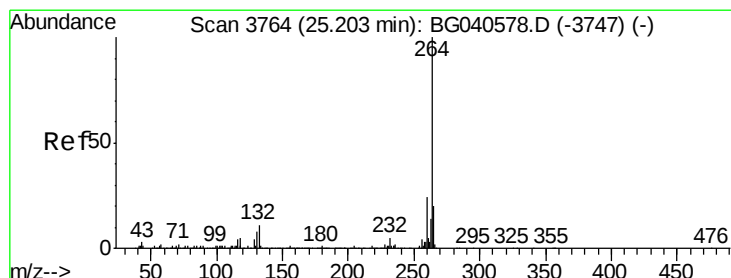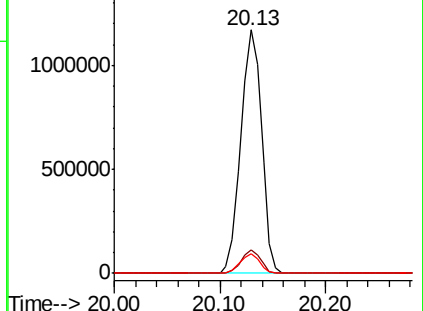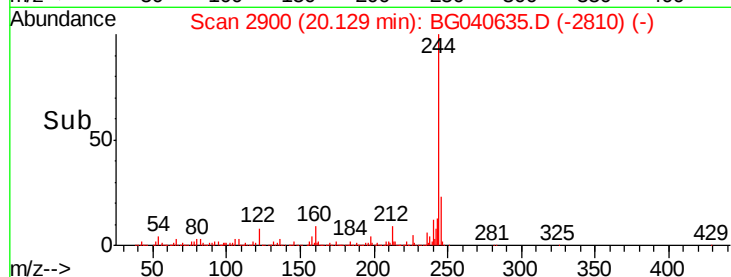

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.21 min Scan# 3764

Delta R.T. 0.00 min

Lab File: BG040635.D

Acq: 26 Apr 2019 18:44


Tgt Ion:264 Resp: 482949

Ion Ratio Lower Upper

264 100

260 23.6 19.2 28.8

265 20.7 16.6 25.0

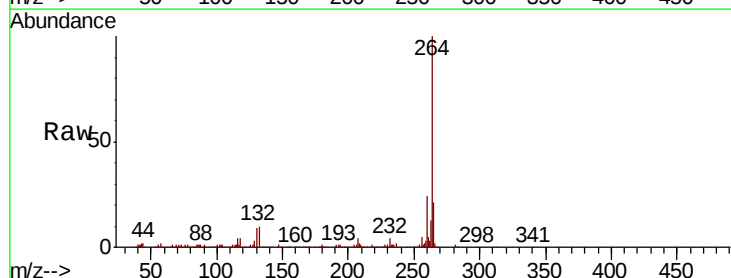

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

