

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042619\
 Data File : BG040650.D
 Acq On : 27 Apr 2019 5:26
 Operator : JU/SJ
 Sample : K2553-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 RBR200034

Quant Time: Apr 29 02:29:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 24 05:35:33 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.15	152	47843	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	193003	20.00	ng	0.00
39) Acenaphthene-d10	14.79	164	142255	20.00	ng	0.00
64) Phenanthrene-d10	17.53	188	390321	20.00	ng	0.00
76) Chrysene-d12	21.81	240	399215	20.00	ng	-0.01
87) Perylene-d12	25.19	264	409785	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.69	112	342536	126.21	ng	0.00
7) Phenol-d6	7.29	99	449773	107.63	ng	0.00
23) Nitrobenzene-d5	9.33	82	440742	105.52	ng	0.00
42) 2,4,6-Tribromophenol	16.27	330	306139	156.57	ng	0.00
45) 2-Fluorobiphenyl	13.41	172	895824	90.95	ng	0.00
79) Terphenyl-d14	20.13	244	1866381	103.57	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042619\
Data File : BG040650.D
Acq On : 27 Apr 2019 5:26
Operator : JU/SJ
Sample : K2553-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
RBR200034

Quant Time: Apr 29 02:29:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 24 05:35:33 2019
Response via : Initial Calibration

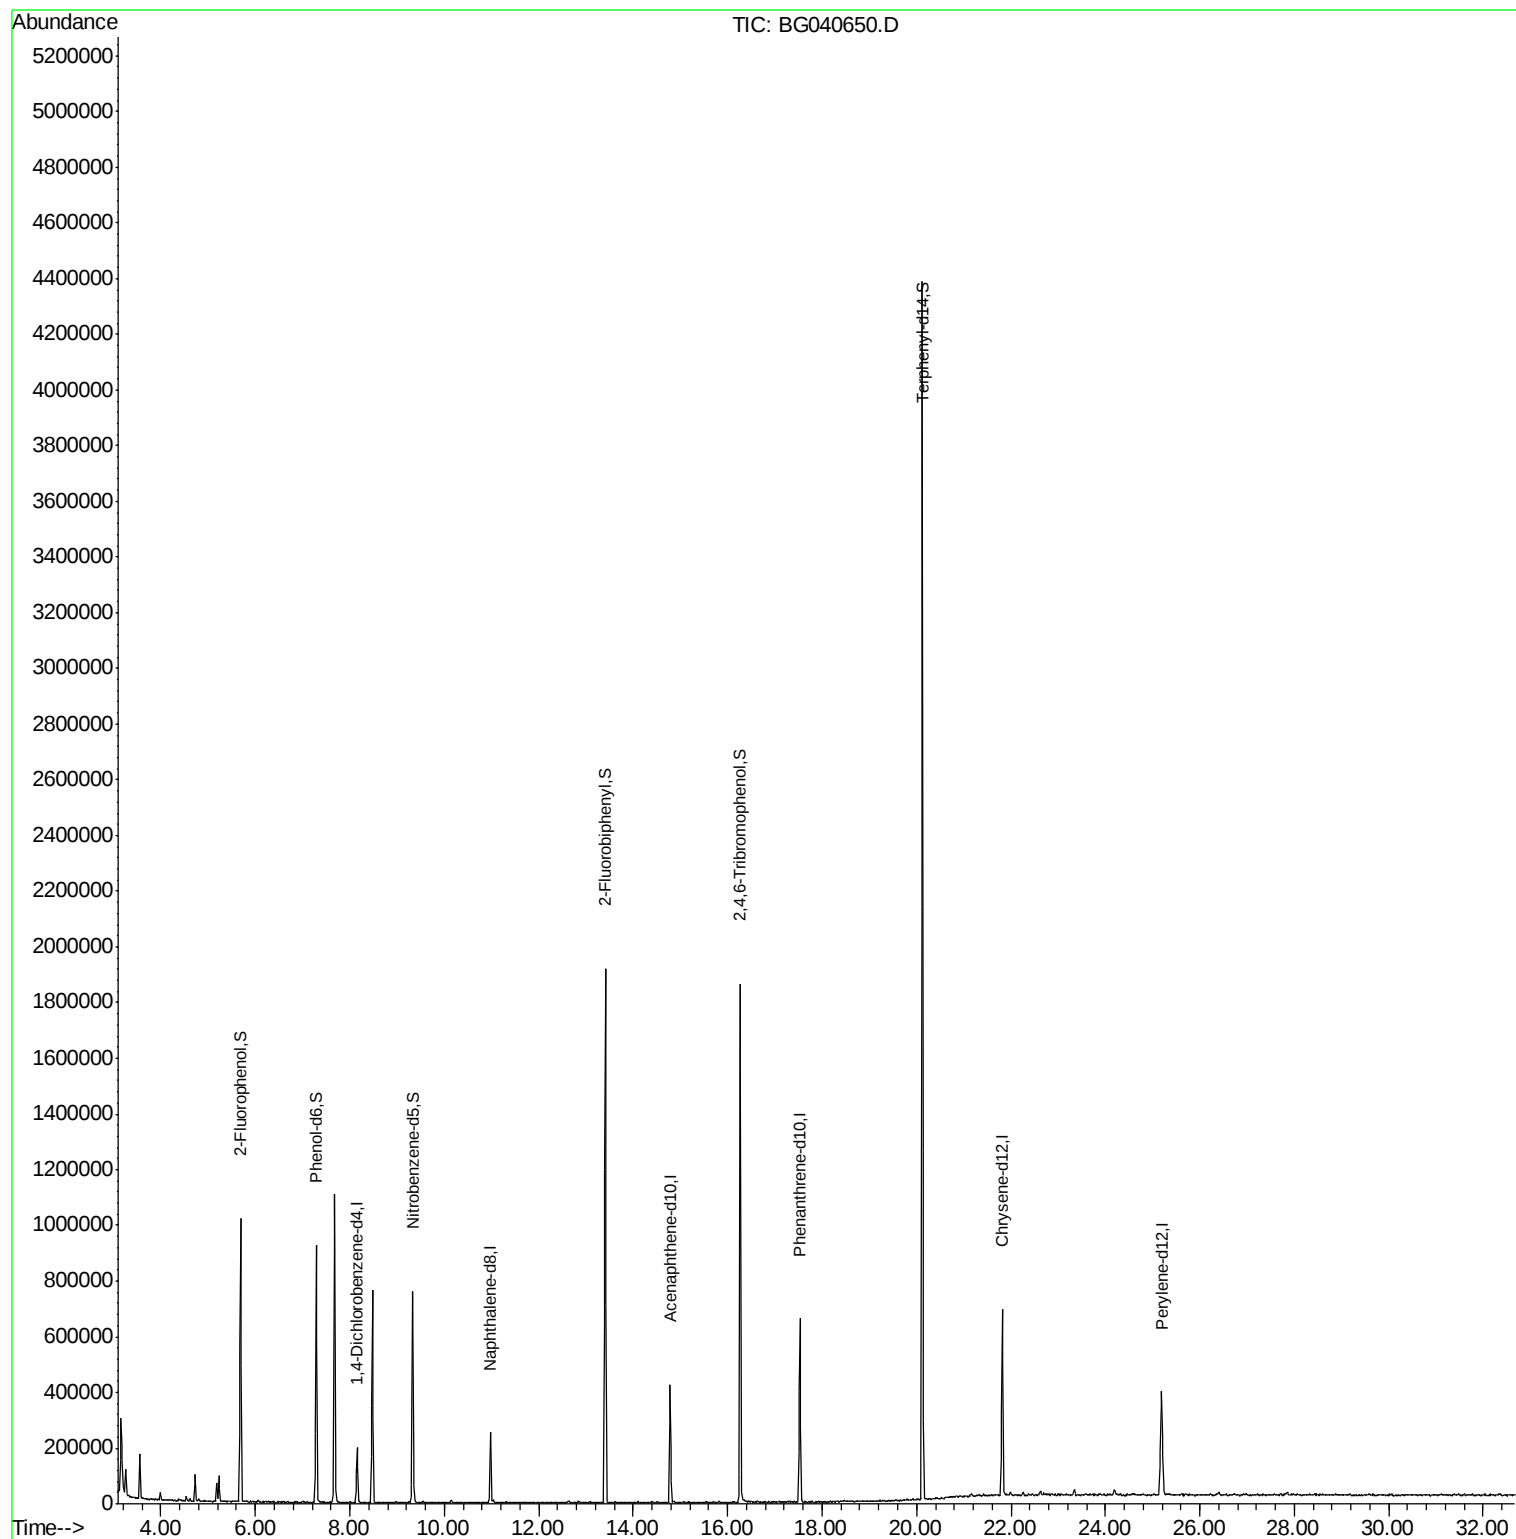

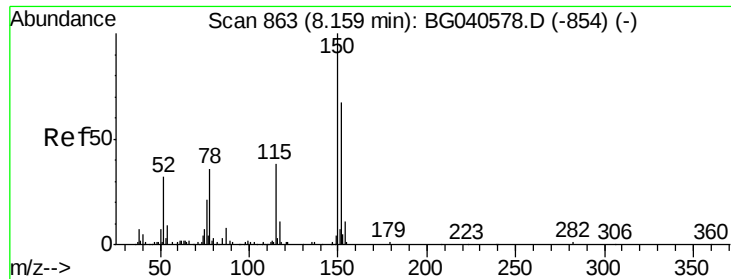


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.15 min Scan# 862
 Delta R.T. -0.01 min
 Lab File: BG040650.D
 Acq: 27 Apr 2019 5:26

Instrument :
 BNA_G
 ClientSampleId :
 RBR200034

Tgt Ion:152 Resp: 47843
 Ion Ratio Lower Upper
 152 100
 150 148.6 120.2 180.2
 115 63.8 46.2 69.2

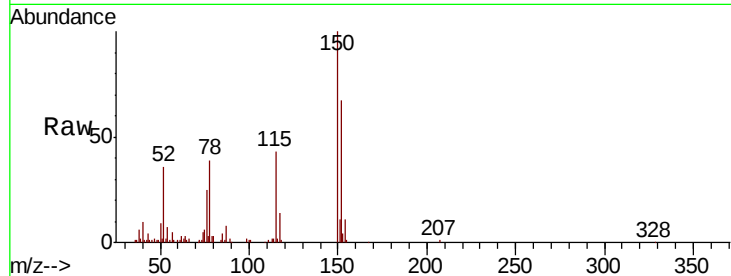


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

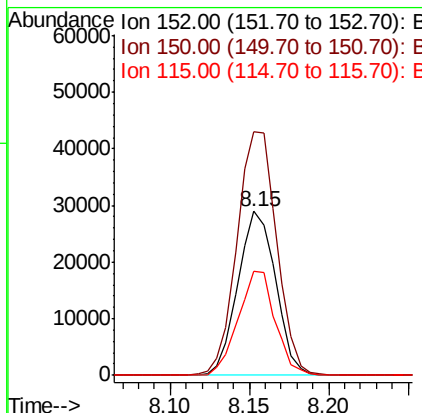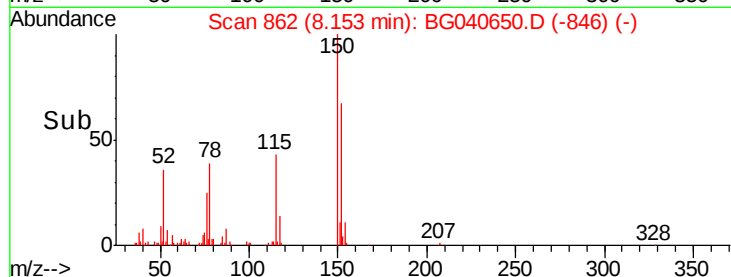



#5

2-Fluorophenol
 Concen: 126.207 ng
 RT: 5.69 min Scan# 442
 Delta R.T. 0.00 min
 Lab File: BG040650.D
 Acq: 27 Apr 2019 5:26

Tgt Ion:112 Resp: 342536
 Ion Ratio Lower Upper
 112 100
 64 79.0 61.4 92.0
 63 47.2 37.8 56.6



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

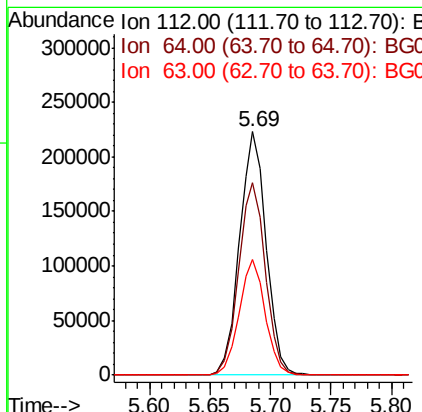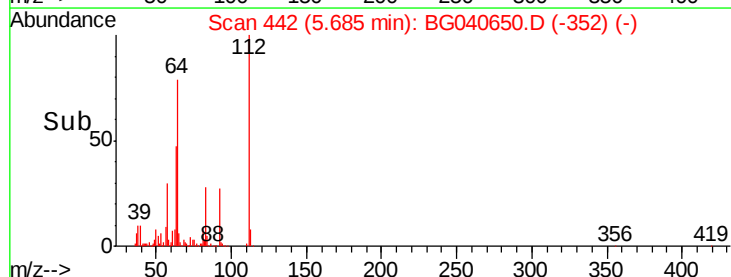



#7

Phenol-d6

Concen: 107.629 ng

RT: 7.29 min Scan# 715

Delta R.T. -0.01 min

Lab File: BG040650.D

Acq: 27 Apr 2019 5:26

Instrument :

BNA_G

ClientSampleId :

RBR200034


Tgt Ion: 99 Resp: 449773

Ion Ratio Lower Upper




99 100

42 26.6 21.8 32.8

71 47.5 38.6 57.8

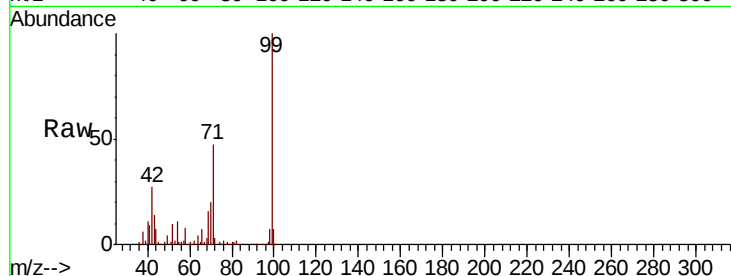

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

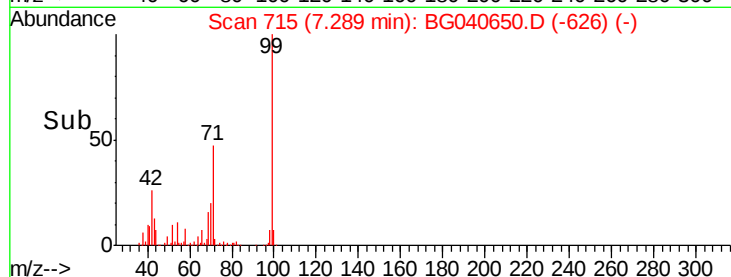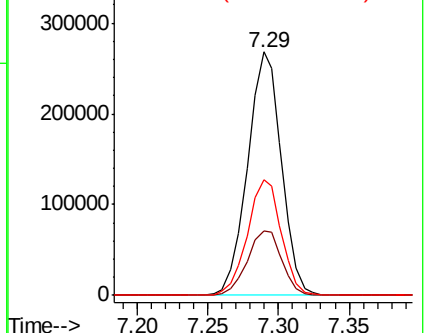

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.98 min Scan# 1344

Delta R.T. 0.00 min

Lab File: BG040650.D

Acq: 27 Apr 2019 5:26

Tgt Ion: 136 Resp: 193003


Ion Ratio Lower Upper

136 100



137 12.2 9.7 14.5


54 10.3 8.6 12.8

68 5.7 4.8 7.2



Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



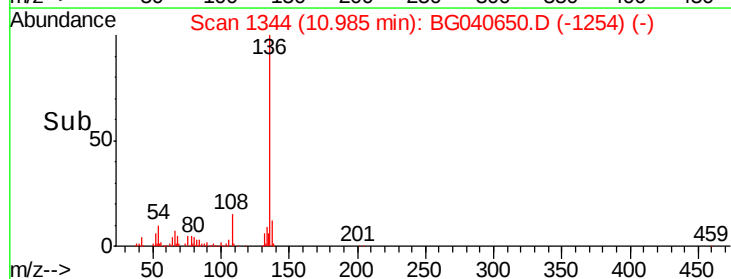
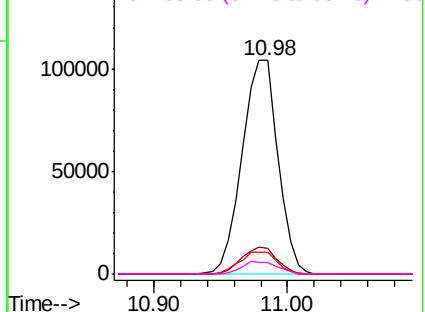


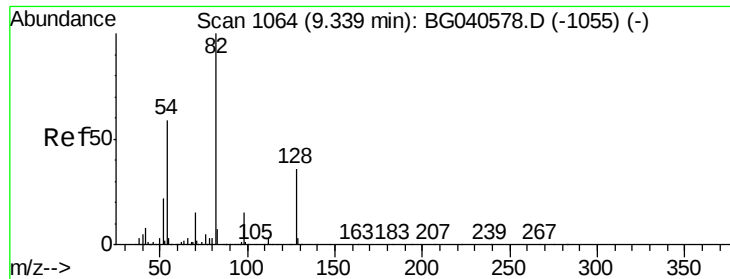

#23
 Nitrobenzene-d5
 Concen: 105.517 ng
 RT: 9.33 min Scan# 1063
 Delta R.T. -0.01 min
 Lab File: BG040650.D
 Acq: 27 Apr 2019 5:26




Instrument :
 BNA_G
 ClientSampleId :
 RBR200034


Tgt Ion	Ratio	Lower	Upper
82	100		
128	34.1	28.9	43.3
54	60.2	47.2	70.8

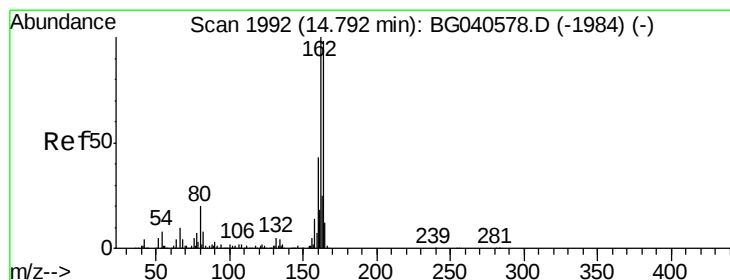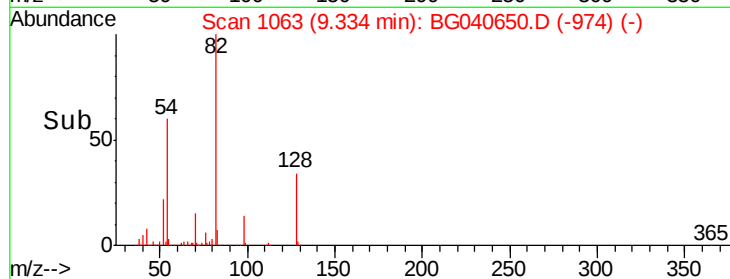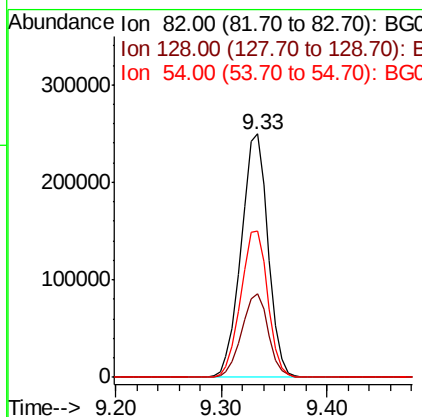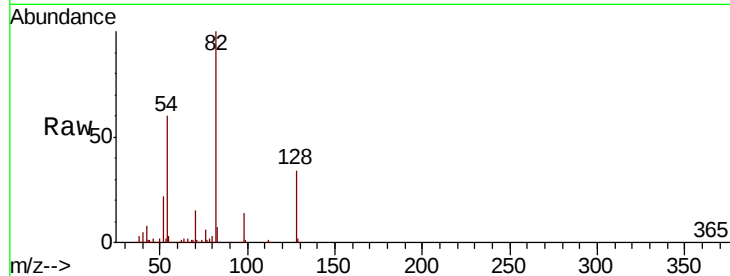

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.79 min Scan# 1991
 Delta R.T. -0.01 min
 Lab File: BG040650.D
 Acq: 27 Apr 2019 5:26

Tgt Ion	Ratio	Lower	Upper
164	100		
162	99.8	81.9	122.9
160	44.9	35.4	53.2

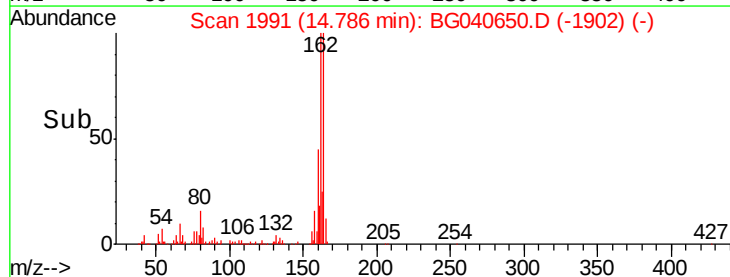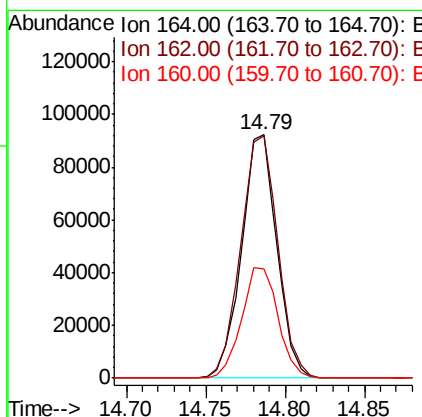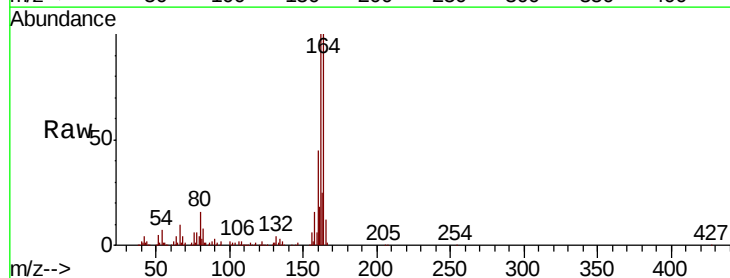


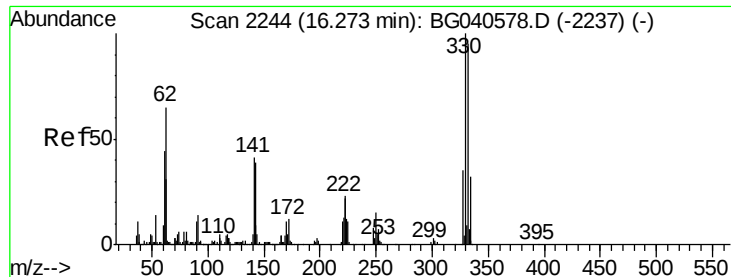

#42
 2,4,6-Tribromophenol
 Concen: 156.567 ng
 RT: 16.27 min Scan# 2243
 Delta R.T. -0.01 min
 Lab File: BG040650.D
 Acq: 27 Apr 2019 5:26

Instrument :
 BNA_G
 ClientSampled :
 RBR200034

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.6	75.9	113.9
141	40.3	32.4	48.6



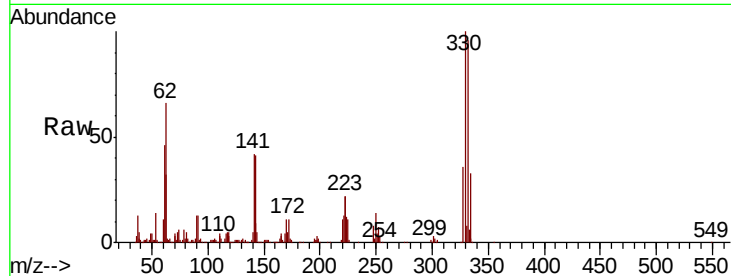


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

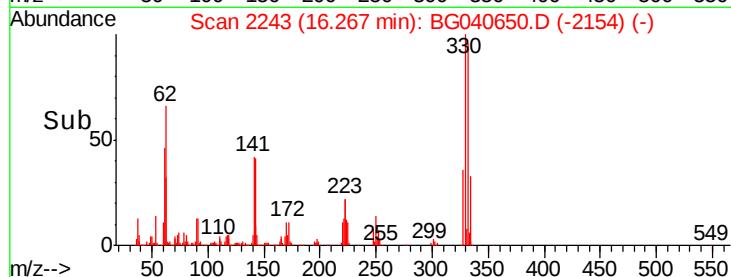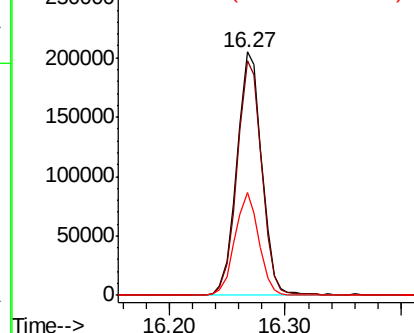

#45
 2-Fluorobiphenyl
 Concen: 90.946 ng
 RT: 13.41 min Scan# 1757
 Delta R.T. -0.01 min
 Lab File: BG040650.D
 Acq: 27 Apr 2019 5:26

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.7	29.4	44.2
170	26.3	19.9	29.9






Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

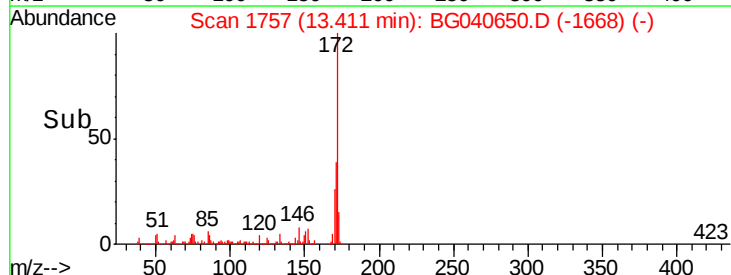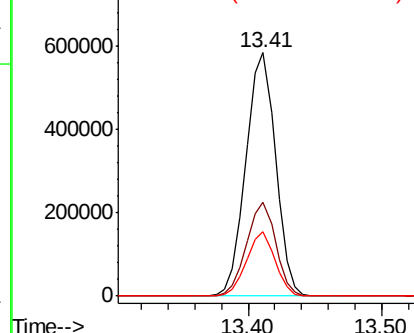

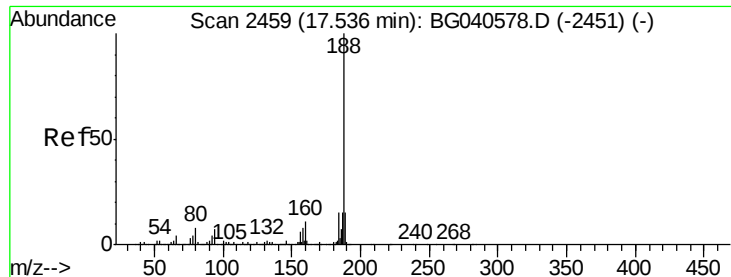

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.53 min Scan# 2458

Delta R.T. -0.01 min

Lab File: BG040650.D

Acq: 27 Apr 2019 5:26

Instrument :

BNA_G

ClientSampleId :

RBR200034


Tgt Ion:188 Resp: 390321

Ion Ratio Lower Upper

188 100

94 6.7 5.6 8.4




80 8.7 6.4 9.6

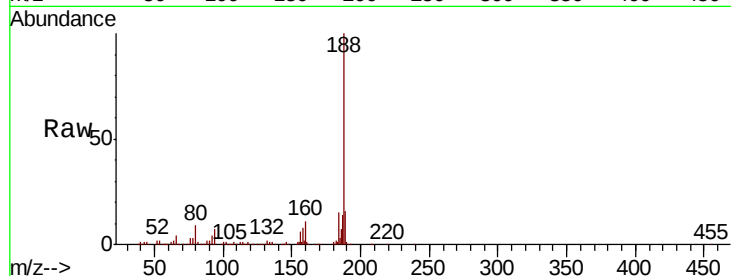

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG040650.D (-3099) (-)

Ion 80.00 (79.70 to 80.70): BG040650.D (-3099) (-)

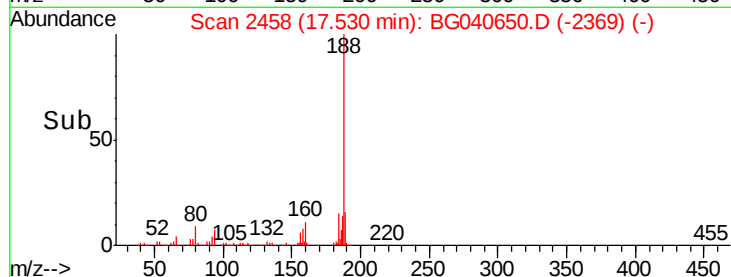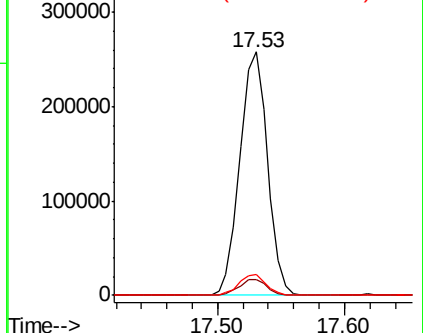

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.81 min Scan# 3187

Delta R.T. -0.01 min

Lab File: BG040650.D

Acq: 27 Apr 2019 5:26


Tgt Ion:240 Resp: 399215

Ion Ratio Lower Upper

240 100

120 5.8 5.0 7.6



236 25.5 20.3 30.5




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

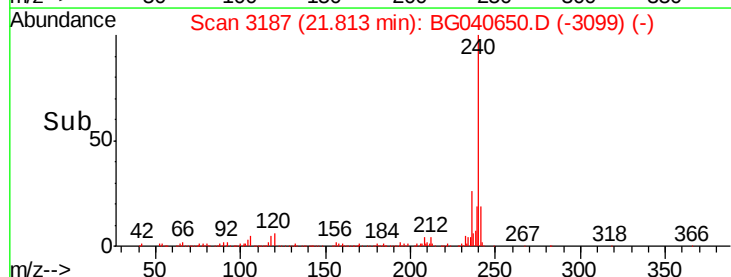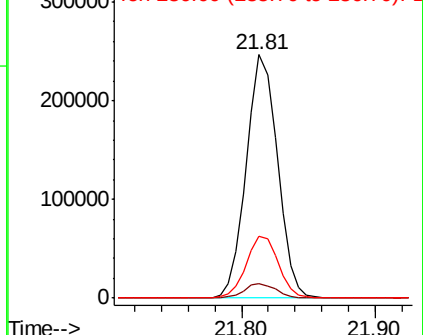


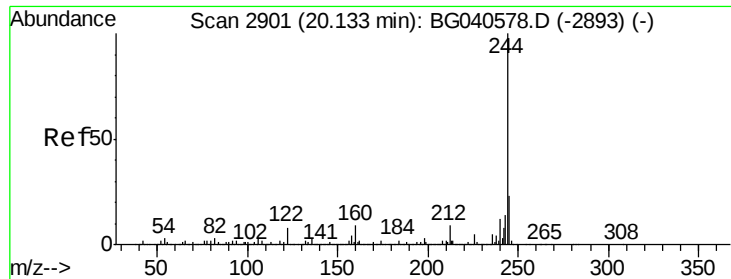




#79
 Terphenyl-d14
 Concen: 103.574 ng
 RT: 20.13 min Scan# 2900
 Delta R.T. -0.01 min
 Lab File: BG040650.D
 Acq: 27 Apr 2019 5:26

Instrument :
 BNA_G
 ClientSampleId :
 RBR200034

Tgt Ion:244 Resp: 1866381
 Ion Ratio Lower Upper
 244 100
 212 9.8 7.2 10.8
 122 8.6 6.6 10.0




Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

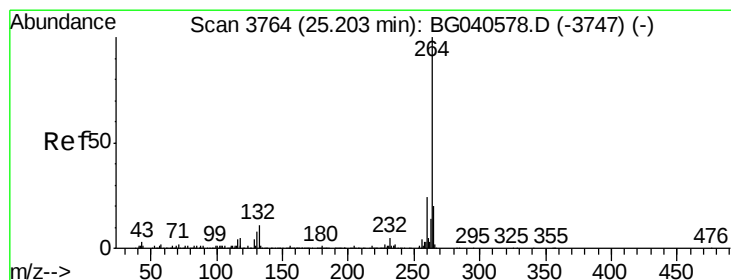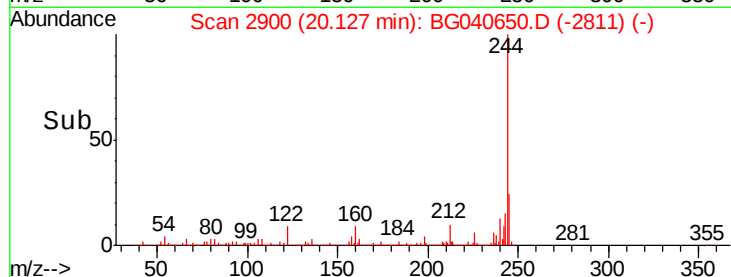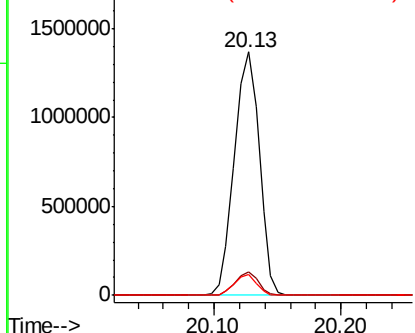

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 25.19 min Scan# 3762
 Delta R.T. -0.01 min
 Lab File: BG040650.D
 Acq: 27 Apr 2019 5:26

Tgt Ion:264 Resp: 409785
 Ion Ratio Lower Upper
 264 100
 260 24.5 19.2 28.8
 265 22.9 16.6 25.0



Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

