


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG042619\
 Data File : BG040621.D
 Acq On : 26 Apr 2019 9:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG042319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 24 05:35:33 2019

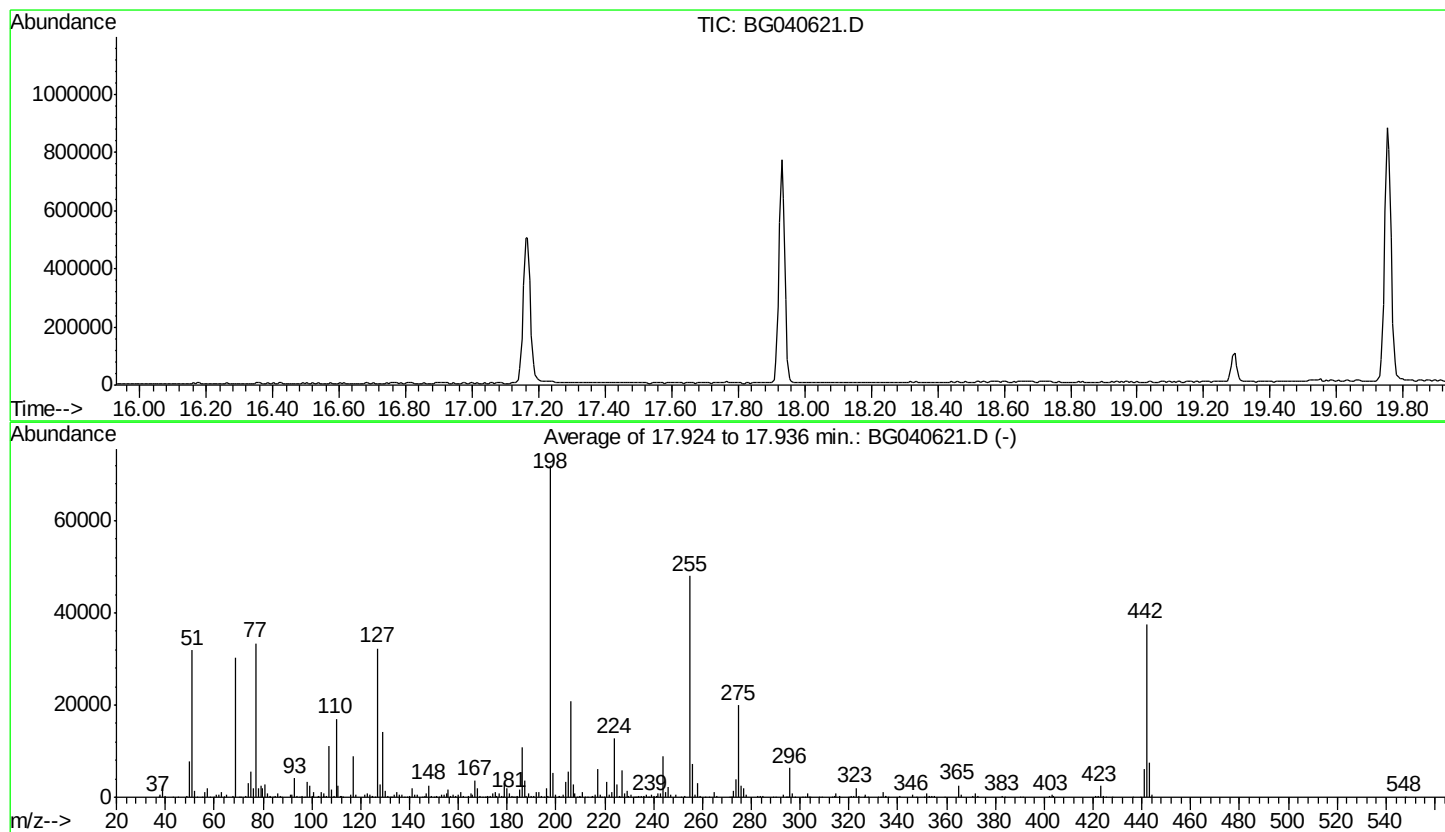

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	31864	PASS
68	69	0.00	2	0.7	225	PASS
69	198	0.00	100	42.0	30186	PASS
70	69	0.00	2	0.4	112	PASS
127	198	10	80	44.9	32336	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71954	PASS
199	198	5	9	7.5	5361	PASS
275	198	10	60	27.7	19914	PASS
365	198	1	100	3.5	2517	PASS
441	198	0.01	100	8.6	6189	PASS
442	198	50	100	52.3	37605	PASS
443	442	15	24	20.1	7549	PASS